

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG082419\
 Data File : FG005718.D
 Signal(s) : FID1A.ch
 Acq On : 24 Aug 2019 11:22
 Operator : DD\AJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Aug 26 01:58:33 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG080819.M
 Quant Title :
 QLast Update : Thu Aug 08 16:03:53 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.745	6168855	48.285 ug/ml
Target Compounds			
2) N-DECANE	4.447	7729966	54.315 ug/ml
3) N-DODECANE	6.476	7928822	54.123 ug/ml
4) N-TETRADECANE	8.278	7871946	53.104 ug/ml
5) N-HEXADECANE	9.884	7839106	52.191 ug/ml
6) N-OCTADECANE	11.330	7607777	50.995 ug/ml
7) N-EICOSANE	12.642	7463467	49.760 ug/ml
8) N-DOCOSANE	13.844	7187867	48.705 ug/ml
10) N-TETRACOSANE	14.951	6992745	48.115 ug/ml
11) N-HEXACOSANE	15.973	6798477	47.366 ug/ml
12) N-OCTACOSANE	16.923	6682385	44.204 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG082419\
Data File : FG005718.D
Signal(s) : FID1A.ch
Acq On : 24 Aug 2019 11:22
Operator : DD\AJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 3 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Aug 26 01:58:33 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG080819.M
Quant Title :
QLast Update : Thu Aug 08 16:03:53 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

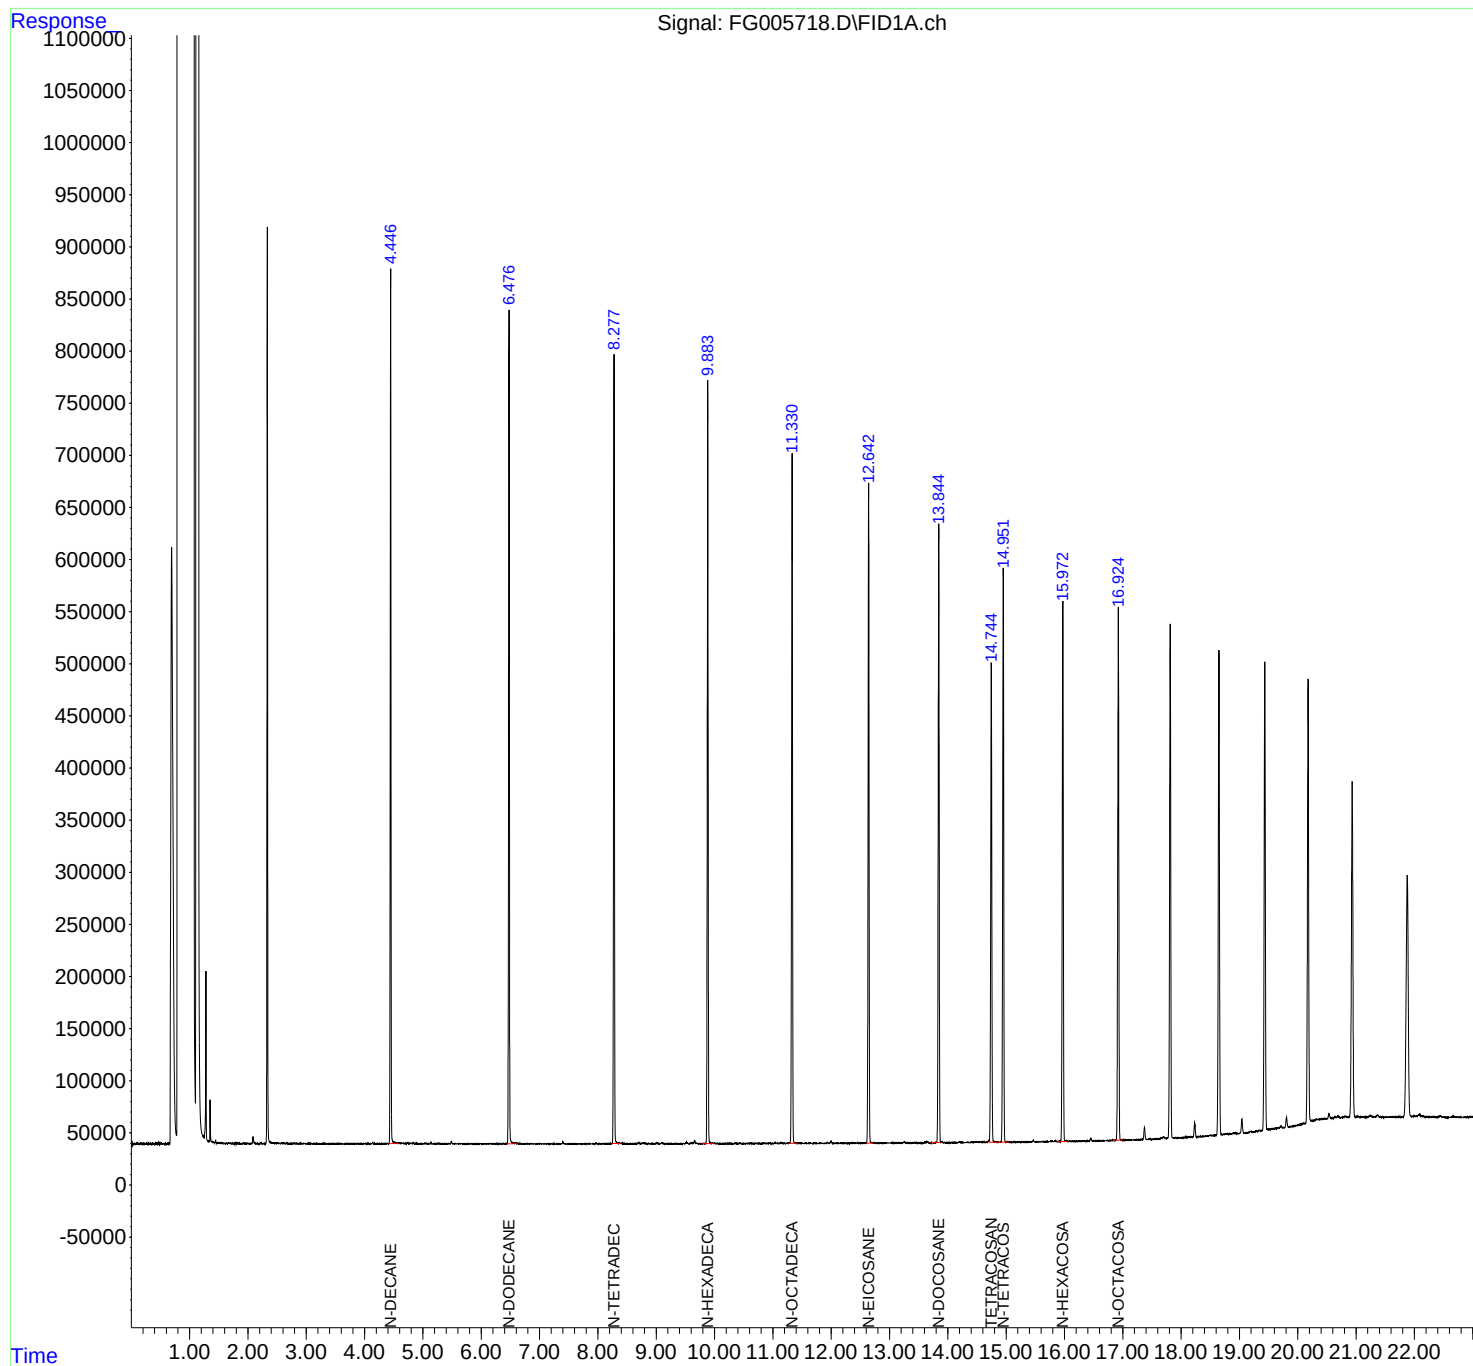

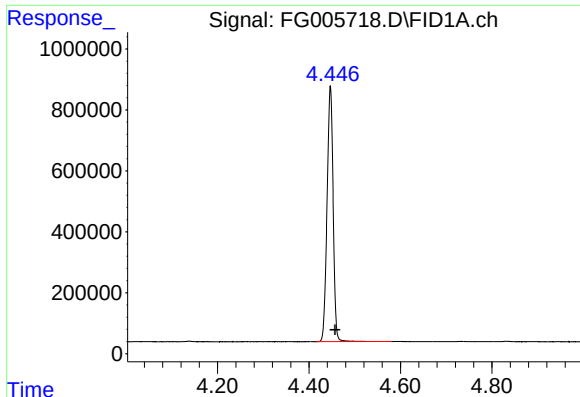


#2 N-DECANE

R.T.: 4.447 min
Delta R.T.: -0.010 min
Response: 7729966
Conc: 54.31 ug/ml

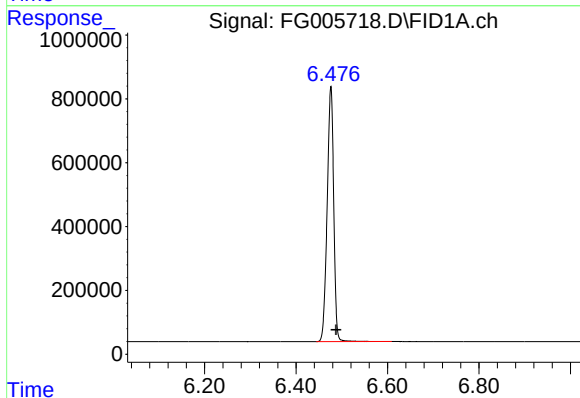


#3 N-DODECANE

R.T.: 6.476 min
Delta R.T.: -0.011 min
Response: 7928822
Conc: 54.12 ug/ml

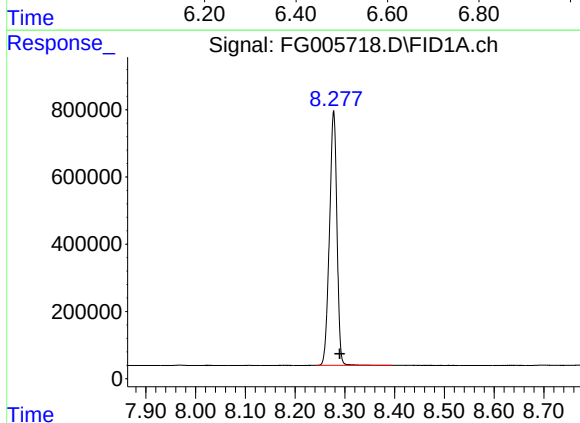


#4 N-TETRADECANE

R.T.: 8.278 min
Delta R.T.: -0.012 min
Response: 7871946
Conc: 53.10 ug/ml

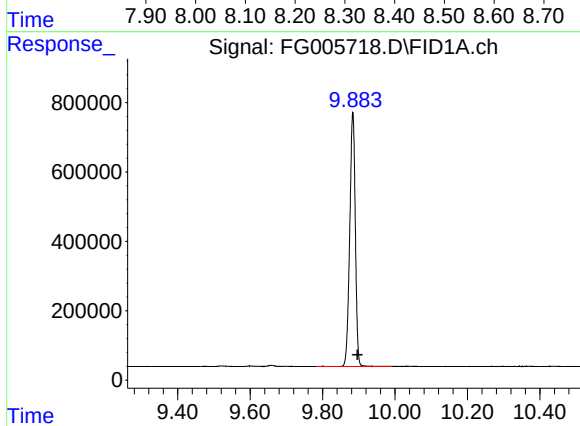


#5 N-HEXADECANE

R.T.: 9.884 min
Delta R.T.: -0.013 min
Response: 7839106
Conc: 52.19 ug/ml

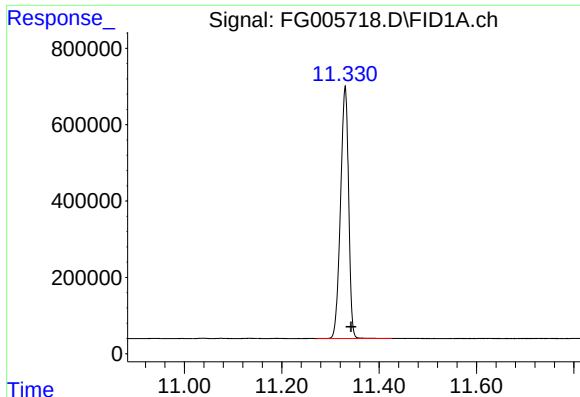


#6 N-OCTADECANE

R.T.: 11.330 min
Delta R.T.: -0.012 min
Response: 7607777
Conc: 50.99 ug/ml

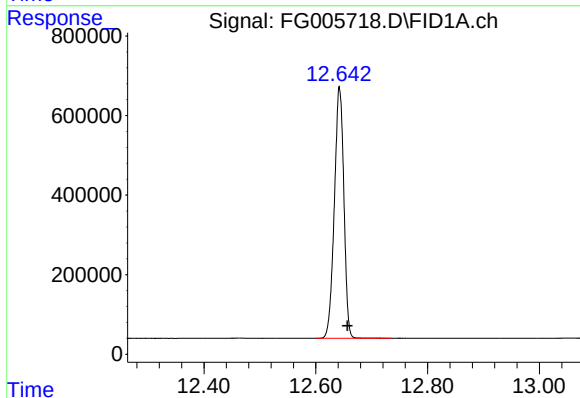


#7 N-EICOSANE

R.T.: 12.642 min
Delta R.T.: -0.014 min
Response: 7463467
Conc: 49.76 ug/ml

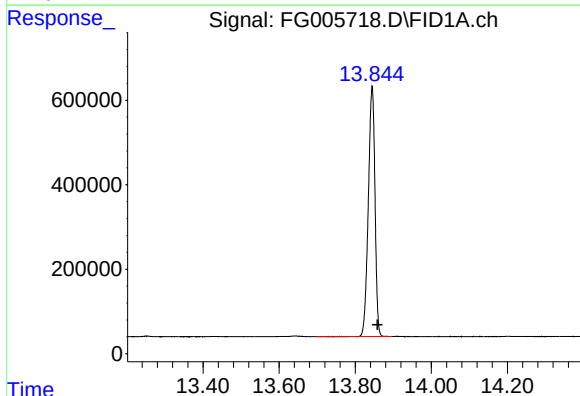


#8 N-DOCOSANE

R.T.: 13.844 min
Delta R.T.: -0.014 min
Response: 7187867
Conc: 48.71 ug/ml

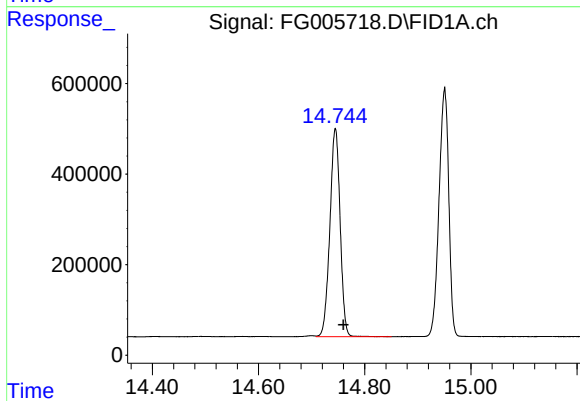


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.745 min
Delta R.T.: -0.015 min
Response: 6168855
Conc: 48.28 ug/ml

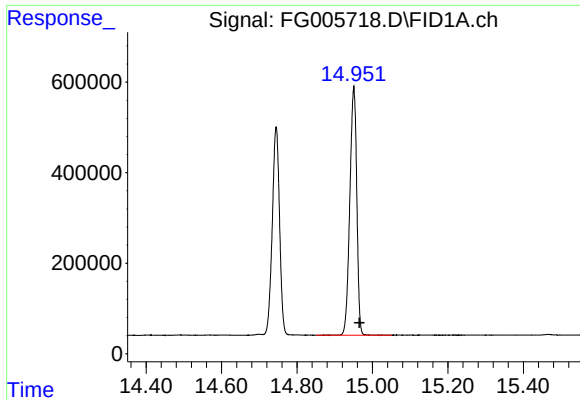


#10 N-TETRACOSANE

R.T.: 14.951 min
Delta R.T.: -0.014 min
Response: 6992745
Conc: 48.11 ug/ml

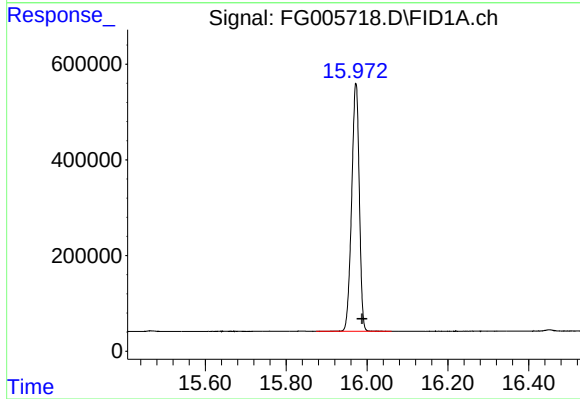

#11 N-HEXACOSANE

R.T.: 15.973 min
Delta R.T.: -0.016 min
Response: 6798477
Conc: 47.37 ug/ml

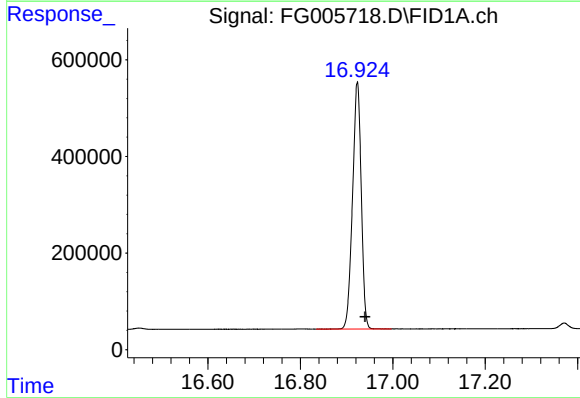

#12 N-OCTACOSANE

R.T.: 16.923 min
Delta R.T.: -0.017 min
Response: 6682385
Conc: 44.20 ug/ml