

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG082522\
 Data File : FG010420.D
 Signal(s) : FID1A.ch
 Acq On : 25 Aug 2022 14:10
 Operator : YP\AJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 25 18:46:23 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG072822.M
 Quant Title :
 QLast Update : Thu Jul 28 15:10:44 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds			
3) N-DODECANE	6.497	3241997	23.586 ug/ml
12) N-OCTACOSANE	16.964	2923907	21.176 ug/ml
13) N-TRIACONTANE	17.849	168130	1.241 ug/ml
14) N-DOTRIACONTANE	18.682	239661	1.824 ug/ml
15) N-TETRATRIACONTANE	19.466	226497	1.810 ug/ml
16) N-HEXATRIACONTANE	20.207	161180	1.398 ug/ml
17) N-OCTATRIACONTANE	20.919	173078	1.523 ug/ml
18) N-TETRACONTANE	21.755	73671	0.628 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG082522\
Data File : FG010420.D
Signal(s) : FID1A.ch
Acq On : 25 Aug 2022 14:10
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 25 18:46:23 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG072822.M
Quant Title :
QLast Update : Thu Jul 28 15:10:44 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

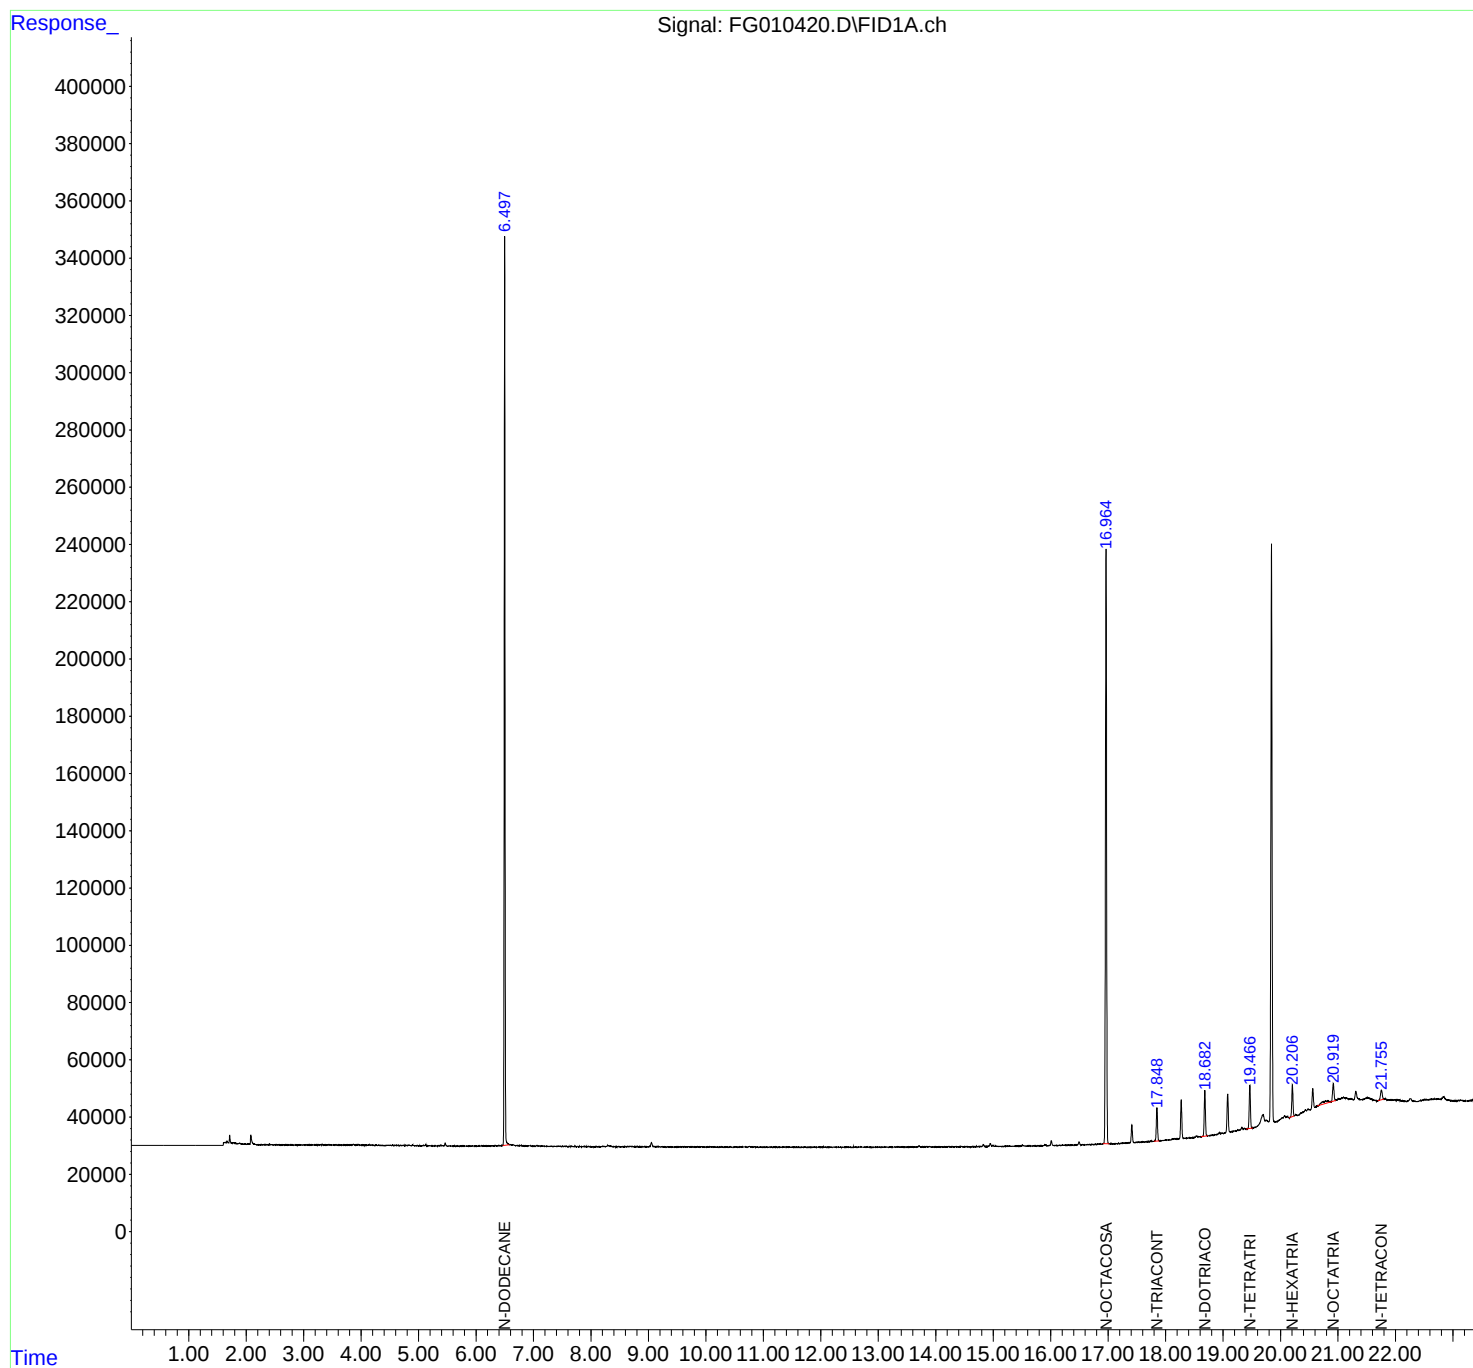


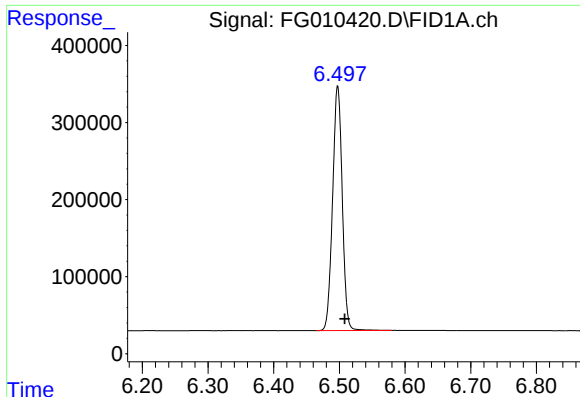

#3 N-DODECANE


R.T.: 6.497 min
Delta R.T.: -0.011 min
Response: 3241997
Conc: 23.59 ug/ml

Instrument :
FID_G
ClientSampleId :

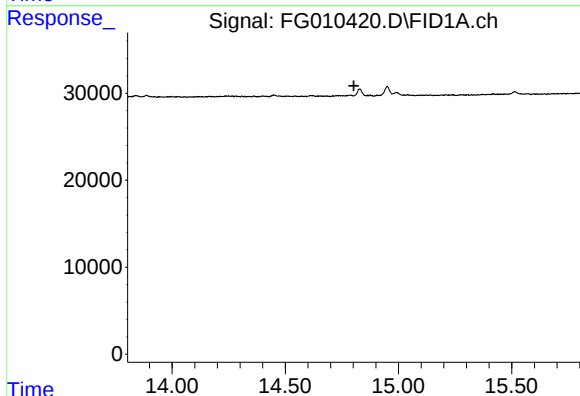


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.803 min
Response: 0
Conc: N.D.

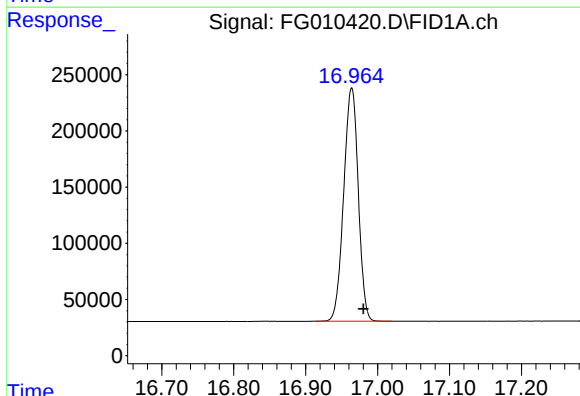


#12 N-OCTACOSANE

R.T.: 16.964 min
Delta R.T.: -0.016 min
Response: 2923907
Conc: 21.18 ug/ml

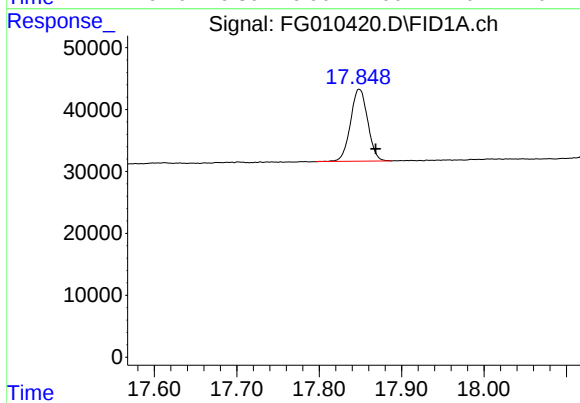

#13 N-TRIACONTANE


R.T.: 17.849 min
Delta R.T.: -0.020 min
Response: 168130
Conc: 1.24 ug/ml

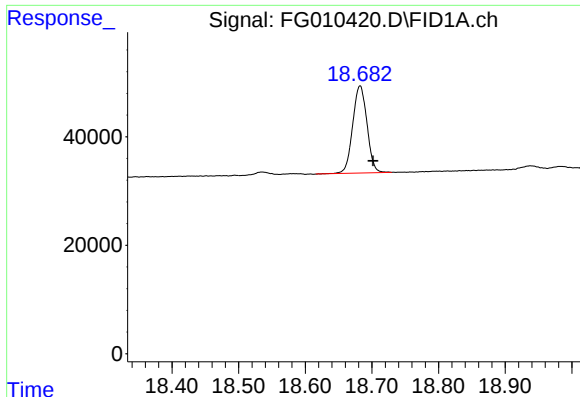

#14 N-DOTRIACONTANE


R.T.: 18.682 min
Delta R.T.: -0.019 min
Response: 239661
Conc: 1.82 ug/ml

Instrument :
FID_G
ClientSampleId :

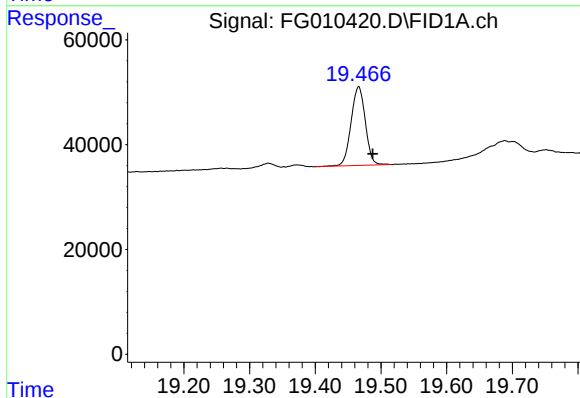


#15 N-TETRATRIACONTANE

R.T.: 19.466 min
Delta R.T.: -0.021 min
Response: 226497
Conc: 1.81 ug/ml

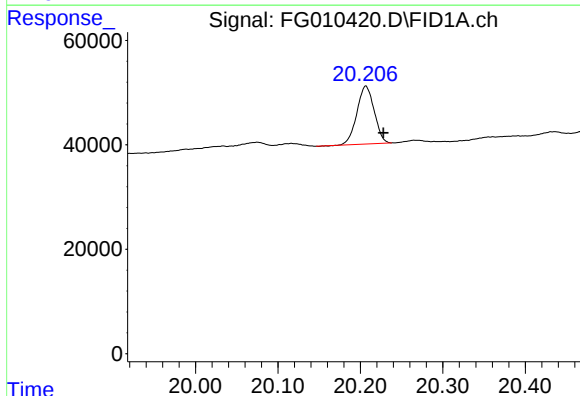


#16 N-HEXATRIACONTANE

R.T.: 20.207 min
Delta R.T.: -0.021 min
Response: 161180
Conc: 1.40 ug/ml

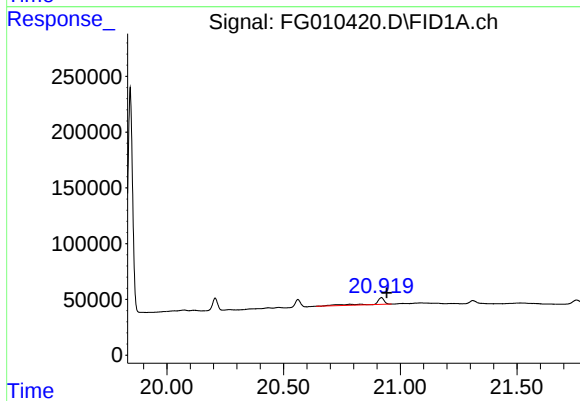

#17 N-OCTATRIACONTANE

R.T.: 20.919 min
Delta R.T.: -0.023 min
Response: 173078
Conc: 1.52 ug/ml

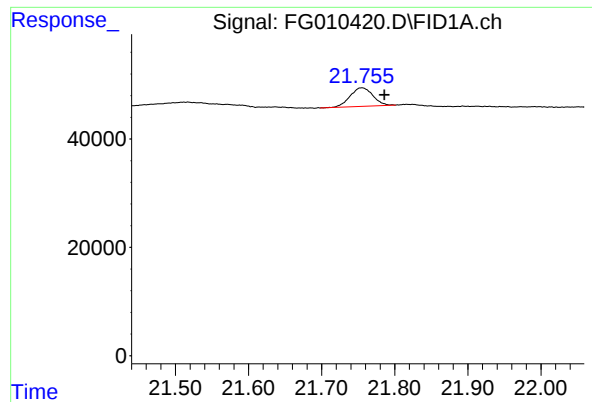

#18 N-TETRACONTANE

R.T.: 21.755 min
Delta R.T.: -0.031 min
Response: 73671
Conc: 0.63 ug/ml

Instrument :

FID_G

ClientSampleId :