

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_G\Data\FG082725\  
Data File : FG016407.D  
Signal(s) : FID1A.ch  
Acq On : 27 Aug 2025 08:12  
Operator : YP\AJ  
Sample : MECL2  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
FID\_G  
ClientSampleId :  
MECL2

Integration File: autoint1.e  
Quant Time: Aug 28 04:18:21 2025  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_G\Method\FG080525.M  
Quant Title :  
QLast Update : Tue Aug 05 12:47:26 2025  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

| Compound                    | R.T.   | Response | Conc Units  |
|-----------------------------|--------|----------|-------------|
| -----                       |        |          |             |
| System Monitoring Compounds |        |          |             |
| Target Compounds            |        |          |             |
| 13) N-TRIACONTANE           | 18.276 | 24904    | 0.229 ug/ml |
| 14) N-DOTRIACONTANE         | 19.114 | 47471    | 0.451 ug/ml |
| 15) N-TETRATRIACONTANE      | 19.902 | 50624    | 0.531 ug/ml |
| 16) N-HEXATRIACONTANE       | 20.649 | 32526    | 0.435 ug/ml |
| -----                       |        |          |             |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_G\Data\FG082725\  
Data File : FG016407.D  
Signal(s) : FID1A.ch  
Acq On : 27 Aug 2025 08:12  
Operator : YP\AJ  
Sample : MECL2  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
FID\_G  
ClientSampleId :  
MECL2

Integration File: autoint1.e  
Quant Time: Aug 28 04:18:21 2025  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_G\Method\FG080525.M  
Quant Title :  
QLast Update : Tue Aug 05 12:47:26 2025  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

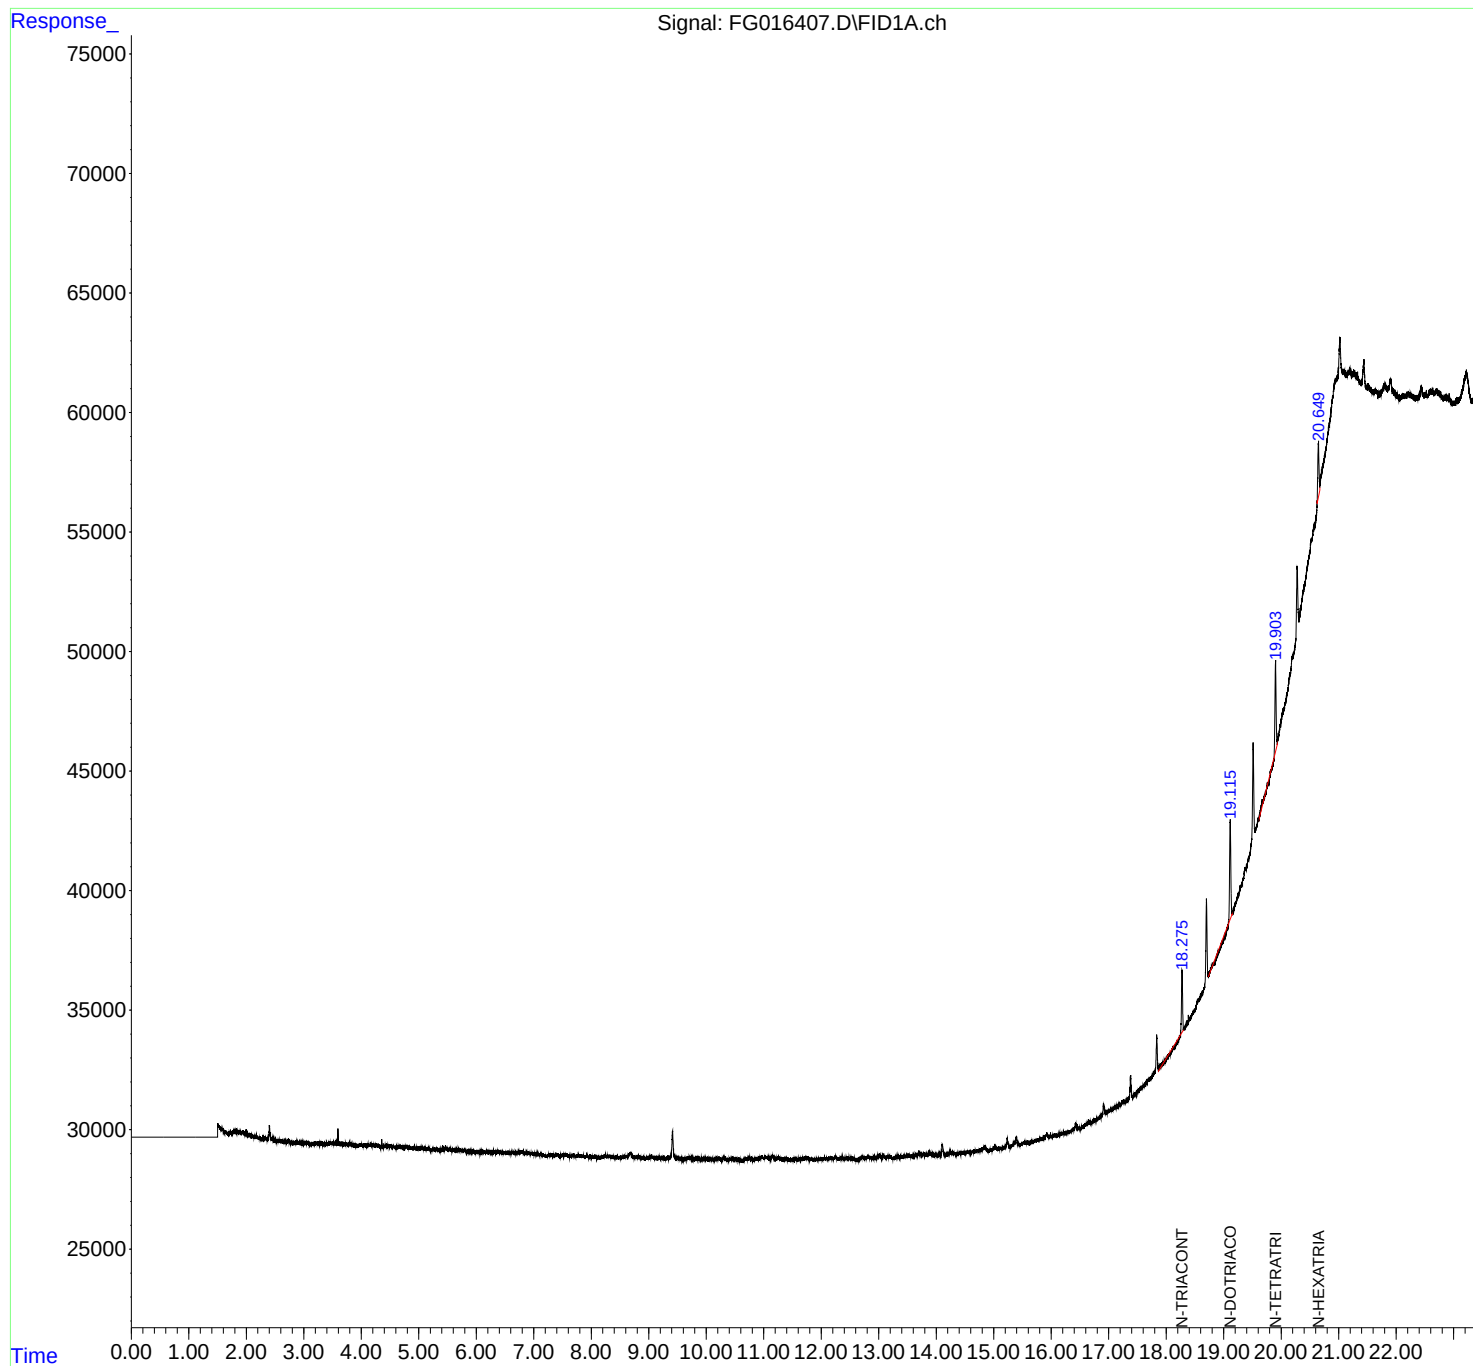


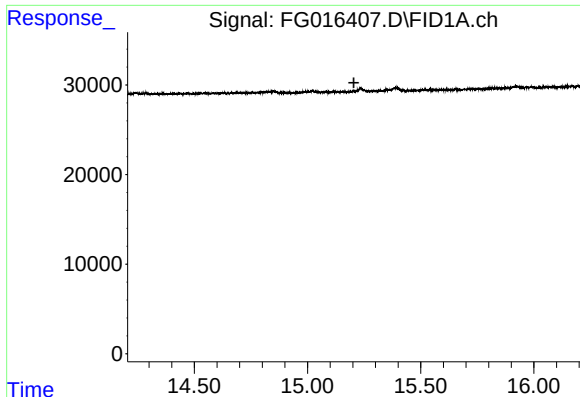

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min  
Exp R.T.: 15.205 min  
Response: 0  
Conc: N.D.

Instrument :  
FID\_G  
ClientSampleId :  
MECL2

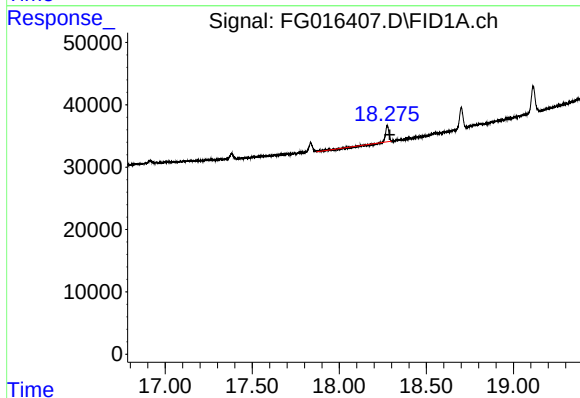


#13 N-TRIACONTANE

R.T.: 18.276 min  
Delta R.T.: -0.015 min  
Response: 24904  
Conc: 0.23 ug/ml

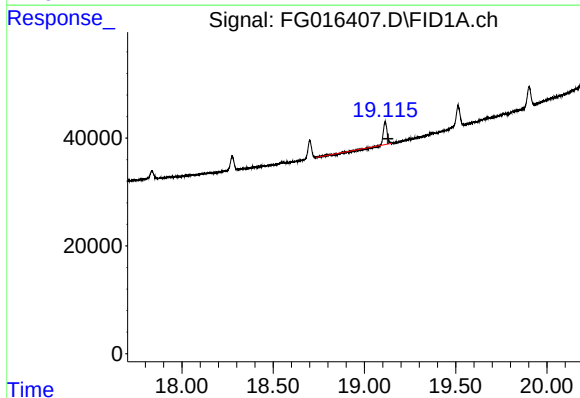


#14 N-DOTRIACONTANE

R.T.: 19.114 min  
Delta R.T.: -0.016 min  
Response: 47471  
Conc: 0.45 ug/ml

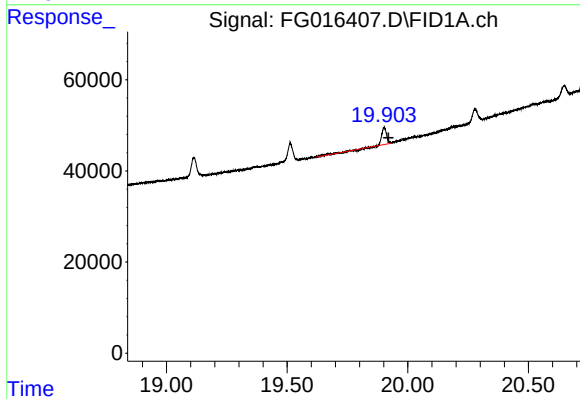

#15 N-TETRATRIACONTANE

R.T.: 19.902 min  
Delta R.T.: -0.018 min  
Response: 50624  
Conc: 0.53 ug/ml

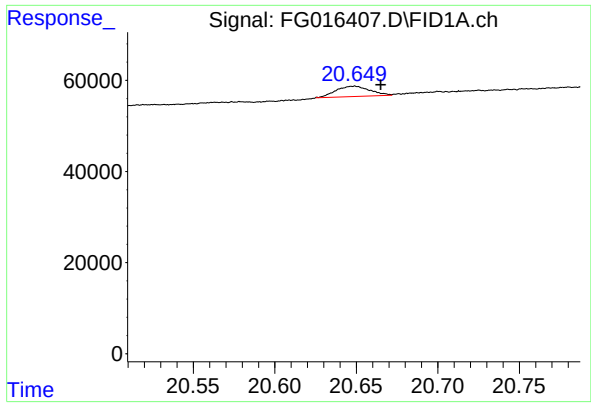

#16 N-HEXATRIACONTANE

R.T.: 20.649 min  
Delta R.T.: -0.016 min  
Response: 32526  
Conc: 0.44 ug/ml

Instrument :  
FID\_G  
ClientSampleId :  
MECL2