

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG082823\
Data File : FG012787.D
Signal(s) : FID1A.ch
Acq On : 28 Aug 2023 10:27
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 29 04:12:49 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG080223.M
Quant Title :
QLast Update : Wed Aug 02 18:57:31 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) N-DODECANE	6.771	2356615	18.347 ug/ml
12) N-OCTACOSANE	17.258	2010030	16.355 ug/ml
13) N-TRIACONTANE	18.146	72623	0.613 ug/ml
14) N-DOTRIACONTANE	18.980	97255	0.866 ug/ml
15) N-TETRATRIACONTANE	19.763	91909	0.970 ug/ml
16) N-HEXATRIACONTANE	20.505	59159	0.729 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG082823\
Data File : FG012787.D
Signal(s) : FID1A.ch
Acq On : 28 Aug 2023 10:27
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 29 04:12:49 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG080223.M
Quant Title :
QLast Update : Wed Aug 02 18:57:31 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

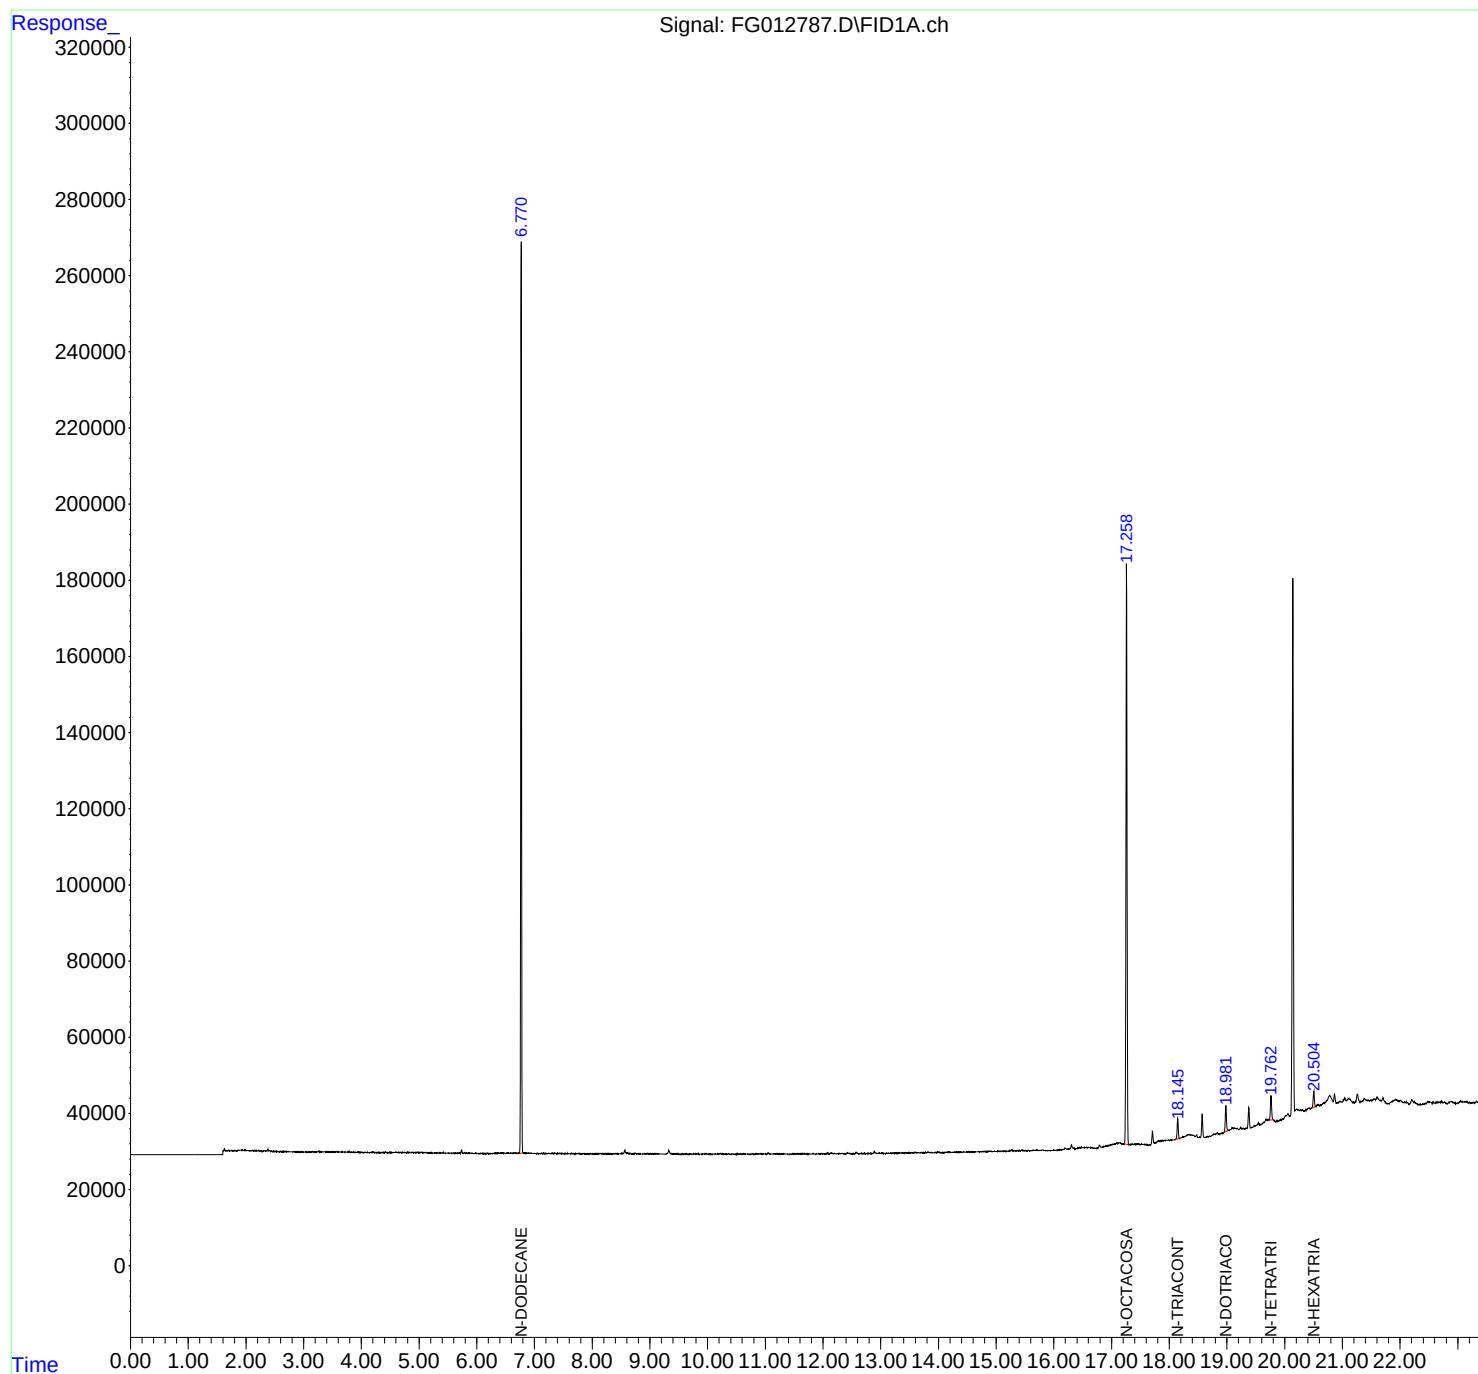

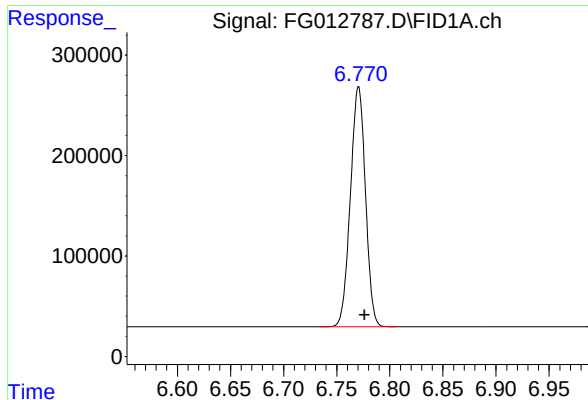


#3 N-DODECANE

R.T.: 6.771 min
Delta R.T.: -0.005 min
Response: 2356615
Conc: 18.35 ug/ml

Instrument :


FID_G

ClientSampleId :

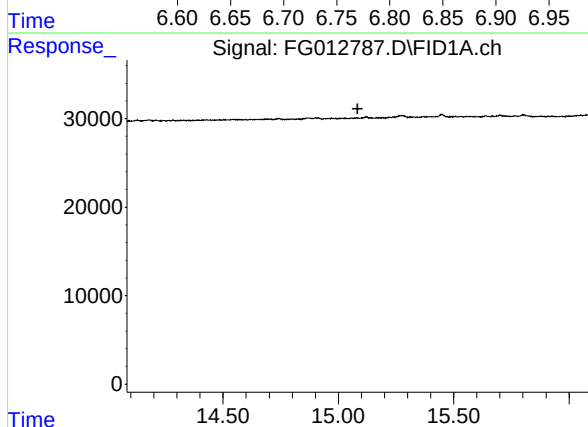


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T.: 15.083 min
Response: 0
Conc: N.D.

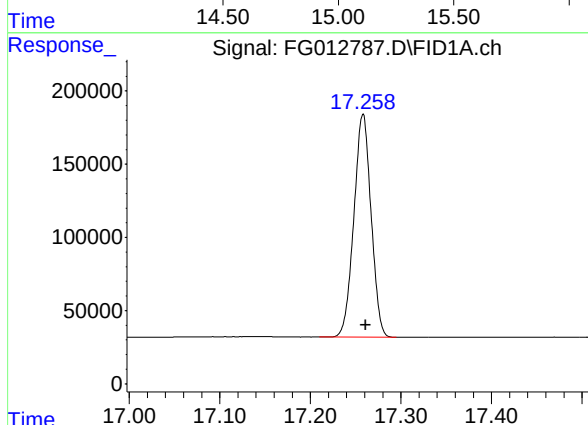


#12 N-OCTACOSANE

R.T.: 17.258 min
Delta R.T.: -0.003 min
Response: 2010030
Conc: 16.35 ug/ml

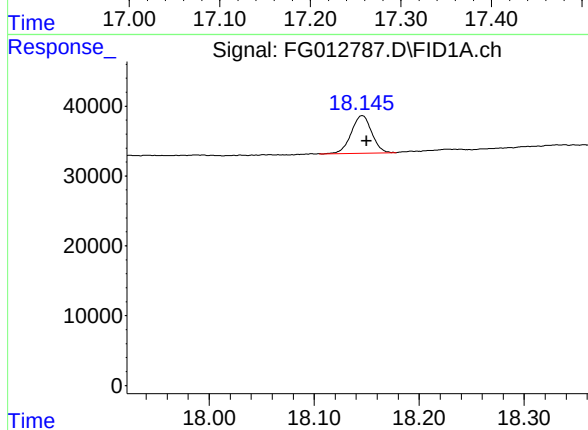

#13 N-TRIACONTANE


R.T.: 18.146 min
Delta R.T.: -0.004 min
Response: 72623
Conc: 0.61 ug/ml

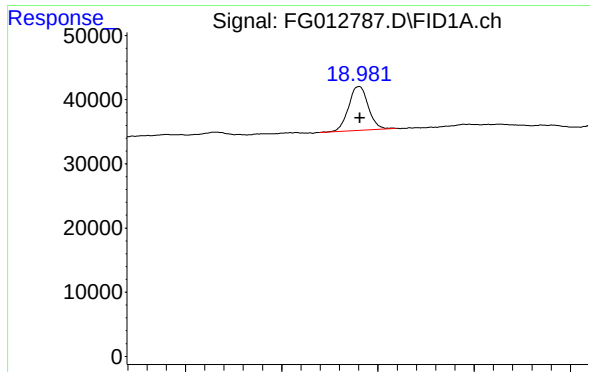

#14 N-DOTRIACONTANE


R.T.: 18.980 min
Delta R.T.: -0.001 min
Response: 97255
Conc: 0.87 ug/ml

Instrument :
FID_G
ClientSampleId :

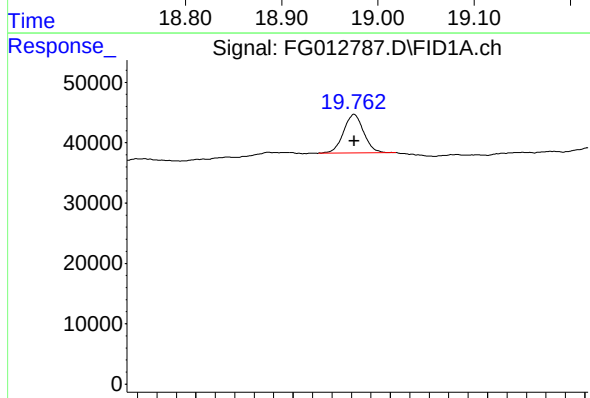

#15 N-TETRATRIACONTANE

R.T.: 19.763 min
Delta R.T.: 0.000 min
Response: 91909
Conc: 0.97 ug/ml

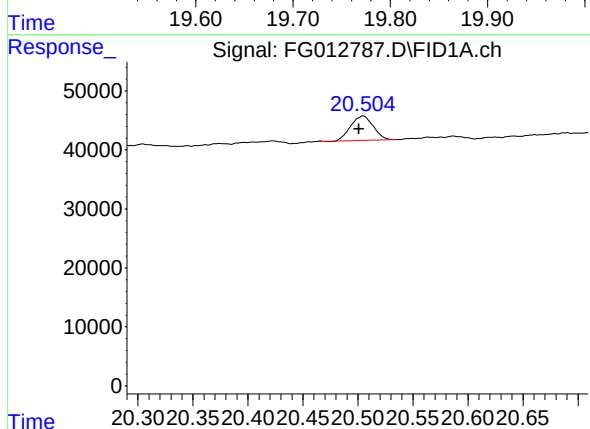

#16 N-HEXATRIACONTANE

R.T.: 20.505 min
Delta R.T.: 0.004 min
Response: 59159
Conc: 0.73 ug/ml