

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG082919\
Data File : FG005787.D
Signal(s) : FID1A.ch
Acq On : 29 Aug 2019 15:46
Operator : DD\AJ
Sample : PB122663BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
PB122663BL

Integration File: autoint1.e
Quant Time: Aug 29 23:16:51 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG080819.M
Quant Title :
QLast Update : Thu Aug 08 16:03:53 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.741	2423401	18.968 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG082919\
Data File : FG005787.D
Signal(s) : FID1A.ch
Acq On : 29 Aug 2019 15:46
Operator : DD\AJ
Sample : PB122663BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
PB122663BL

Integration File: autoint1.e
Quant Time: Aug 29 23:16:51 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG080819.M
Quant Title :
QLast Update : Thu Aug 08 16:03:53 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

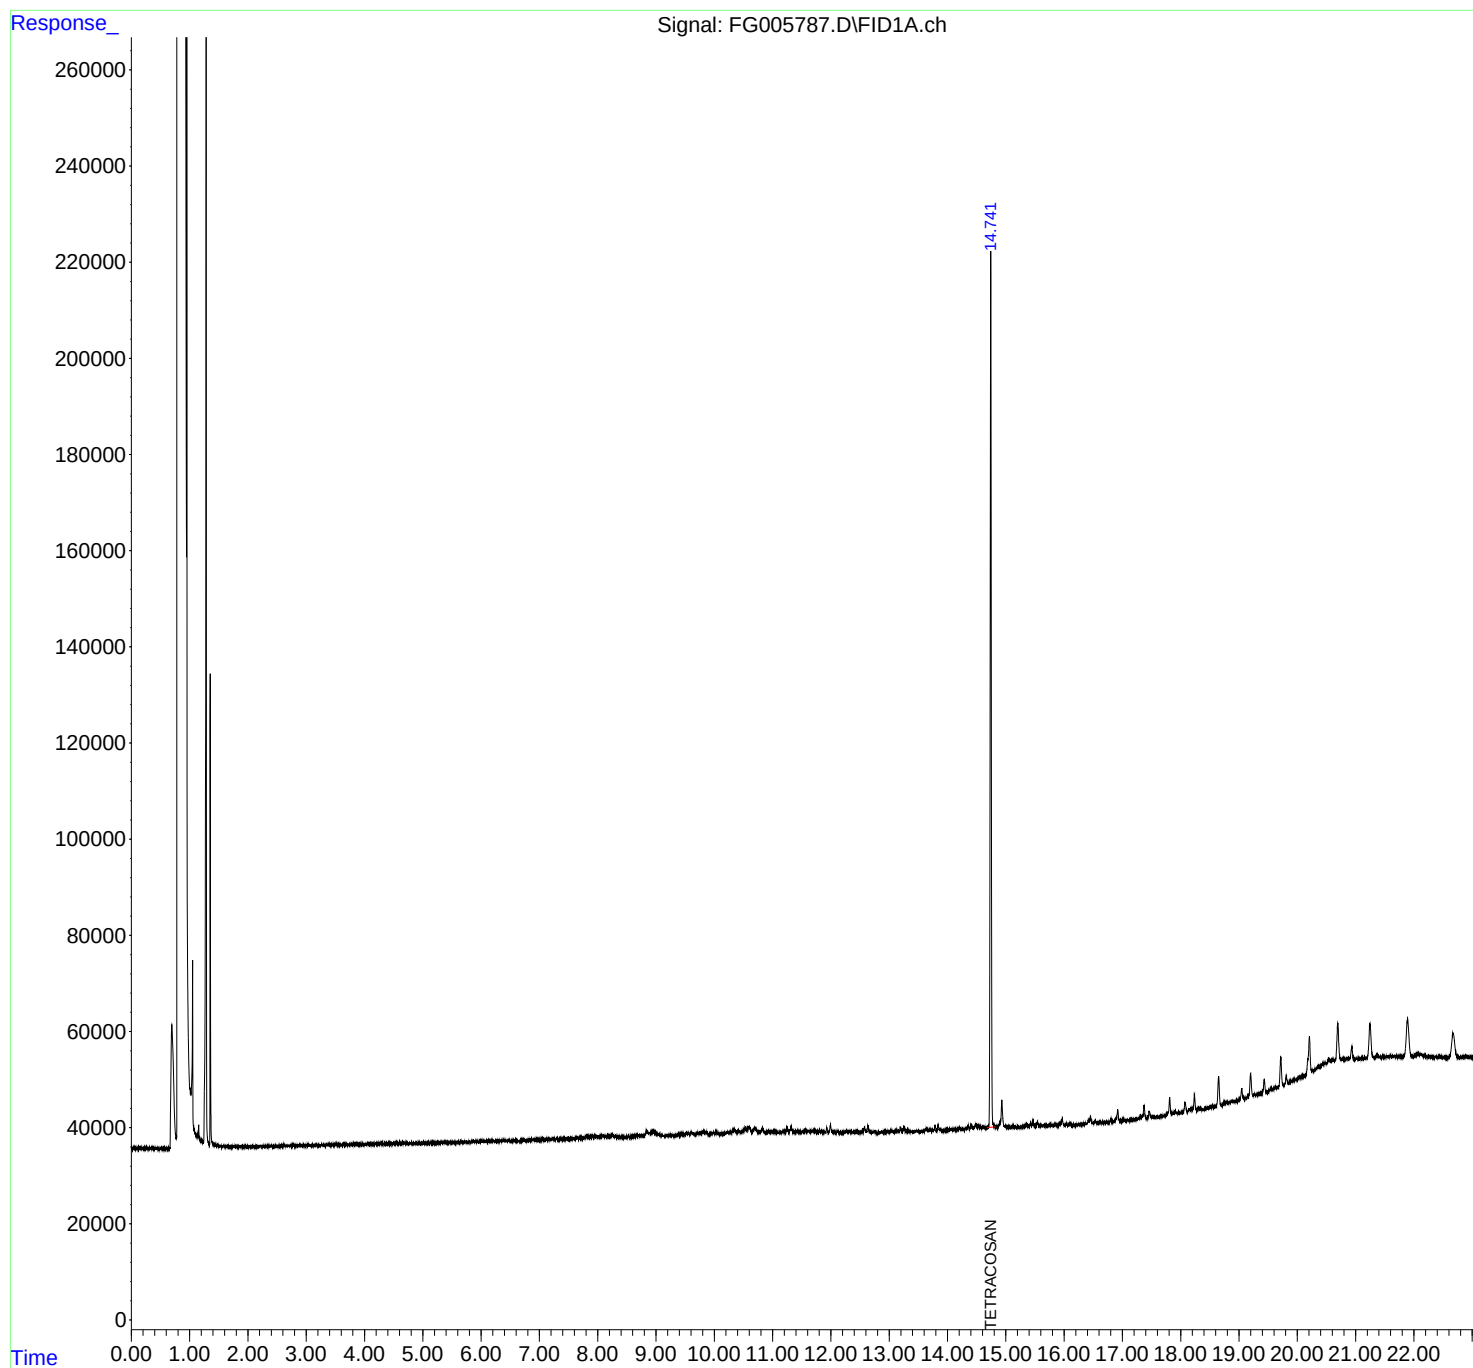

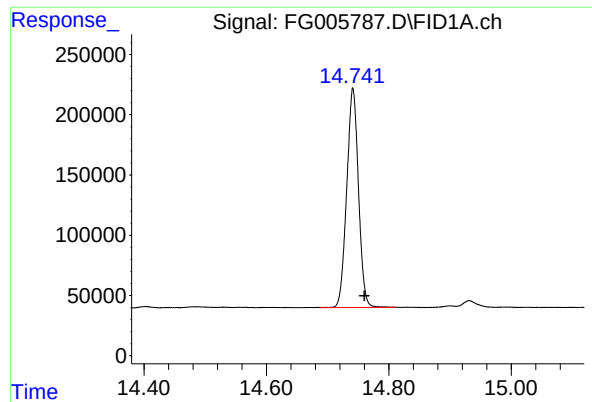

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.741 min
Delta R.T.: -0.018 min
Response: 2423401
Conc: 18.97 ug/ml

Instrument :
FID_G
ClientSampleId :
PB122663BL