

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG082923AL\
 Data File : FG012801.D
 Signal(s) : FID1A.ch
 Acq On : 29 Aug 2023 09:44
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 29 23:14:32 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\Aliphatic EPH 081023.M
 Quant Title : GC Extractables
 QLast Update : Thu Aug 10 15:32:13 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
17) T n-Tricontane (C30)	18.143	30264	0.304 ug/ml
18) T n-Dotriacontane (C32)	18.977	44111	0.446 ug/ml
19) T n-Tetratriacontane (C34)	19.760	33987	0.369 ug/ml
20) T n-Hexatriacontane (C36)	20.501	19463	0.217 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG082923AL\
Data File : FG012801.D
Signal(s) : FID1A.ch
Acq On : 29 Aug 2023 09:44
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 29 23:14:32 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\Aliphatic EPH 081023.M
Quant Title : GC Extractables
QLast Update : Thu Aug 10 15:32:13 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

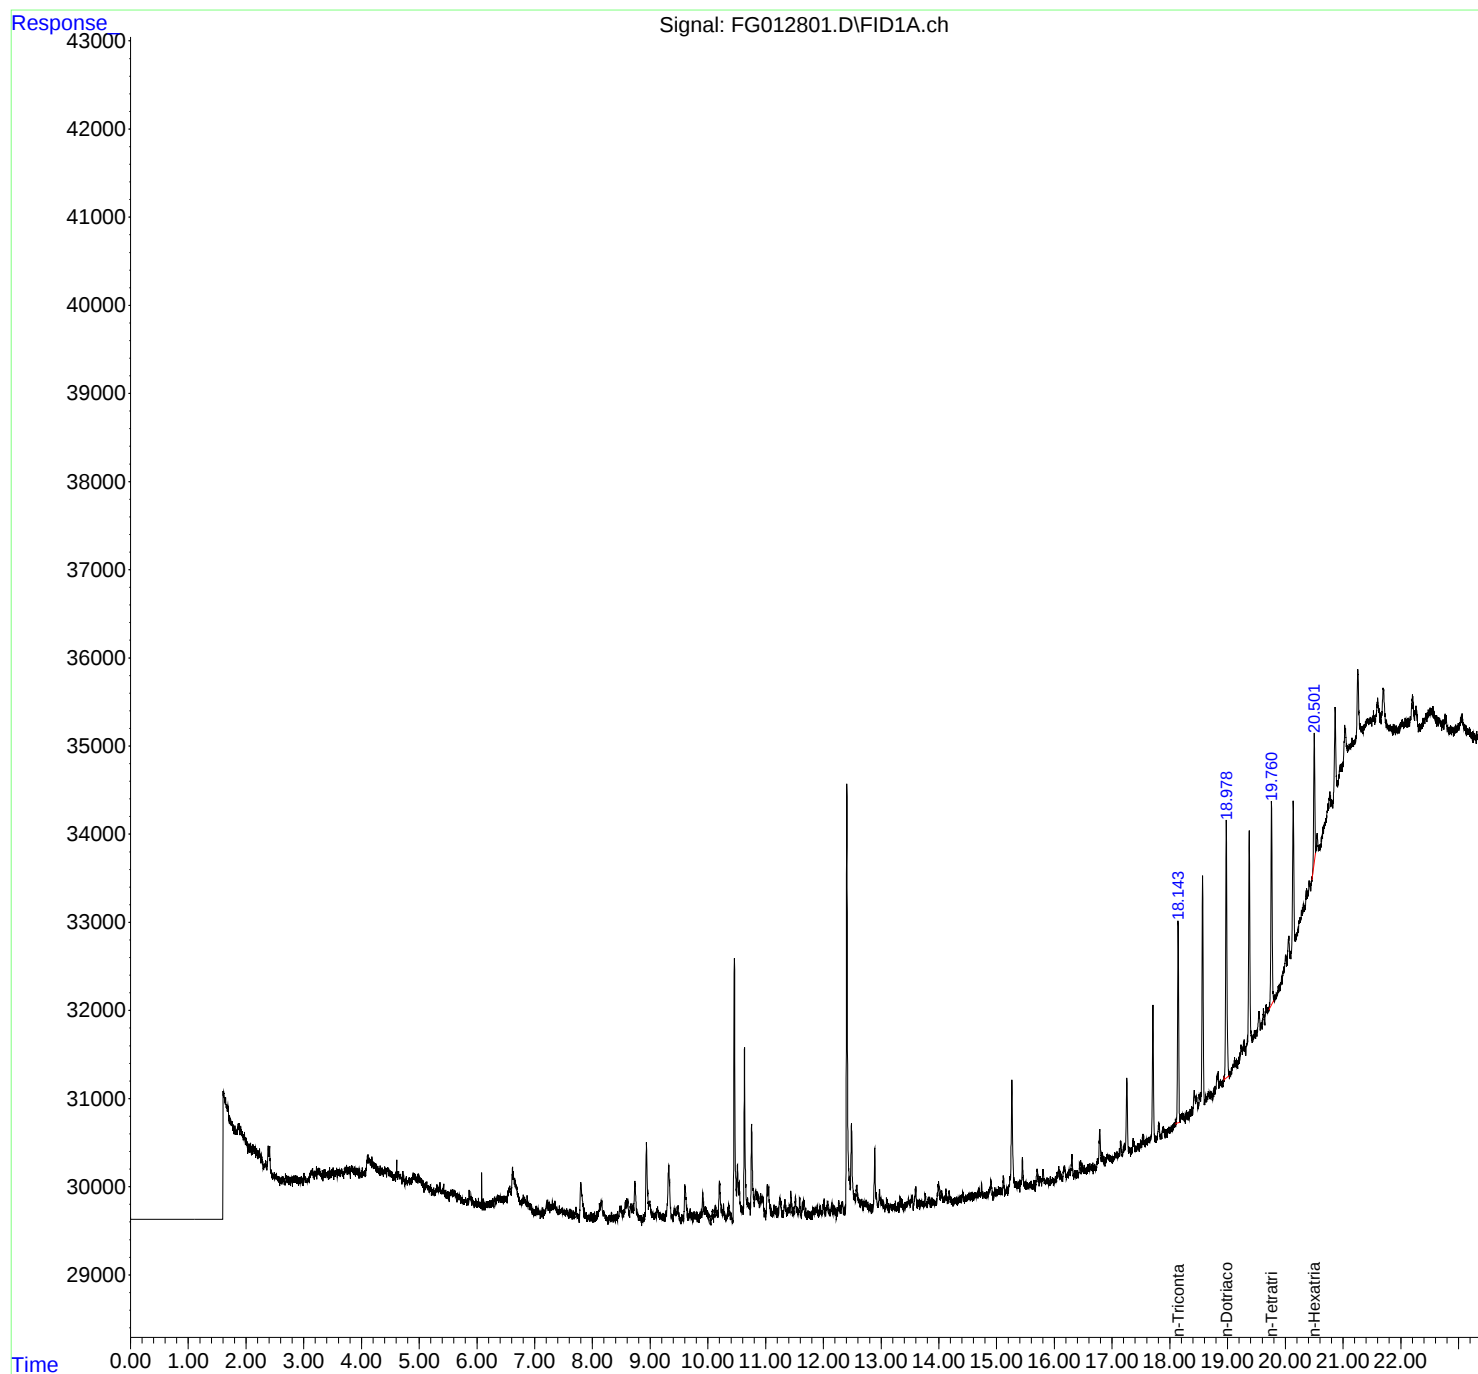


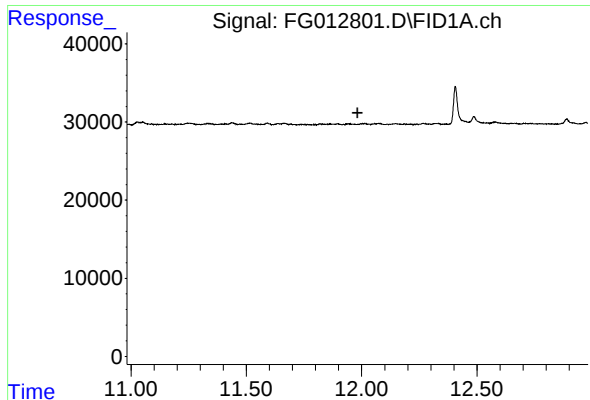

#9 ortho-Terphenyl (SURRE)


R.T.: 0.000 min
Exp R.T.: 11.982 min
Response: 0
Conc: N.D.

Instrument :
FID_G
ClientSampleId :

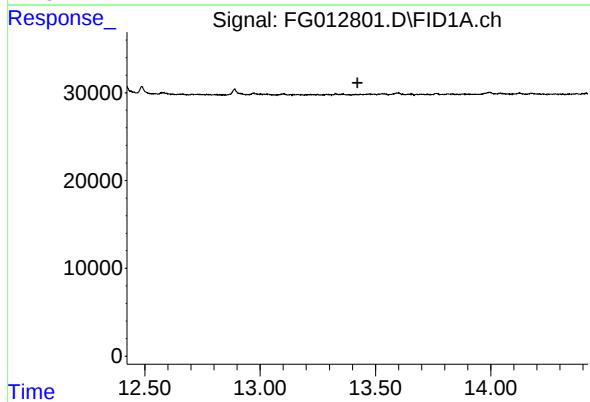


#12 1-chlorooctadecane (SURRE)

R.T.: 0.000 min
Exp R.T.: 13.422 min
Response: 0
Conc: N.D.

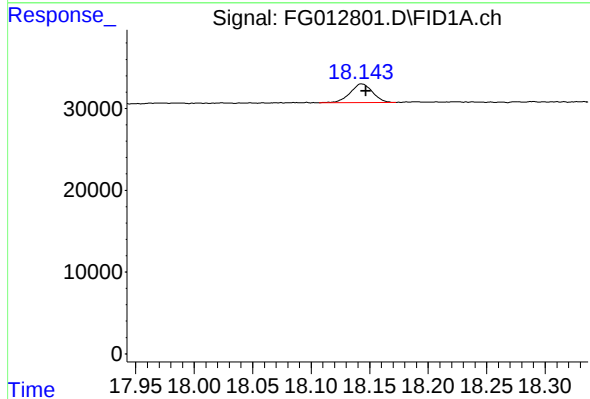


#17 n-Tricontane (C30)

R.T.: 18.143 min
Delta R.T.: -0.004 min
Response: 30264
Conc: 0.30 ug/ml

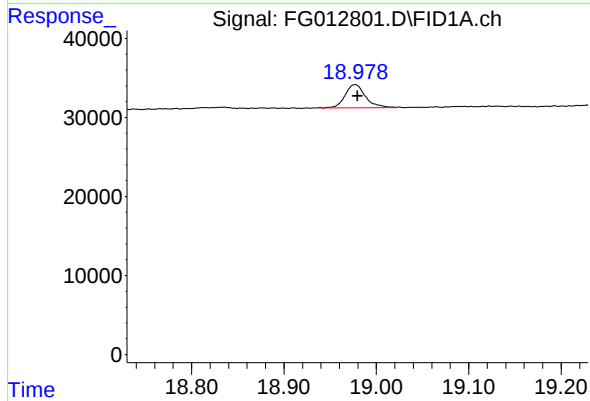

#18 n-Dotriacontane (C32)


R.T.: 18.977 min
Delta R.T.: -0.003 min
Response: 44111
Conc: 0.45 ug/ml

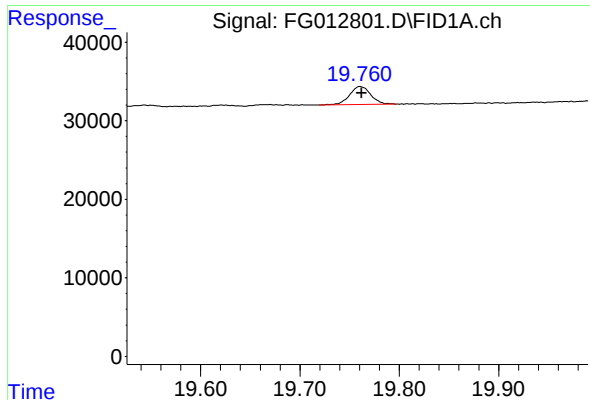

#19 n-Tetratriacontane (C34)

R.T.: 19.760 min
Delta R.T.: -0.002 min
Response: 33987
Conc: 0.37 ug/ml

Instrument :
FID_G
ClientSampleId :

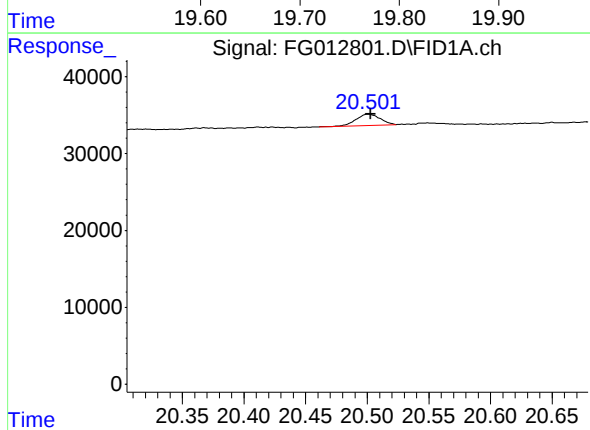

#20 n-Hexatriacontane (C36)

R.T.: 20.501 min
Delta R.T.: -0.002 min
Response: 19463
Conc: 0.22 ug/ml