

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG082923AL\
 Data File : FG012808.D
 Signal(s) : FID1A.ch
 Acq On : 29 Aug 2023 16:39
 Operator : YP\AJ
 Sample : 04196-06D
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 29 23:15:25 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\Aliphatic EPH 081023.M
 Quant Title : GC Extractables
 QLast Update : Thu Aug 10 15:32:13 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	11.982	3360543	24.928 ug/ml
Spiked Amount 50.000		Recovery =	49.86%
12) S 1-chlorooctadecane (S...	13.422	2658603	25.489 ug/ml
Spiked Amount 50.000		Recovery =	50.98%
Target Compounds			
1) T n-Nonane (C9)	3.325	33632	0.324 ug/ml
6) T n-Tetradecane (C14)	8.569	737670	6.865 ug/ml
10) T n-Eicosane (C20)	13.031f	34638	0.314 ug/ml
11) T n-Heneicosane (C21)	13.646f	21037	0.191 ug/ml
14) T n-Tetracosane (C24)	15.279	43307	0.401 ug/ml
15) T n-Hexacosane (C26)	16.304	30249	0.288 ug/ml
16) T n-Octacosane (C28)	17.256	60441	0.597 ug/ml
17) T n-Tricontane (C30)	18.144	110412	1.108 ug/ml
18) T n-Dotriacontane (C32)	18.977	168455	1.704 ug/ml
19) T n-Tetratriacontane (C34)	19.763	112921	1.227 ug/ml
20) T n-Hexatriacontane (C36)	20.501	78656	0.876 ug/ml
21) T n-Octatriacontane (C38)	21.257	60569	0.713 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG082923AL\
Data File : FG012808.D
Signal(s) : FID1A.ch
Acq On : 29 Aug 2023 16:39
Operator : YP\AJ
Sample : 04196-06D
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 29 23:15:25 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\Aliphatic EPH 081023.M
Quant Title : GC Extractables
QLast Update : Thu Aug 10 15:32:13 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

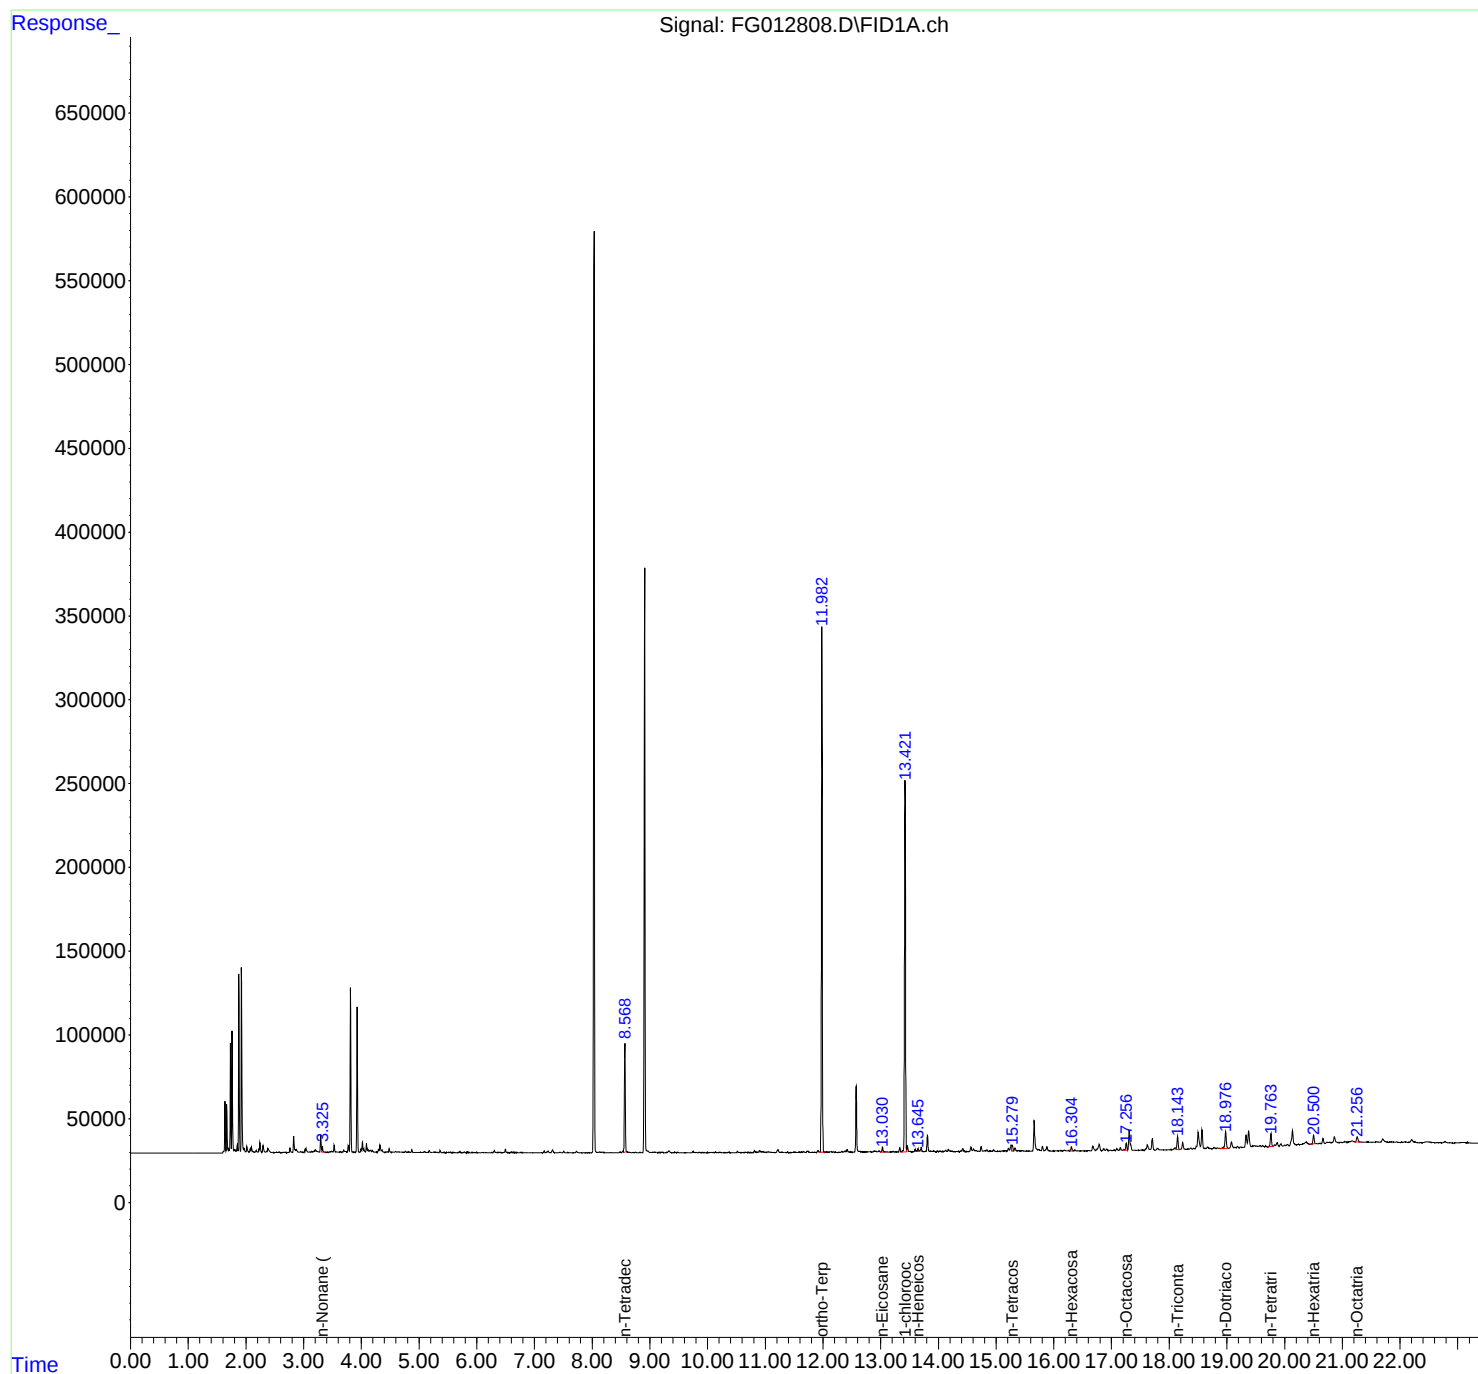


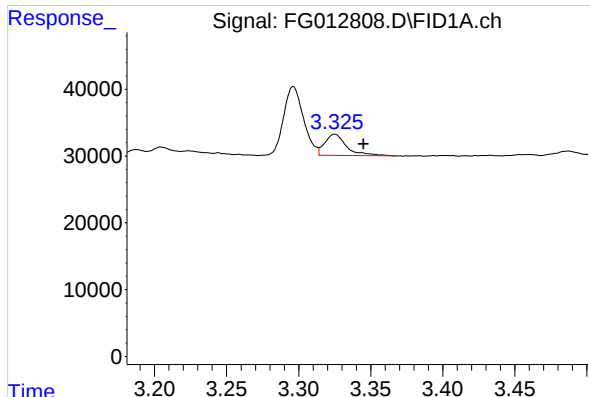

#1 n-Nonane (C9)


R.T.: 3.325 min
Delta R.T.: -0.020 min
Response: 33632
Conc: 0.32 ug/ml

Instrument :
FID_G
ClientSampleId :

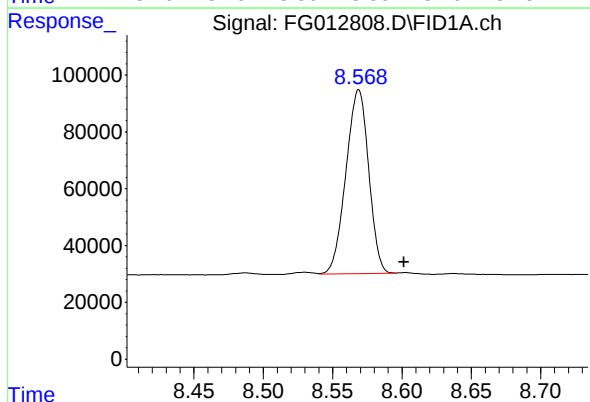


#6 n-Tetradecane (C14)

R.T.: 8.569 min
Delta R.T.: -0.032 min
Response: 737670
Conc: 6.87 ug/ml

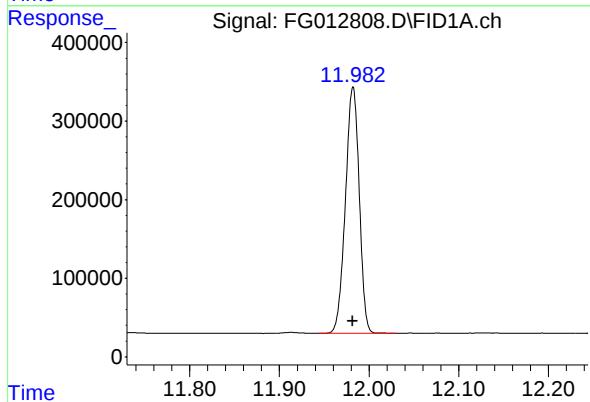


#9 ortho-Terphenyl (SURR)

R.T.: 11.982 min
Delta R.T.: 0.000 min
Response: 3360543
Conc: 24.93 ug/ml

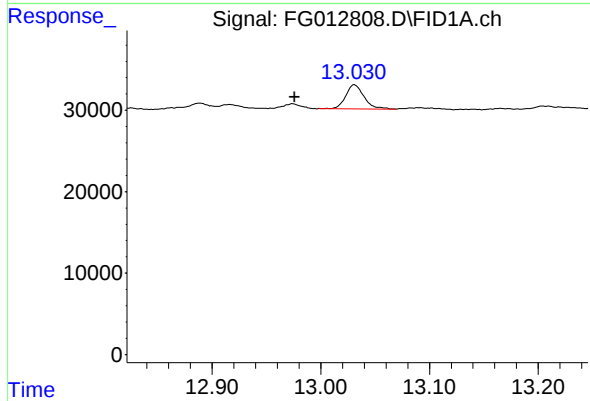

#10 n-Eicosane (C20)


R.T.: 13.031 min
Delta R.T.: 0.055 min
Response: 34638
Conc: 0.31 ug/ml

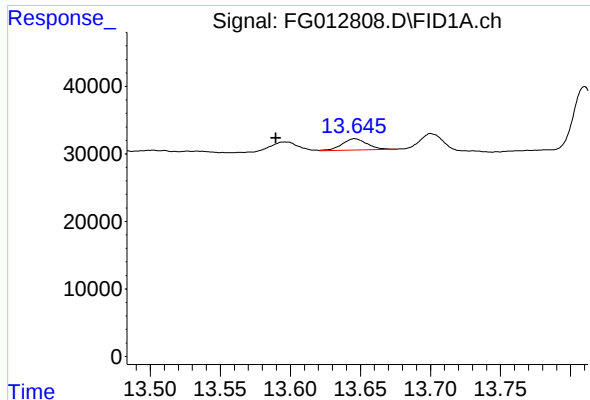

#11 n-Heneicosane (C21)


R.T.: 13.646 min
Delta R.T.: 0.056 min
Response: 21037
Conc: 0.19 ug/ml

Instrument :
FID_G
ClientSampleId :

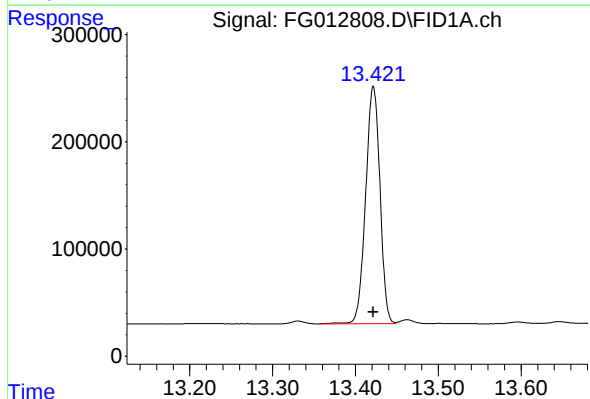


#12 1-chlorooctadecane (SURR)

R.T.: 13.422 min
Delta R.T.: 0.000 min
Response: 2658603
Conc: 25.49 ug/ml

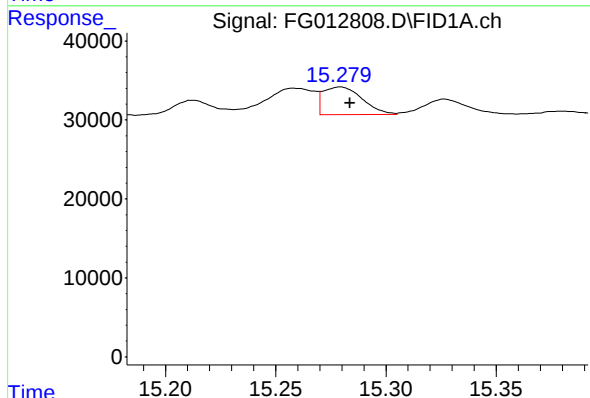


#14 n-Tetracosane (C24)

R.T.: 15.279 min
Delta R.T.: -0.005 min
Response: 43307
Conc: 0.40 ug/ml

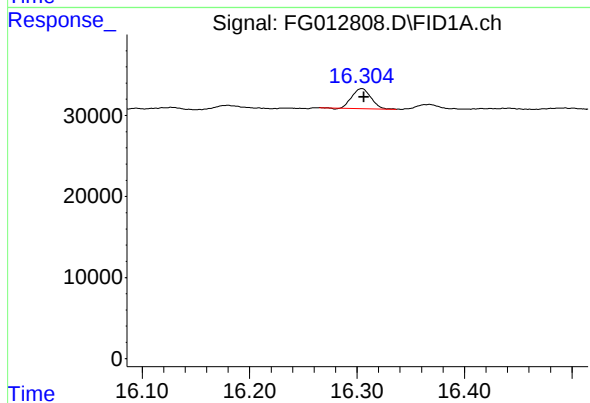

#15 n-Hexacosane (C26)

R.T.: 16.304 min
Delta R.T.: -0.002 min
Response: 30249
Conc: 0.29 ug/ml

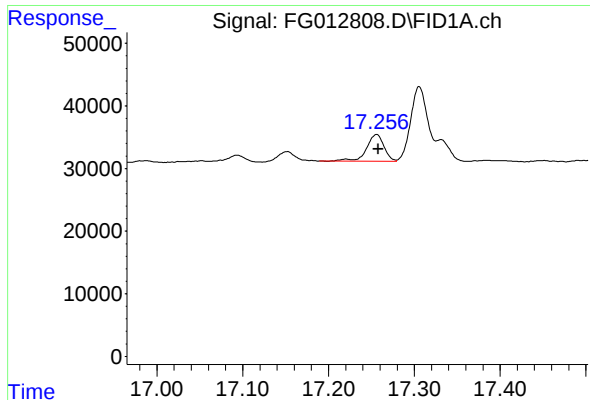


#16 n-Octacosane (C28)

R.T.: 17.256 min
Delta R.T.: -0.002 min
Response: 60441
Conc: 0.60 ug/ml

Instrument :


FID_G

ClientSampleId :

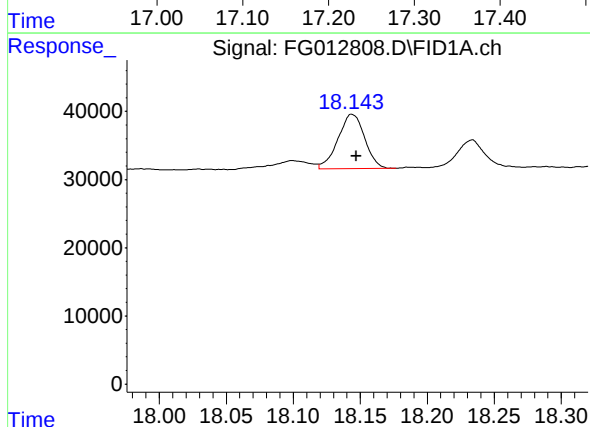


#17 n-Tricontane (C30)

R.T.: 18.144 min
Delta R.T.: -0.003 min
Response: 110412
Conc: 1.11 ug/ml

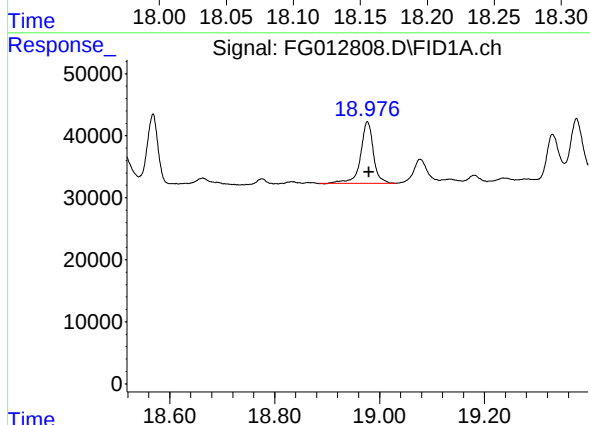


#18 n-Dotriacontane (C32)

R.T.: 18.977 min
Delta R.T.: -0.003 min
Response: 168455
Conc: 1.70 ug/ml

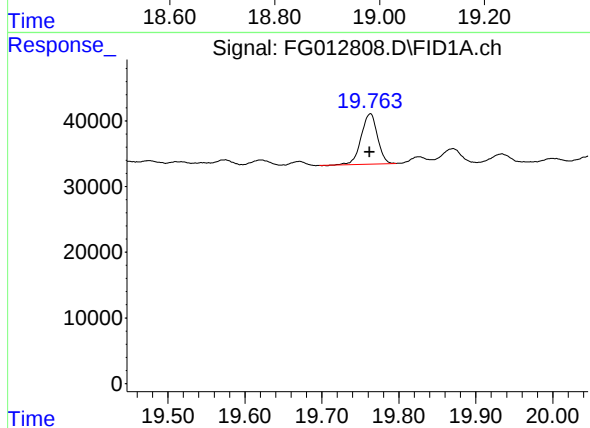

#19 n-Tetratriacontane (C34)


R.T.: 19.763 min
Delta R.T.: 0.000 min
Response: 112921
Conc: 1.23 ug/ml

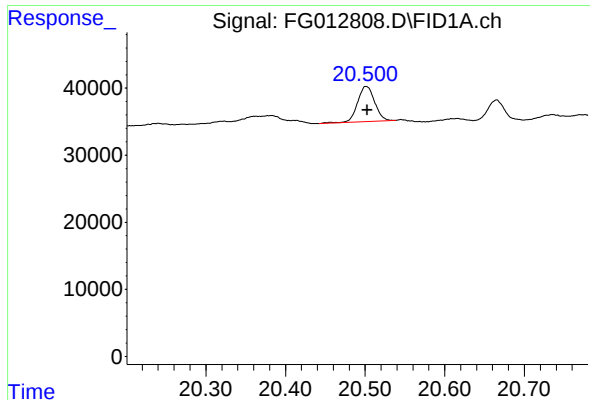

#20 n-Hexatriacontane (C36)

R.T.: 20.501 min
Delta R.T.: -0.002 min
Response: 78656
Conc: 0.88 ug/ml

Instrument :
FID_G
ClientSampleId :

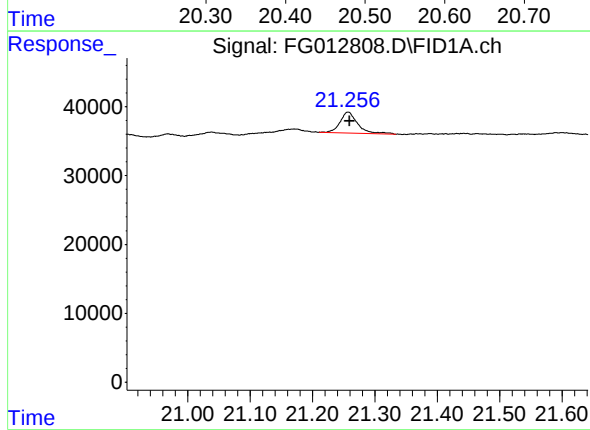

#21 n-Octatriacontane (C38)

R.T.: 21.257 min
Delta R.T.: -0.003 min
Response: 60569
Conc: 0.71 ug/ml