

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG083022\
Data File : FG010452.D
Signal(s) : FID1A.ch
Acq On : 30 Aug 2022 22:39
Operator : YP\AJ
Sample : N4439-03
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
KTS2-MH-02-0-20

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/31/2022
Supervised By :Ankita Jodhani 08/31/2022

Integration File: autoint1.e
Quant Time: Aug 31 04:47:17 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG082622.M
Quant Title :
QLast Update : Fri Aug 26 23:48:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.789	1445132	11.808 ug/mlm
Target Compounds			

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG083022\
Data File : FG010452.D
Signal(s) : FID1A.ch
Acq On : 30 Aug 2022 22:39
Operator : YP\AJ
Sample : N4439-03
Misc :
ALS Vial : 14 Sample Multiplier: 1


Instrument :
FID_G
ClientSampleId :
KTS2-MH-02-0-20


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/31/2022
Supervised By :Ankita Jodhani 08/31/2022

Integration File: autoint1.e
Quant Time: Aug 31 04:47:17 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG082622.M
Quant Title :
QLast Update : Fri Aug 26 23:48:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

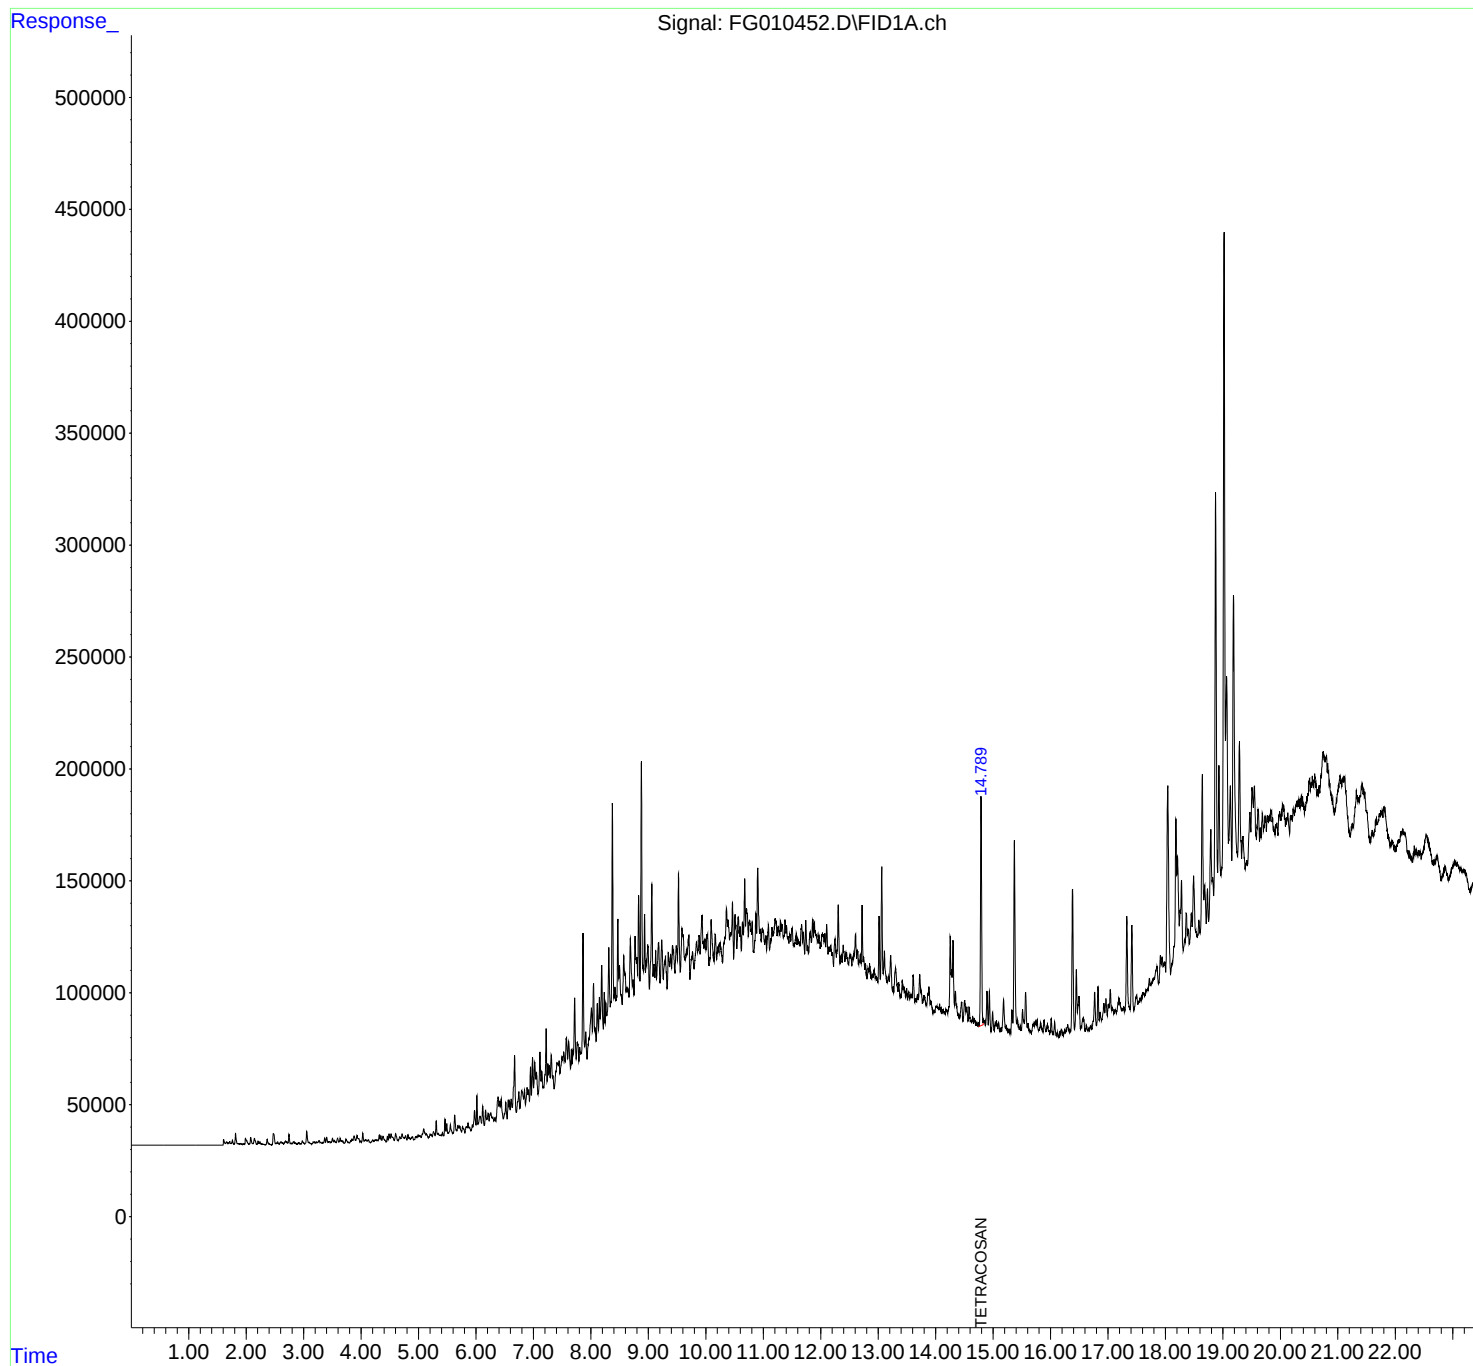

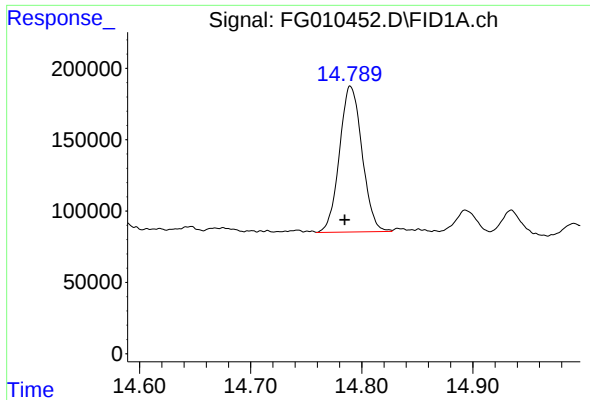

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.789 min
Delta R.T.: 0.004 min
Response: 1445132
Conc: 11.81 ug/ml

Instrument :
FID_G
ClientSampleId :
KTS2-MH-02-0-20

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/31/2022
Supervised By :Ankita Jodhani 08/31/2022