

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG083023\
 Data File : FG012834.D
 Signal(s) : FID1A.ch
 Acq On : 30 Aug 2023 18:48
 Operator : YP\AJ
 Sample : 04221-01
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :
 AU-5-082923

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/31/2023
 Supervised By :Ankita Jodhani 08/31/2023

Integration File: autoint1.e
 Quant Time: Aug 31 00:51:42 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG080223.M
 Quant Title :
 QLast Update : Wed Aug 02 18:57:31 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.081	2167353	19.375 ug/mlm
Target Compounds			

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG083023\
Data File : FG012834.D
Signal(s) : FID1A.ch
Acq On : 30 Aug 2023 18:48
Operator : YP\AJ
Sample : 04221-01
Misc :
ALS Vial : 15 Sample Multiplier: 1


Instrument :
FID_G
ClientSampleId :
AU-5-082923


Manual Integrations
APPROVED

Reviewed By : Yogesh Patel 08/31/2023
Supervised By : Ankita Jodhani 08/31/2023

Integration File: autoint1.e
Quant Time: Aug 31 00:51:42 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG080223.M
Quant Title :
QLast Update : Wed Aug 02 18:57:31 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

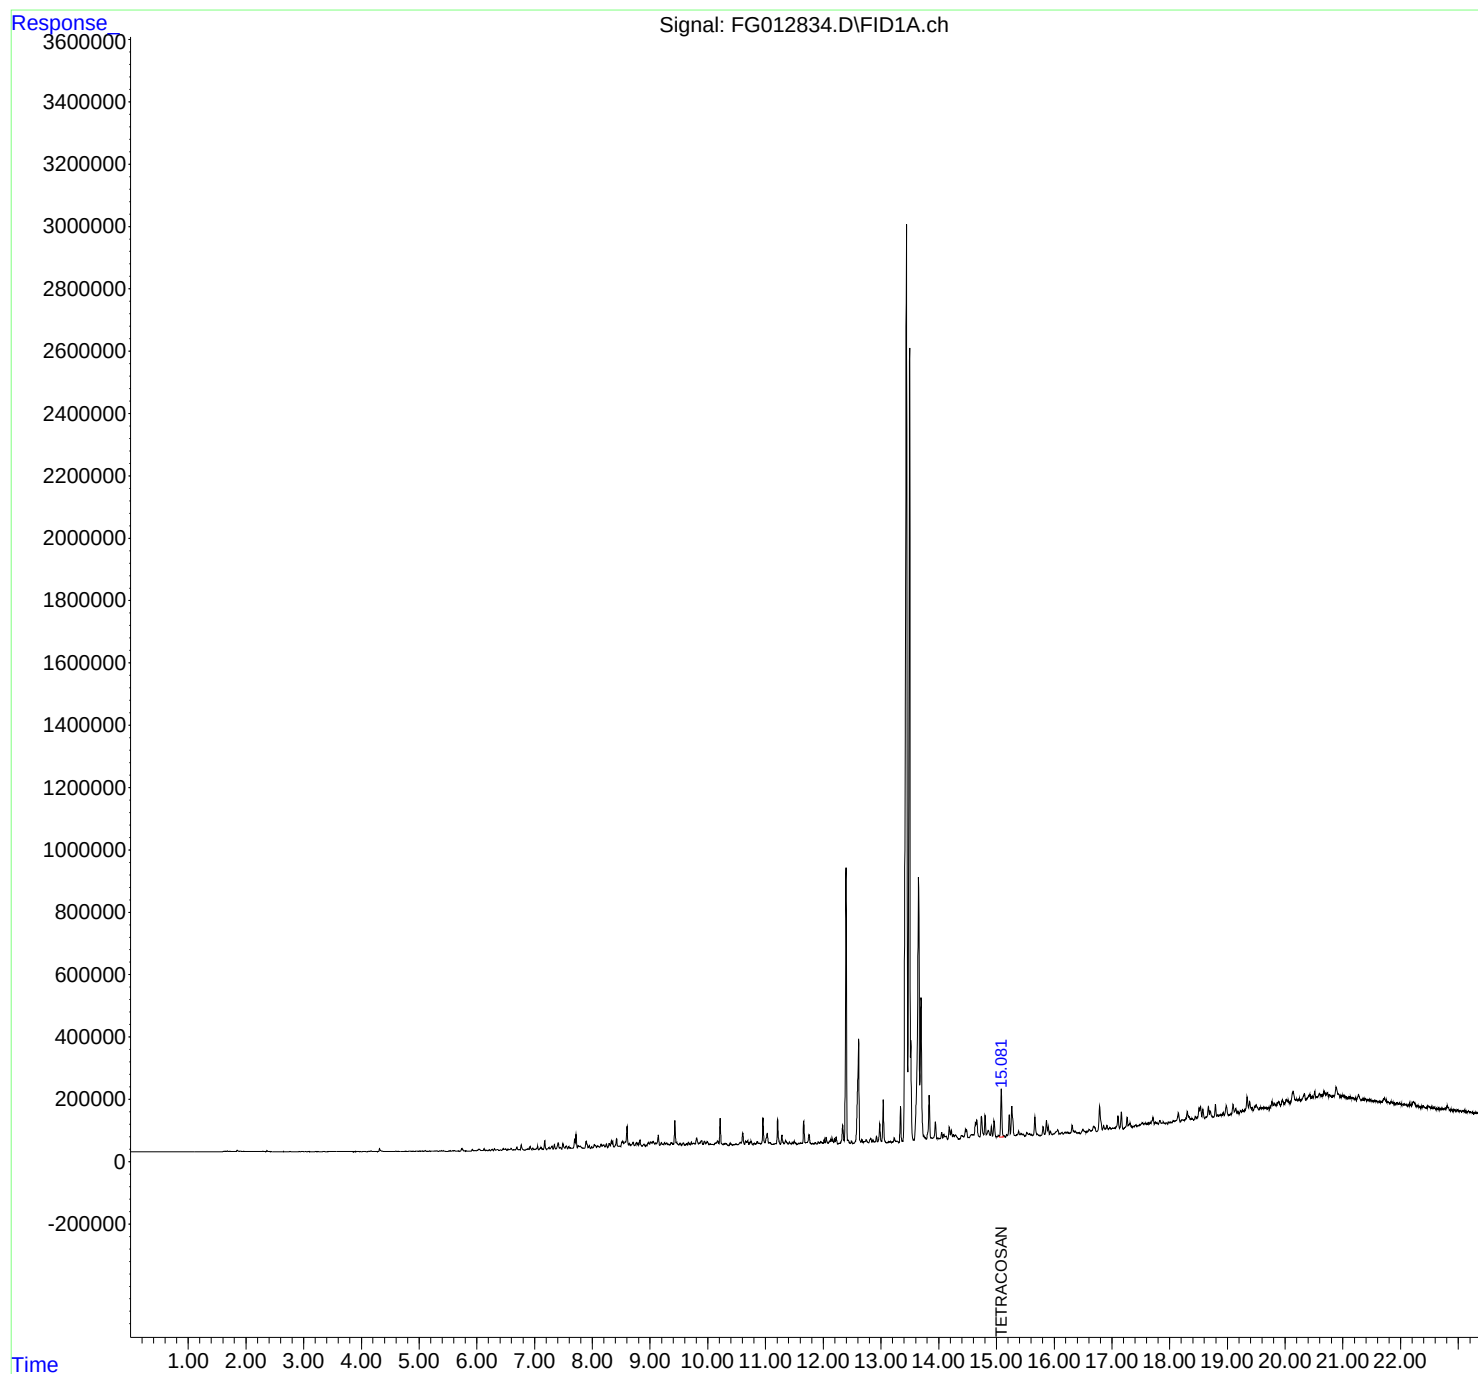

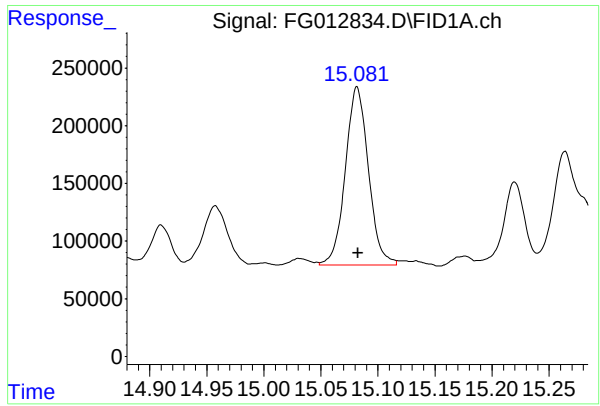

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.081 min
Delta R.T.: -0.002 min
Response: 2167353
Conc: 19.37 ug/ml

Instrument :
FID_G
ClientSampleId :
AU-5-082923

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/31/2023
Supervised By :Ankita Jodhani 08/31/2023