

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_G\Data\FG083023\  
Data File : FG012837.D  
Signal(s) : FID1A.ch  
Acq On : 30 Aug 2023 20:19  
Operator : YP\AJ  
Sample : I.BLK  
Misc :  
ALS Vial : 2 Sample Multiplier: 1

Instrument :  
FID\_G  
ClientSampleId :  
I.BLK

Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 08/31/2023  
Supervised By :Ankita Jodhani 08/31/2023

Integration File: autoint1.e  
Quant Time: Aug 31 00:52:05 2023  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_G\Method\FG080223.M  
Quant Title :  
QLast Update : Wed Aug 02 18:57:31 2023  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

| Compound                      | R.T.   | Response | Conc Units    |
|-------------------------------|--------|----------|---------------|
| -----                         |        |          |               |
| System Monitoring Compounds   |        |          |               |
| 9) S TETRACOSANE-d50 (SURR... | 15.084 | 1933948  | 17.288 ug/mlm |
| Target Compounds              |        |          |               |
| -----                         |        |          |               |

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_G\Data\FG083023\  
Data File : FG012837.D  
Signal(s) : FID1A.ch  
Acq On : 30 Aug 2023 20:19  
Operator : YP\AJ  
Sample : I.BLK  
Misc :  
ALS Vial : 2 Sample Multiplier: 1


Instrument :  
FID\_G  
ClientSampleId :  
I.BLK


Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 08/31/2023  
Supervised By :Ankita Jodhani 08/31/2023

Integration File: autoint1.e  
Quant Time: Aug 31 00:52:05 2023  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_G\Method\FG080223.M  
Quant Title :  
QLast Update : Wed Aug 02 18:57:31 2023  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

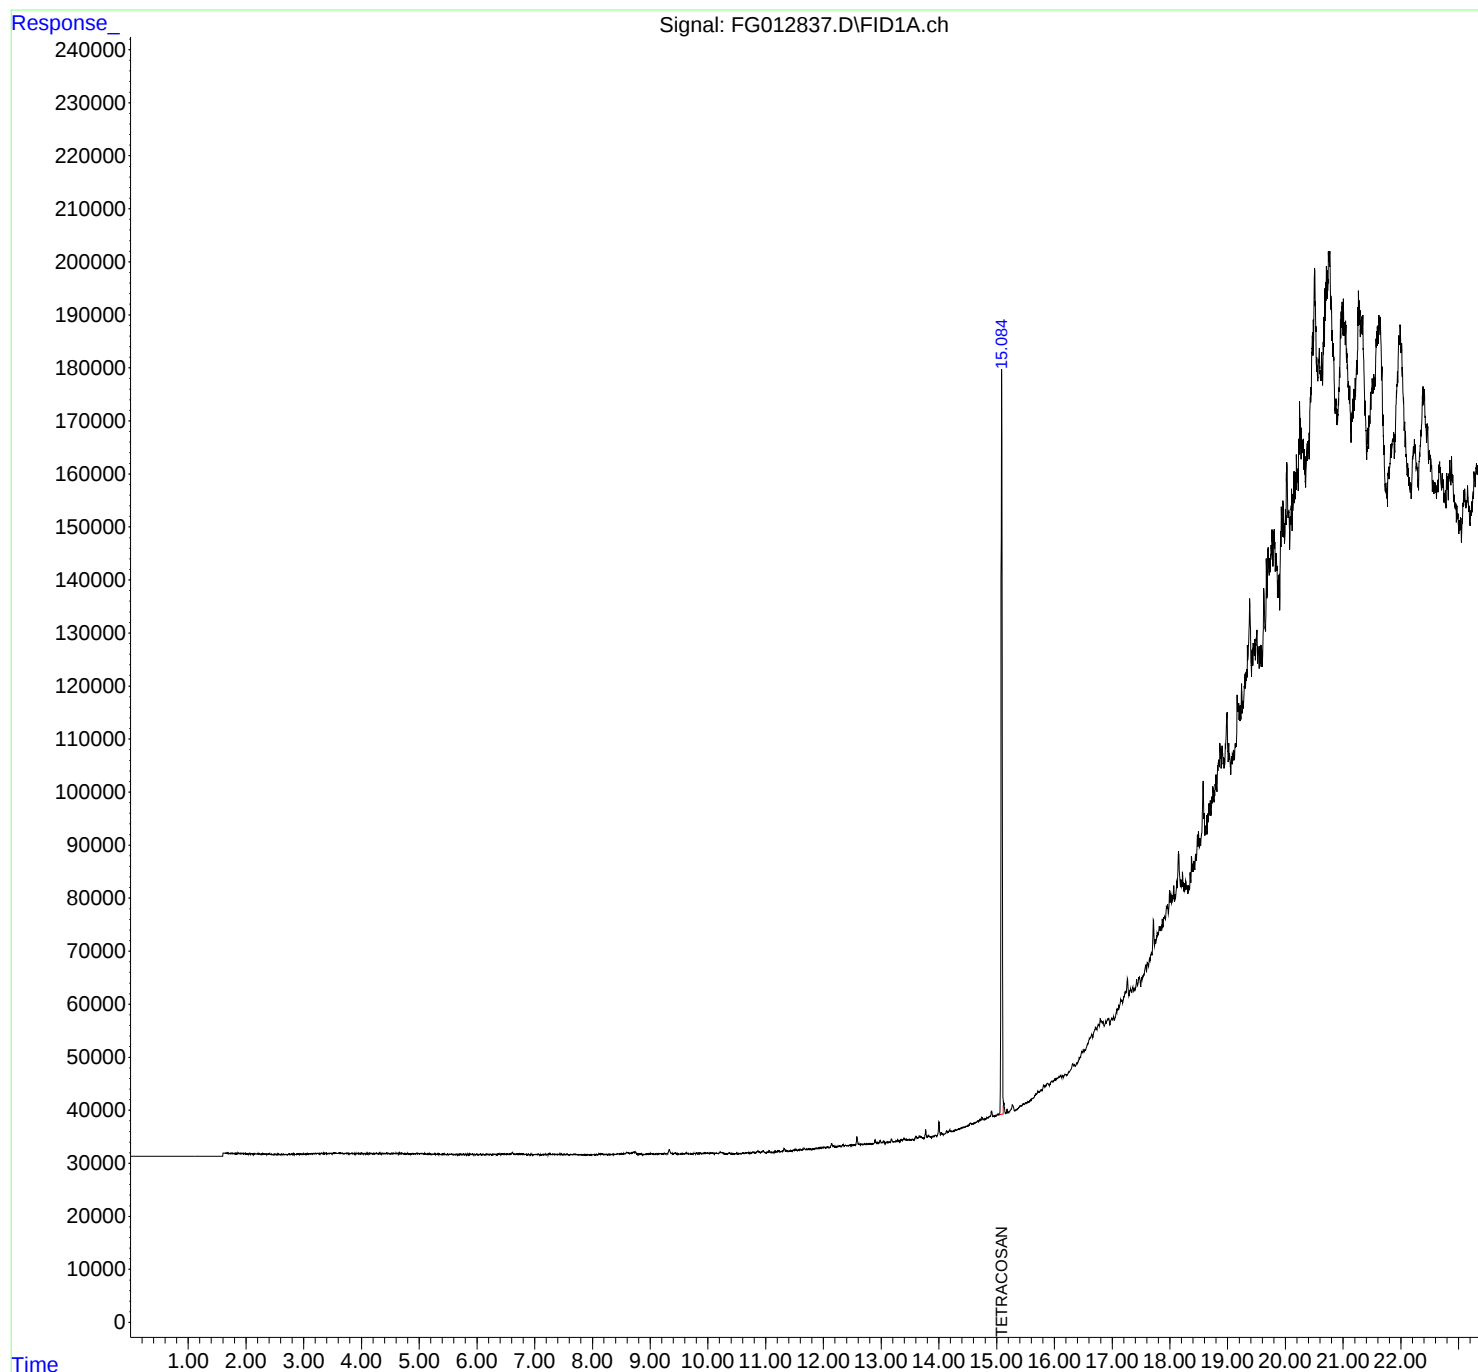

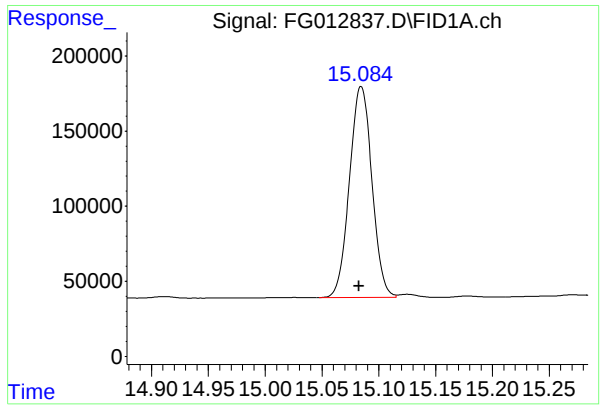

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.084 min  
Delta R.T.: 0.001 min  
Response: 1933948  
Conc: 17.29 ug/ml

Instrument :

FID\_G

ClientSampleId :

I.BLK

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 08/31/2023

Supervised By :Ankita Jodhani 08/31/2023