

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG083118\
 Data File : FG002223.D
 Signal(s) : FID1A.ch
 Acq On : 31 Aug 2018 17:38
 Operator : AJ\SJ
 Sample : J4282-15 10X
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 31 23:26:52 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG083018.M
 Quant Title :
 QLast Update : Thu Aug 30 14:49:31 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.427	310335	2.460 ug/ml
Target Compounds			
4) N-TETRADECANE	8.053f	88117	0.671 ug/ml
7) N-EICOSANE	12.382	1585168	11.158 ug/ml
8) N-DOCOSANE	13.546	298314	2.090 ug/ml
10) N-TETRACOSANE	14.602	1142629	7.993 ug/ml
11) N-HEXACOSANE	15.651	127198	0.886 ug/ml
12) N-OCTACOSANE	16.612	319316	2.182 ug/ml
13) N-TRIACONTANE	17.480	240905	1.588 ug/ml
14) N-DOTRIACONTANE	18.285	606685	4.113 ug/ml
15) N-TETRATRIACONTANE	19.110	127255	0.922 ug/ml
16) N-HEXATRIACONTANE	19.837	51891	0.405 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG083118\
Data File : FG002223.D
Signal(s) : FID1A.ch
Acq On : 31 Aug 2018 17:38
Operator : AJ\SJ
Sample : J4282-15 10X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 31 23:26:52 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG083018.M
Quant Title :
QLast Update : Thu Aug 30 14:49:31 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

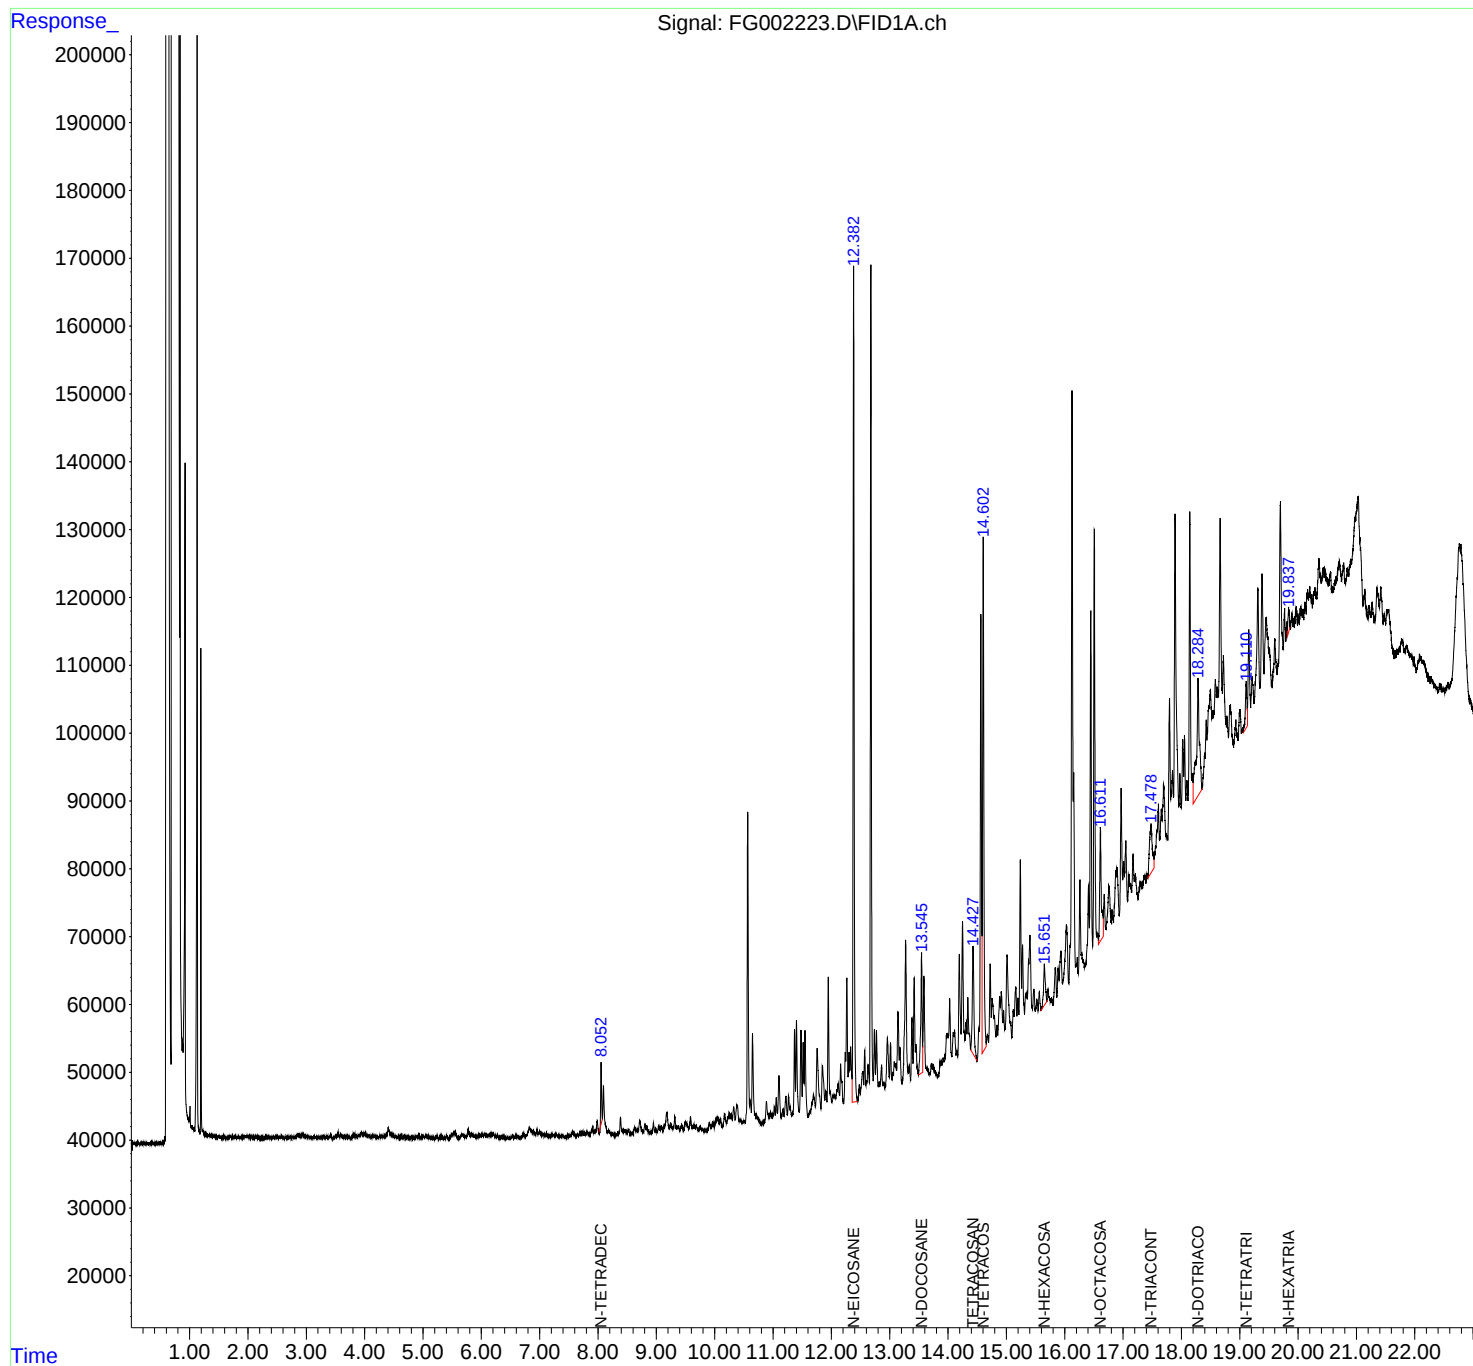


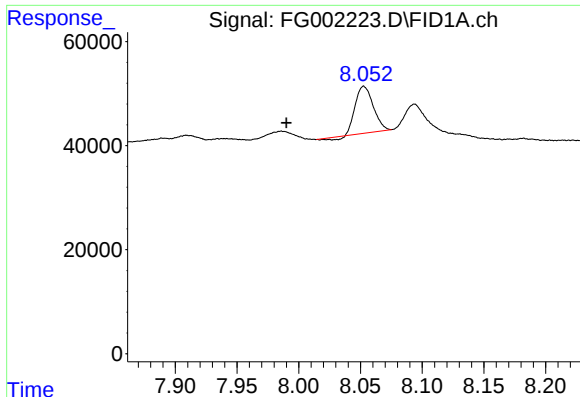

#4 N-TETRADECANE


R.T.: 8.053 min
Delta R.T.: 0.063 min
Response: 88117
Conc: 0.67 ug/ml

Instrument :
FID_G
ClientSampleId :

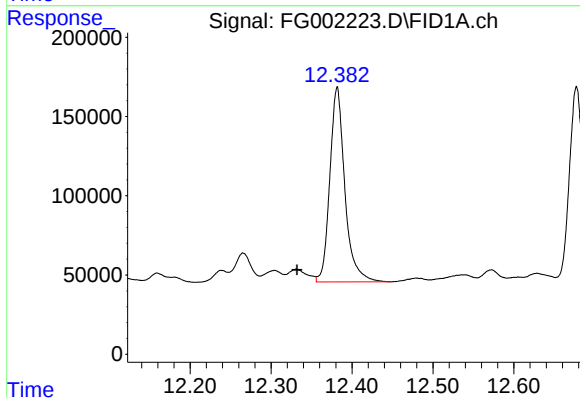


#7 N-EICOSANE

R.T.: 12.382 min
Delta R.T.: 0.049 min
Response: 1585168
Conc: 11.16 ug/ml

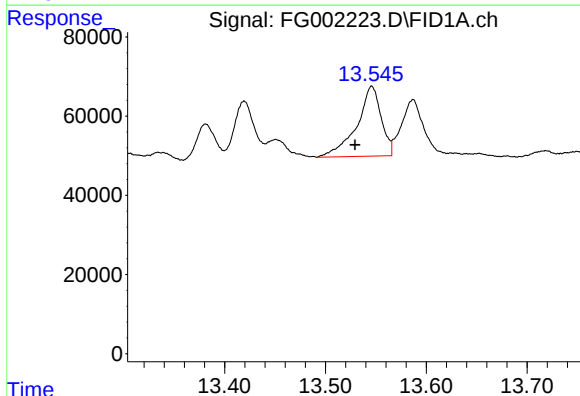


#8 N-DOCOSANE

R.T.: 13.546 min
Delta R.T.: 0.017 min
Response: 298314
Conc: 2.09 ug/ml

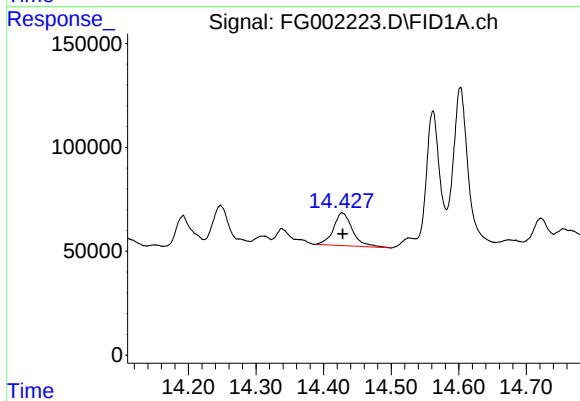

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.427 min
Delta R.T.: -0.001 min
Response: 310335
Conc: 2.46 ug/ml

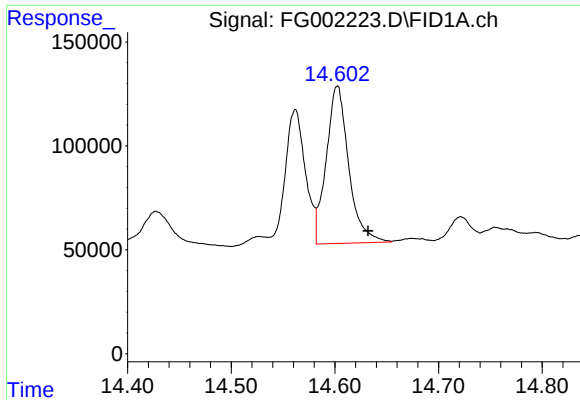

#10 N-TETRACOSANE


R.T.: 14.602 min
Delta R.T.: -0.029 min
Response: 1142629
Conc: 7.99 ug/ml

Instrument :
FID_G
ClientSampleId :

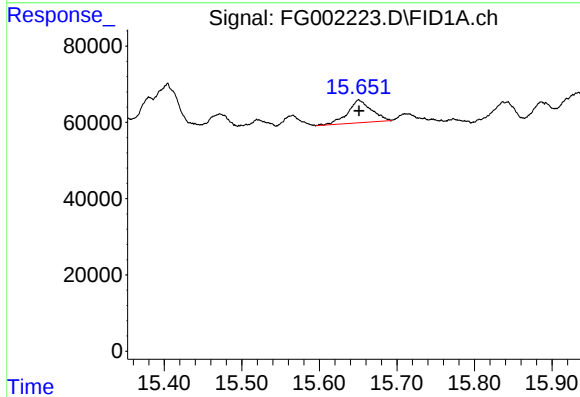


#11 N-HEXACOSANE

R.T.: 15.651 min
Delta R.T.: 0.000 min
Response: 127198
Conc: 0.89 ug/ml

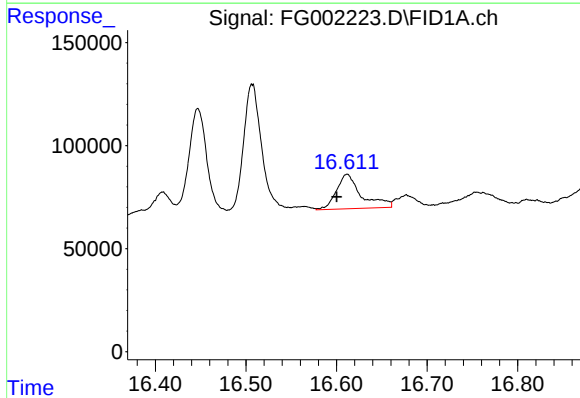


#12 N-OCTACOSANE

R.T.: 16.612 min
Delta R.T.: 0.012 min
Response: 319316
Conc: 2.18 ug/ml

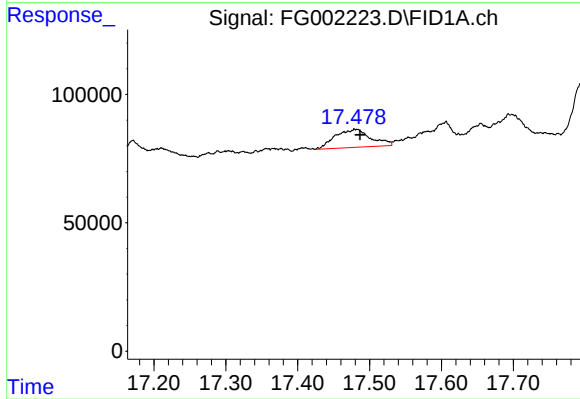

#13 N-TRIACONTANE


R.T.: 17.480 min
Delta R.T.: -0.007 min
Response: 240905
Conc: 1.59 ug/ml

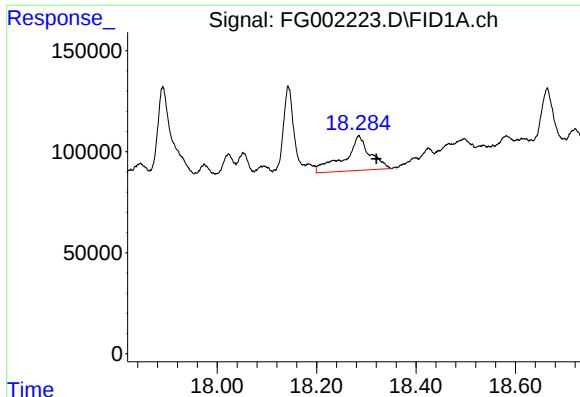

#14 N-DOTRIACONTANE


R.T.: 18.285 min
Delta R.T.: -0.035 min
Response: 606685
Conc: 4.11 ug/ml

Instrument :
FID_G
ClientSampleId :

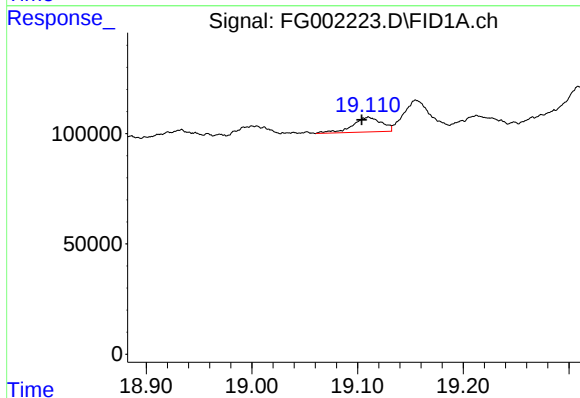

#15 N-TETRATRIACONTANE

R.T.: 19.110 min
Delta R.T.: 0.006 min
Response: 127255
Conc: 0.92 ug/ml

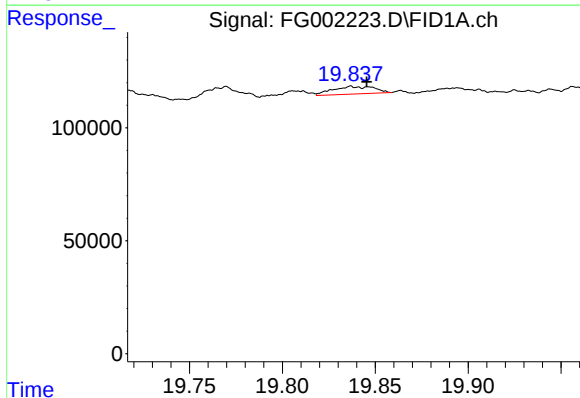

#16 N-HEXATRIACONTANE

R.T.: 19.837 min
Delta R.T.: -0.008 min
Response: 51891
Conc: 0.40 ug/ml