

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG083118\
 Data File : FG002226.D
 Signal(s) : FID1A.ch
 Acq On : 31 Aug 2018 19:08
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 31 23:27:27 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG083018.M
 Quant Title :
 QLast Update : Thu Aug 30 14:49:31 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.426	2348973	18.619 ug/ml
Target Compounds			
13) N-TRIACONTANE	17.487	70760	0.466 ug/ml
14) N-DOTRIACONTANE	18.319	722400	4.898 ug/ml
16) N-HEXATRIACONTANE	19.845	1010126	7.877 ug/ml
18) N-TETRACONTANE	21.394	109564	1.010 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG083118\
Data File : FG002226.D
Signal(s) : FID1A.ch
Acq On : 31 Aug 2018 19:08
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 31 23:27:27 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG083018.M
Quant Title :
QLast Update : Thu Aug 30 14:49:31 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

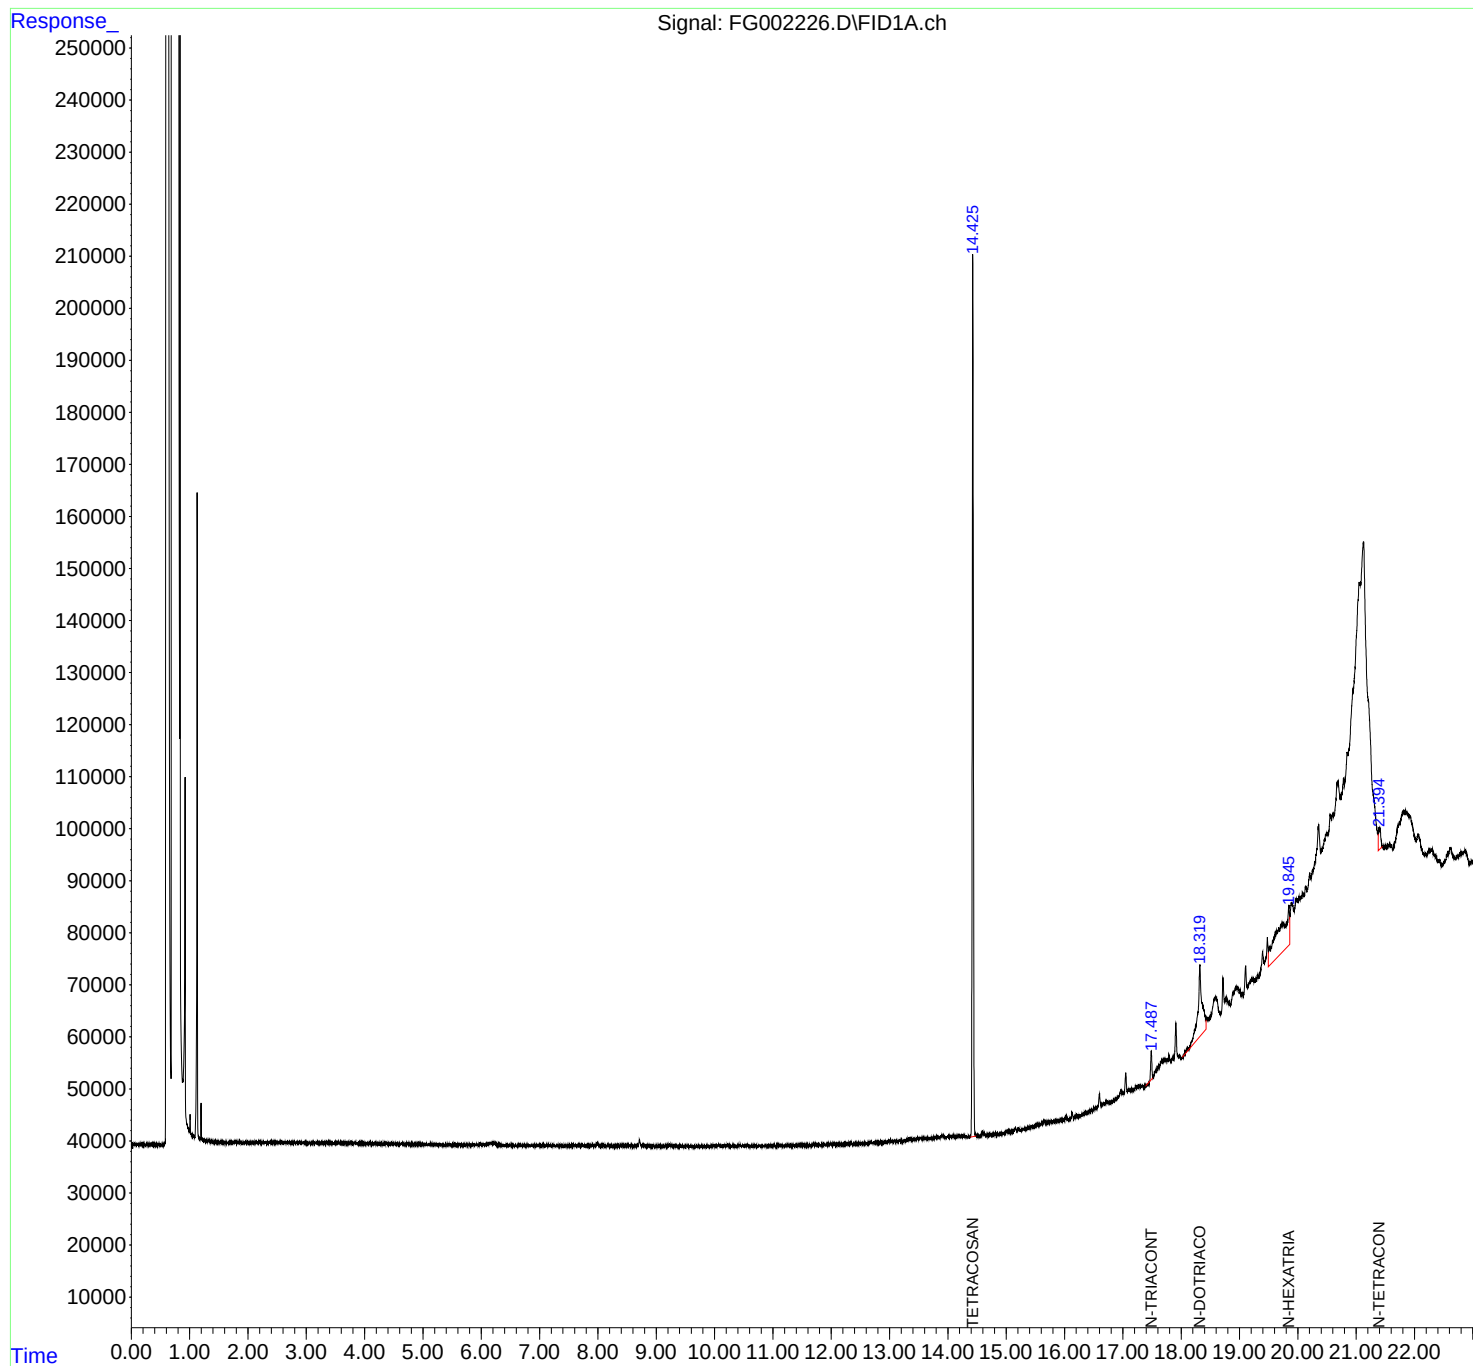


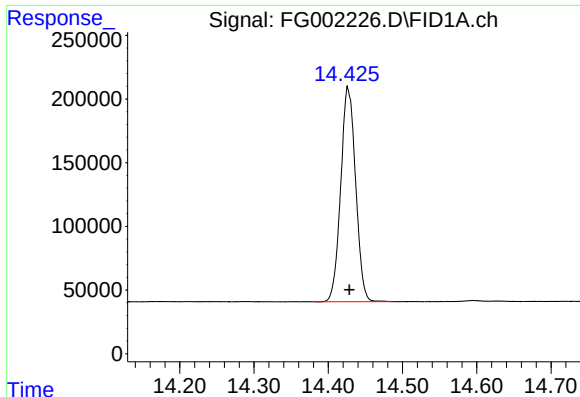

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.426 min
Delta R.T.: -0.002 min
Response: 2348973
Conc: 18.62 ug/ml

Instrument :
FID_G
ClientSampleId :

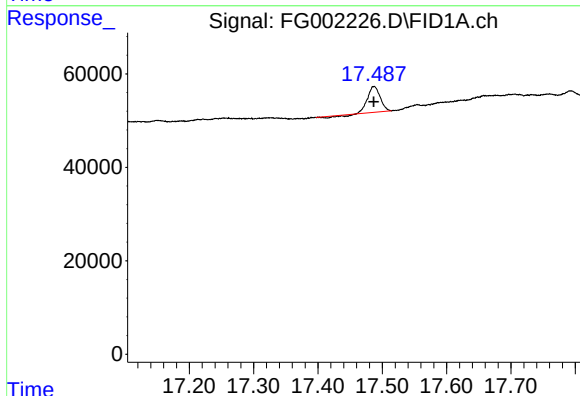


#13 N-TRIACONTANE

R.T.: 17.487 min
Delta R.T.: 0.000 min
Response: 70760
Conc: 0.47 ug/ml

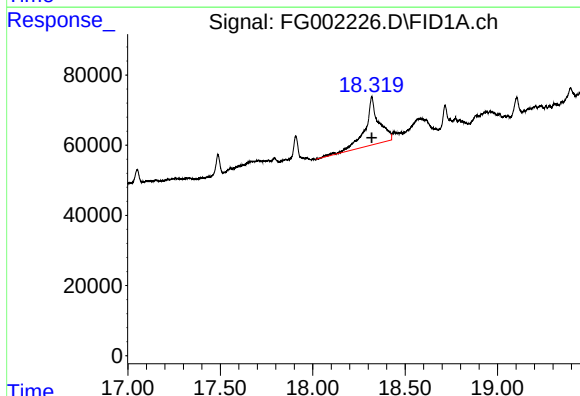


#14 N-DOTRIACONTANE

R.T.: 18.319 min
Delta R.T.: 0.000 min
Response: 722400
Conc: 4.90 ug/ml

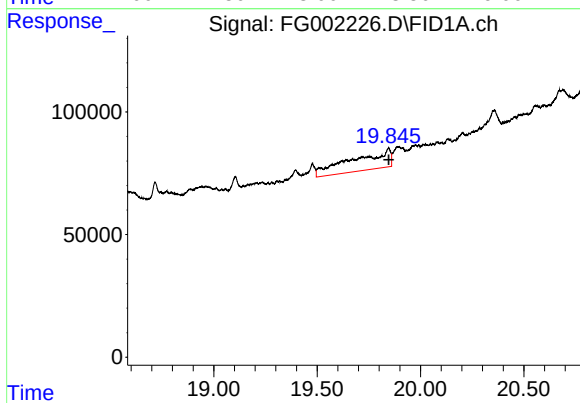

#16 N-HEXATRIACONTANE

R.T.: 19.845 min
Delta R.T.: 0.000 min
Response: 1010126
Conc: 7.88 ug/ml

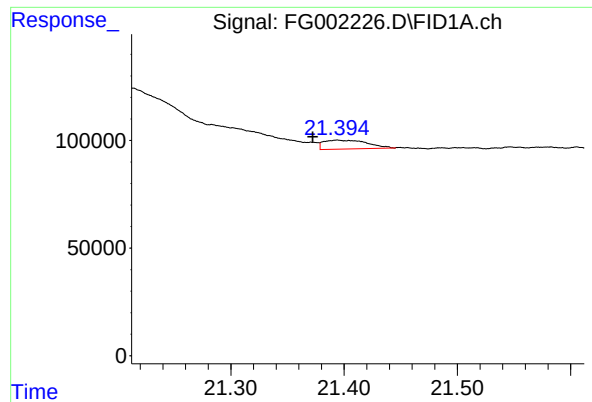

#18 N-TETRACONTANE

R.T.: 21.394 min
Delta R.T.: 0.021 min
Response: 109564
Conc: 1.01 ug/ml

Instrument :
FID_G
ClientSampleId :