

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG083118\
 Data File : FG002230.D
 Signal(s) : FID1A.ch
 Acq On : 31 Aug 2018 21:09
 Operator : AJ\SJ
 Sample : J4720-02 25X
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 31 23:28:20 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG083018.M
 Quant Title :
 QLast Update : Thu Aug 30 14:49:31 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
6) N-OCTADECANE	11.003	16868	0.120 ug/ml
7) N-EICOSANE	12.383f	866024	6.096 ug/ml
10) N-TETRACOSANE	14.607	406694	2.845 ug/ml
14) N-DOTRIACONTANE	18.318	171936	1.166 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG083118\
Data File : FG002230.D
Signal(s) : FID1A.ch
Acq On : 31 Aug 2018 21:09
Operator : AJ\SJ
Sample : J4720-02 25X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 31 23:28:20 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG083018.M
Quant Title :
QLast Update : Thu Aug 30 14:49:31 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

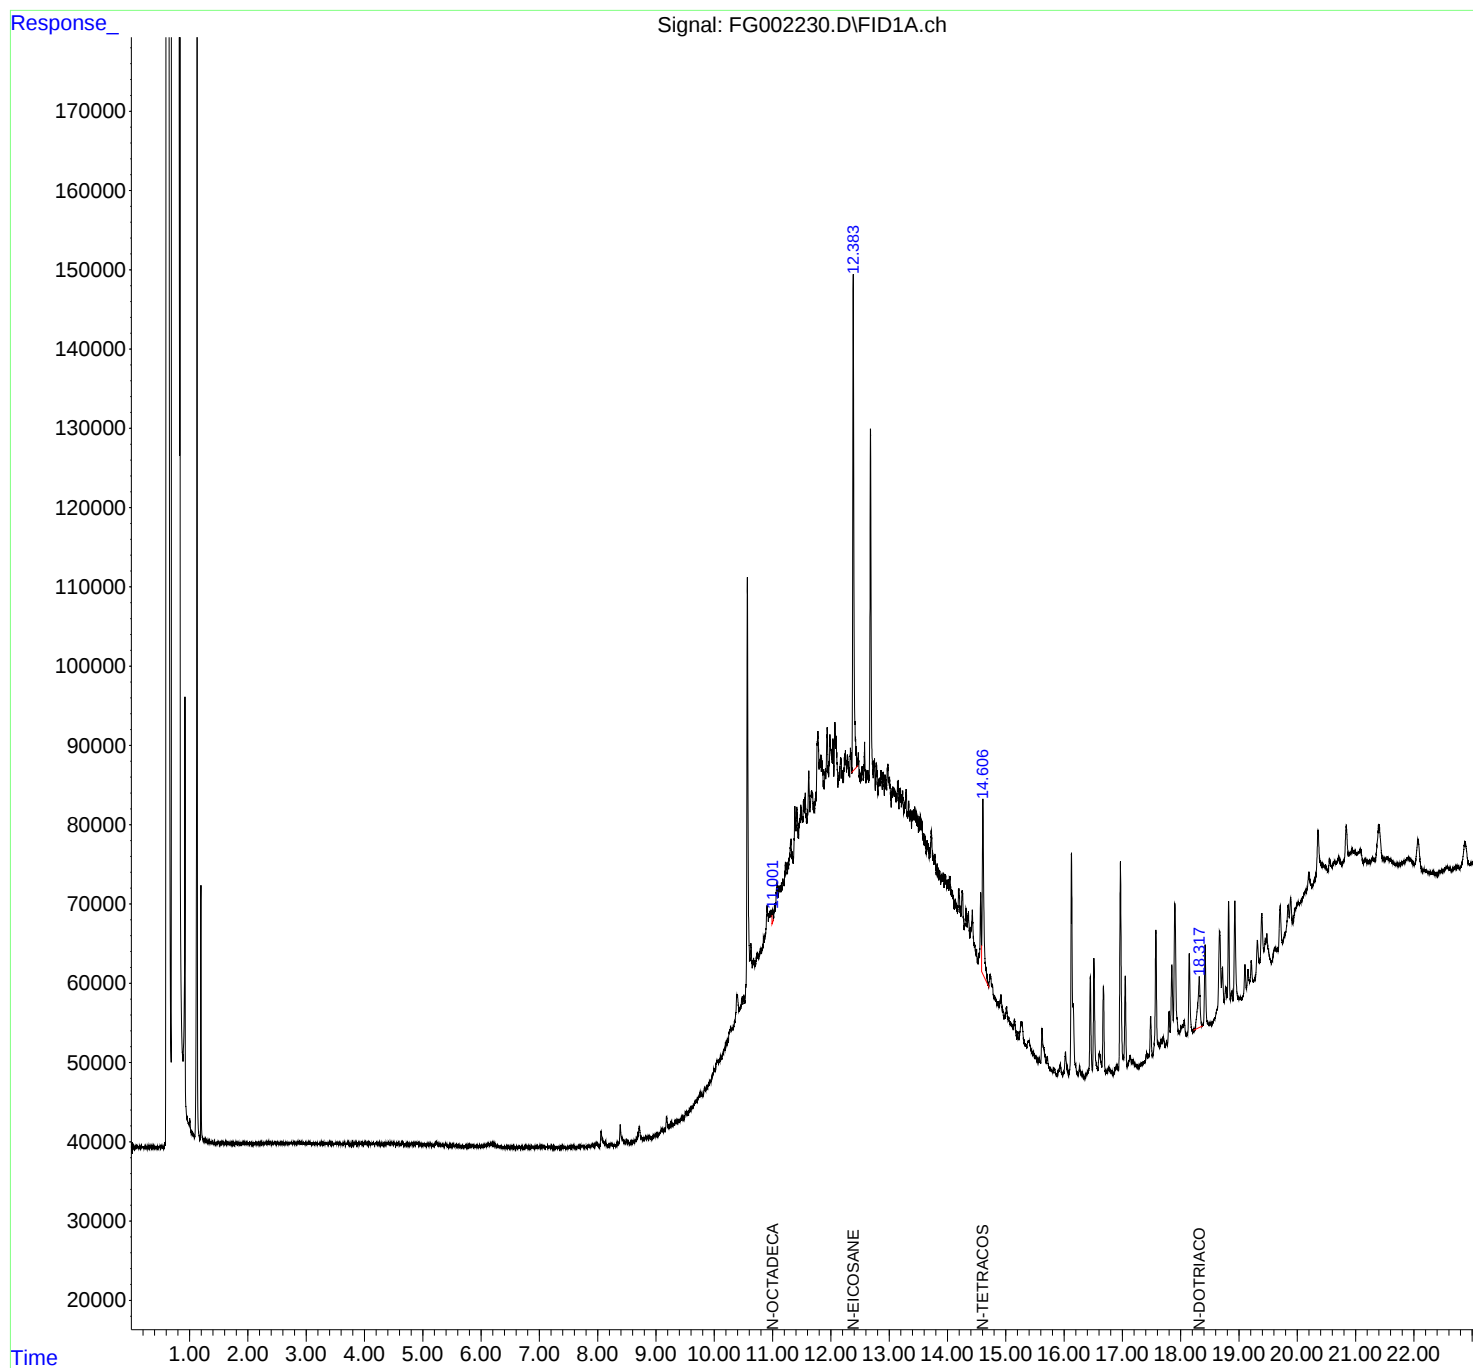


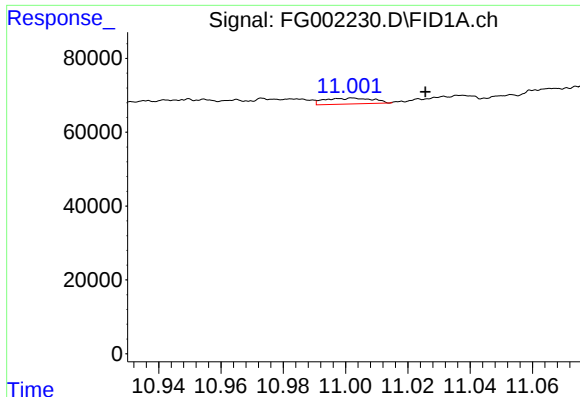

#6 N-OCTADECANE


R.T.: 11.003 min
Delta R.T.: -0.023 min
Response: 16868
Conc: 0.12 ug/ml

Instrument :
FID_G
ClientSampleId :

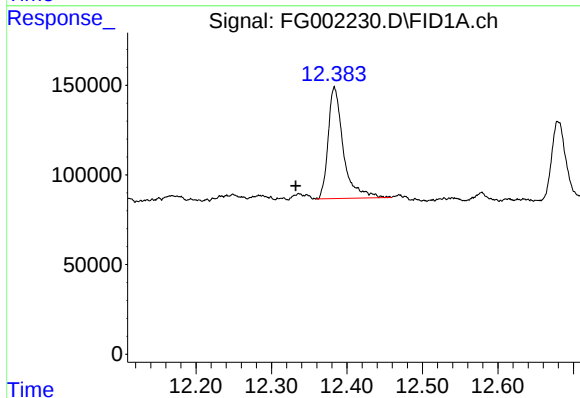


#7 N-EICOSANE

R.T.: 12.383 min
Delta R.T.: 0.051 min
Response: 866024
Conc: 6.10 ug/ml

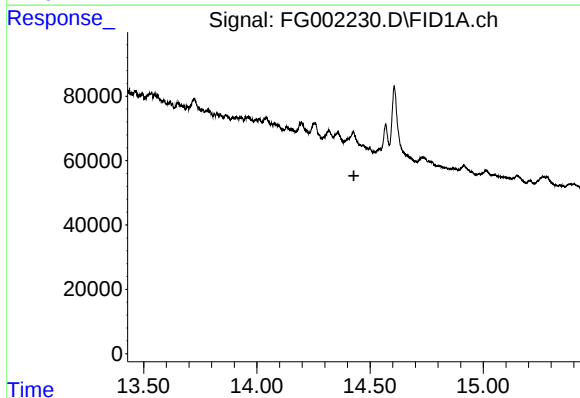


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.429 min
Response: 0
Conc: N.D.

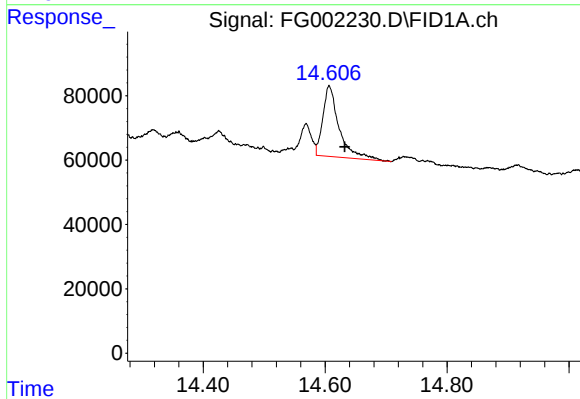

#10 N-TETRACOSANE

R.T.: 14.607 min
Delta R.T.: -0.025 min
Response: 406694
Conc: 2.84 ug/ml

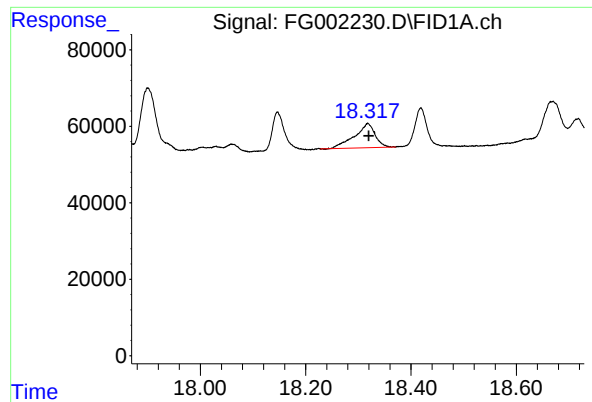

#14 N-DOTRIACONTANE

R.T.: 18.318 min
Delta R.T.: -0.002 min
Response: 171936
Conc: 1.17 ug/ml

Instrument :
FID_G
ClientSampleId :