

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG083118\
 Data File : FG002231.D
 Signal(s) : FID1A.ch
 Acq On : 31 Aug 2018 21:39
 Operator : AJ\SJ
 Sample : J4720-03 20X
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 31 23:28:28 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG083018.M
 Quant Title :
 QLast Update : Thu Aug 30 14:49:31 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.430	248923	1.973 ug/ml
Target Compounds			
7) N-EICOSANE	12.330	250031	1.760 ug/ml
8) N-DOCOSANE	13.544	457512	3.206 ug/ml
10) N-TETRACOSANE	14.601	1538040	10.758 ug/ml
11) N-HEXACOSANE	15.648	154874	1.079 ug/ml
12) N-OCTACOSANE	16.611	253998	1.736 ug/ml
13) N-TRIACONTANE	17.484	200561	1.322 ug/ml
14) N-DOTRIACONTANE	18.317	249609	1.692 ug/ml
15) N-TETRATRIACONTANE	19.104	179354	1.300 ug/ml
16) N-HEXATRIACONTANE	19.843	211177	1.647 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG083118\
Data File : FG002231.D
Signal(s) : FID1A.ch
Acq On : 31 Aug 2018 21:39
Operator : AJ\SJ
Sample : J4720-03 20X
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 31 23:28:28 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG083018.M
Quant Title :
QLast Update : Thu Aug 30 14:49:31 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

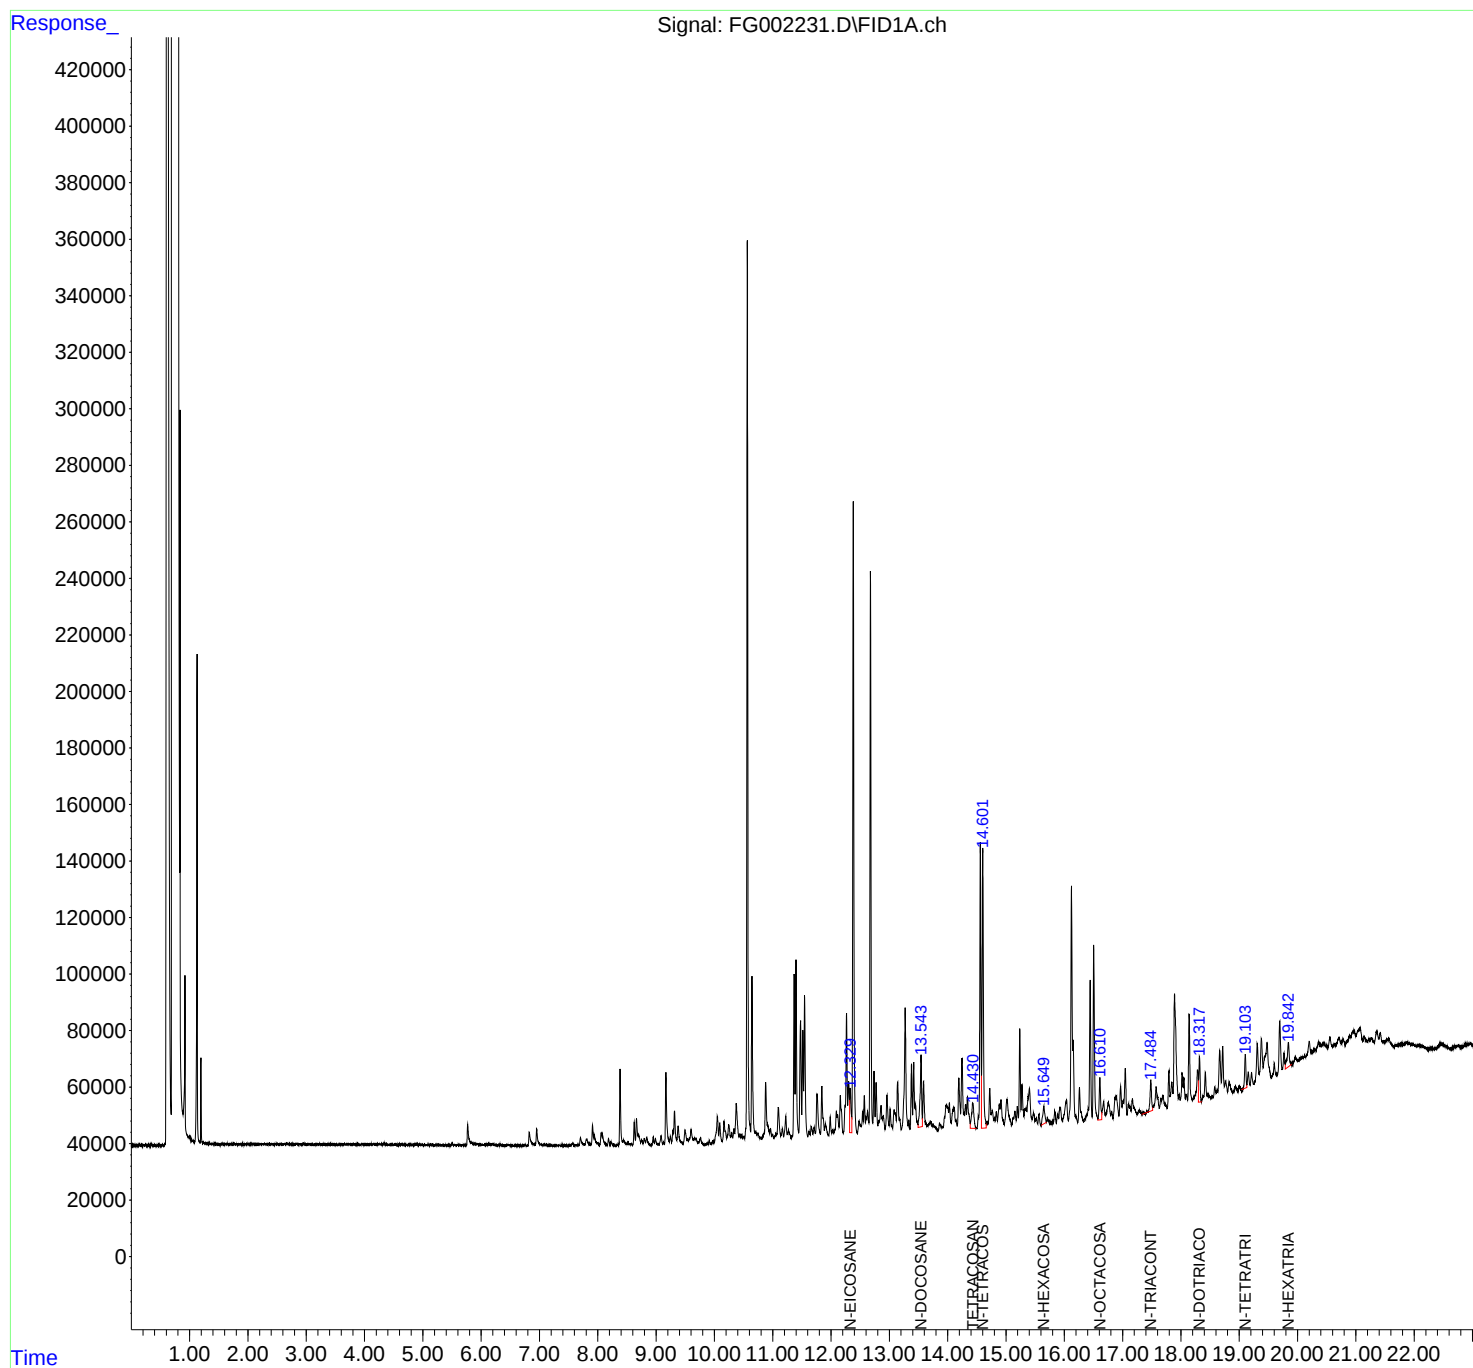


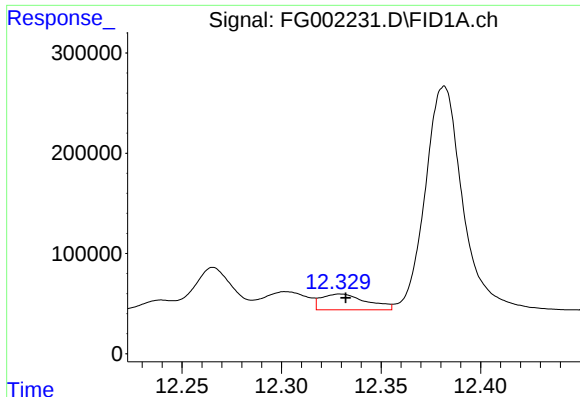

#7 N-EICOSANE


R.T.: 12.330 min
Delta R.T.: -0.003 min
Response: 250031
Conc: 1.76 ug/ml

Instrument :
FID_G
ClientSampleId :

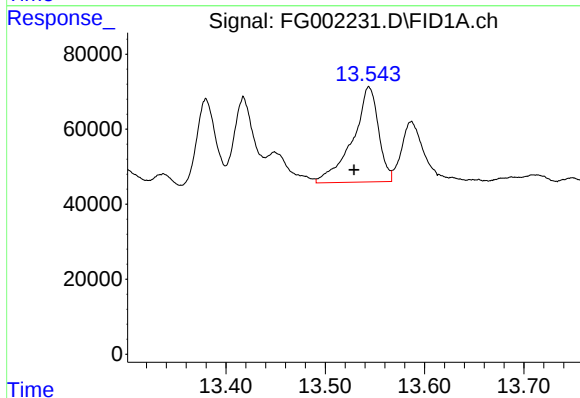


#8 N-DOCOSANE

R.T.: 13.544 min
Delta R.T.: 0.015 min
Response: 457512
Conc: 3.21 ug/ml

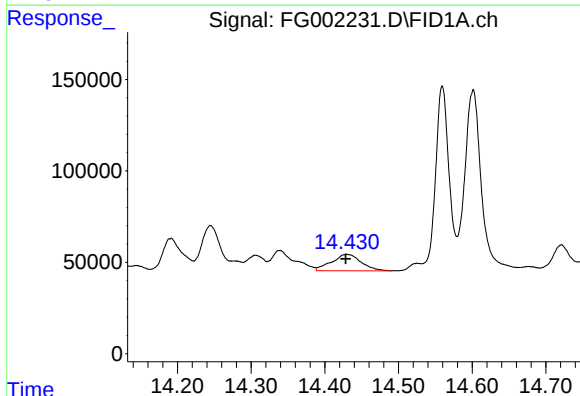


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.430 min
Delta R.T.: 0.002 min
Response: 248923
Conc: 1.97 ug/ml

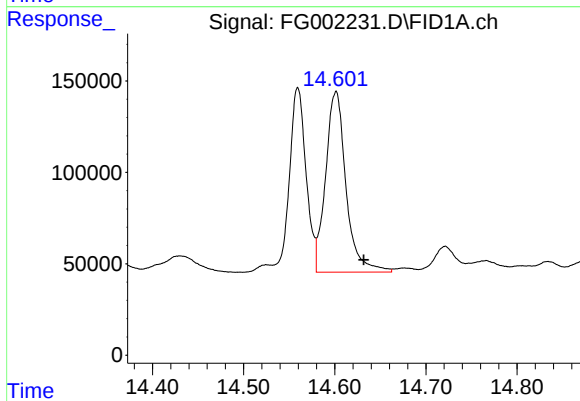

#10 N-TETRACOSANE


R.T.: 14.601 min
Delta R.T.: -0.030 min
Response: 1538040
Conc: 10.76 ug/ml

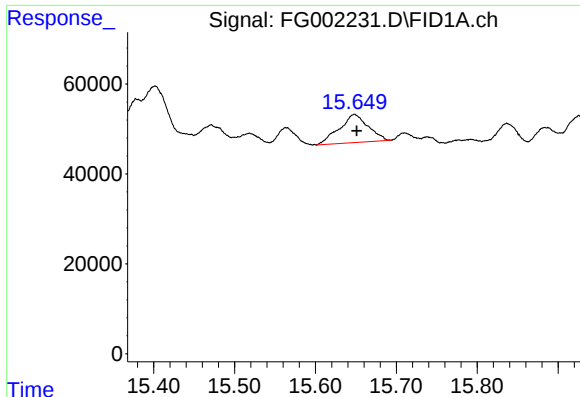

#11 N-HEXACOSANE


R.T.: 15.648 min
Delta R.T.: -0.003 min
Response: 154874
Conc: 1.08 ug/ml

Instrument :
FID_G
ClientSampleId :

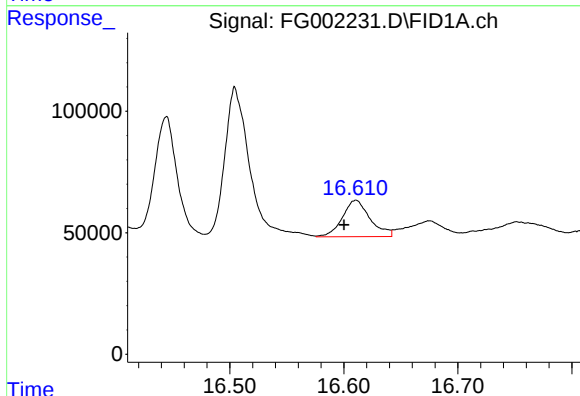


#12 N-OCTACOSANE

R.T.: 16.611 min
Delta R.T.: 0.011 min
Response: 253998
Conc: 1.74 ug/ml

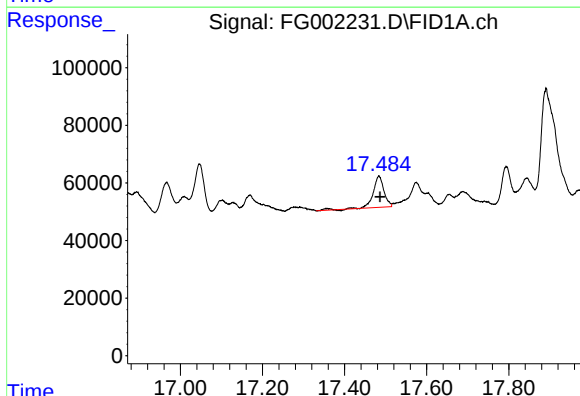


#13 N-TRIACONTANE

R.T.: 17.484 min
Delta R.T.: -0.003 min
Response: 200561
Conc: 1.32 ug/ml

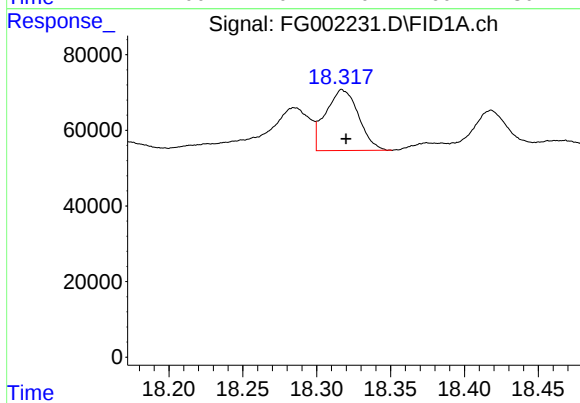

#14 N-DOTRIACONTANE


R.T.: 18.317 min
Delta R.T.: -0.003 min
Response: 249609
Conc: 1.69 ug/ml

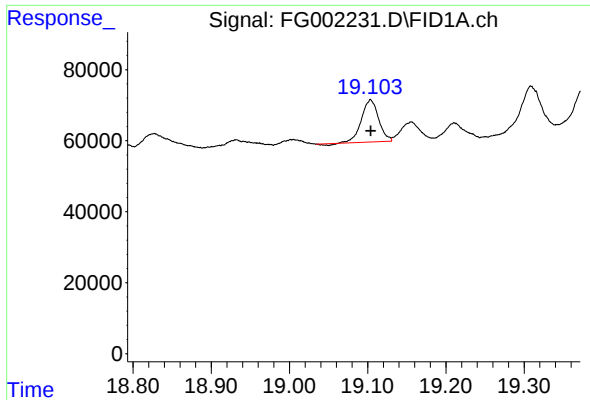

#15 N-TETRATRIACONTANE

R.T.: 19.104 min
Delta R.T.: 0.000 min
Response: 179354
Conc: 1.30 ug/ml

Instrument :
FID_G
ClientSampleId :

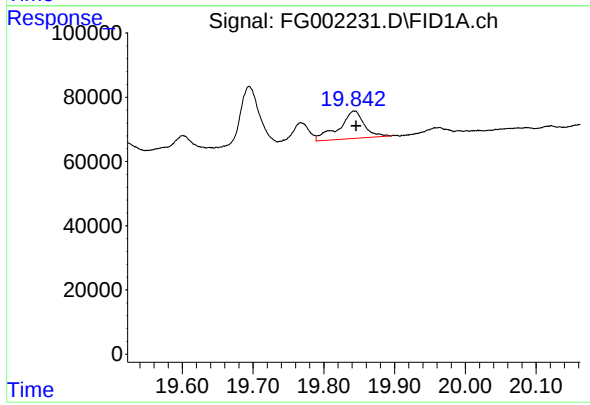

#16 N-HEXATRIACONTANE

R.T.: 19.843 min
Delta R.T.: -0.002 min
Response: 211177
Conc: 1.65 ug/ml