

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG083118\
 Data File : FG002219.D
 Signal(s) : FID1A.ch
 Acq On : 31 Aug 2018 15:37
 Operator : AJ\SJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: Sample.e
 Quant Time: Aug 31 23:26:07 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG083018.M
 Quant Title :
 QLast Update : Thu Aug 30 14:49:31 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.429	6063690	48.062 ug/ml
Target Compounds			
2) N-DECANE	4.189	6315217	52.612 ug/ml
3) N-DODECANE	6.201	6545206	52.009 ug/ml
4) N-TETRADECANE	7.991	6732351	51.283 ug/ml
5) N-HEXADECANE	9.588	6865193	50.437 ug/ml
6) N-OCTADECANE	11.026	6958251	49.537 ug/ml
7) N-EICOSANE	12.333	6937289	48.831 ug/ml
8) N-DOCOSANE	13.530	6891297	48.286 ug/ml
10) N-TETRACOSANE	14.632	6822390	47.722 ug/ml
11) N-HEXACOSANE	15.653	6767454	47.135 ug/ml
12) N-OCTACOSANE	16.602	6685555	45.694 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG083118\
Data File : FG002219.D
Signal(s) : FID1A.ch
Acq On : 31 Aug 2018 15:37
Operator : AJ\SJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: Sample.e
Quant Time: Aug 31 23:26:07 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG083018.M
Quant Title :
QLast Update : Thu Aug 30 14:49:31 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

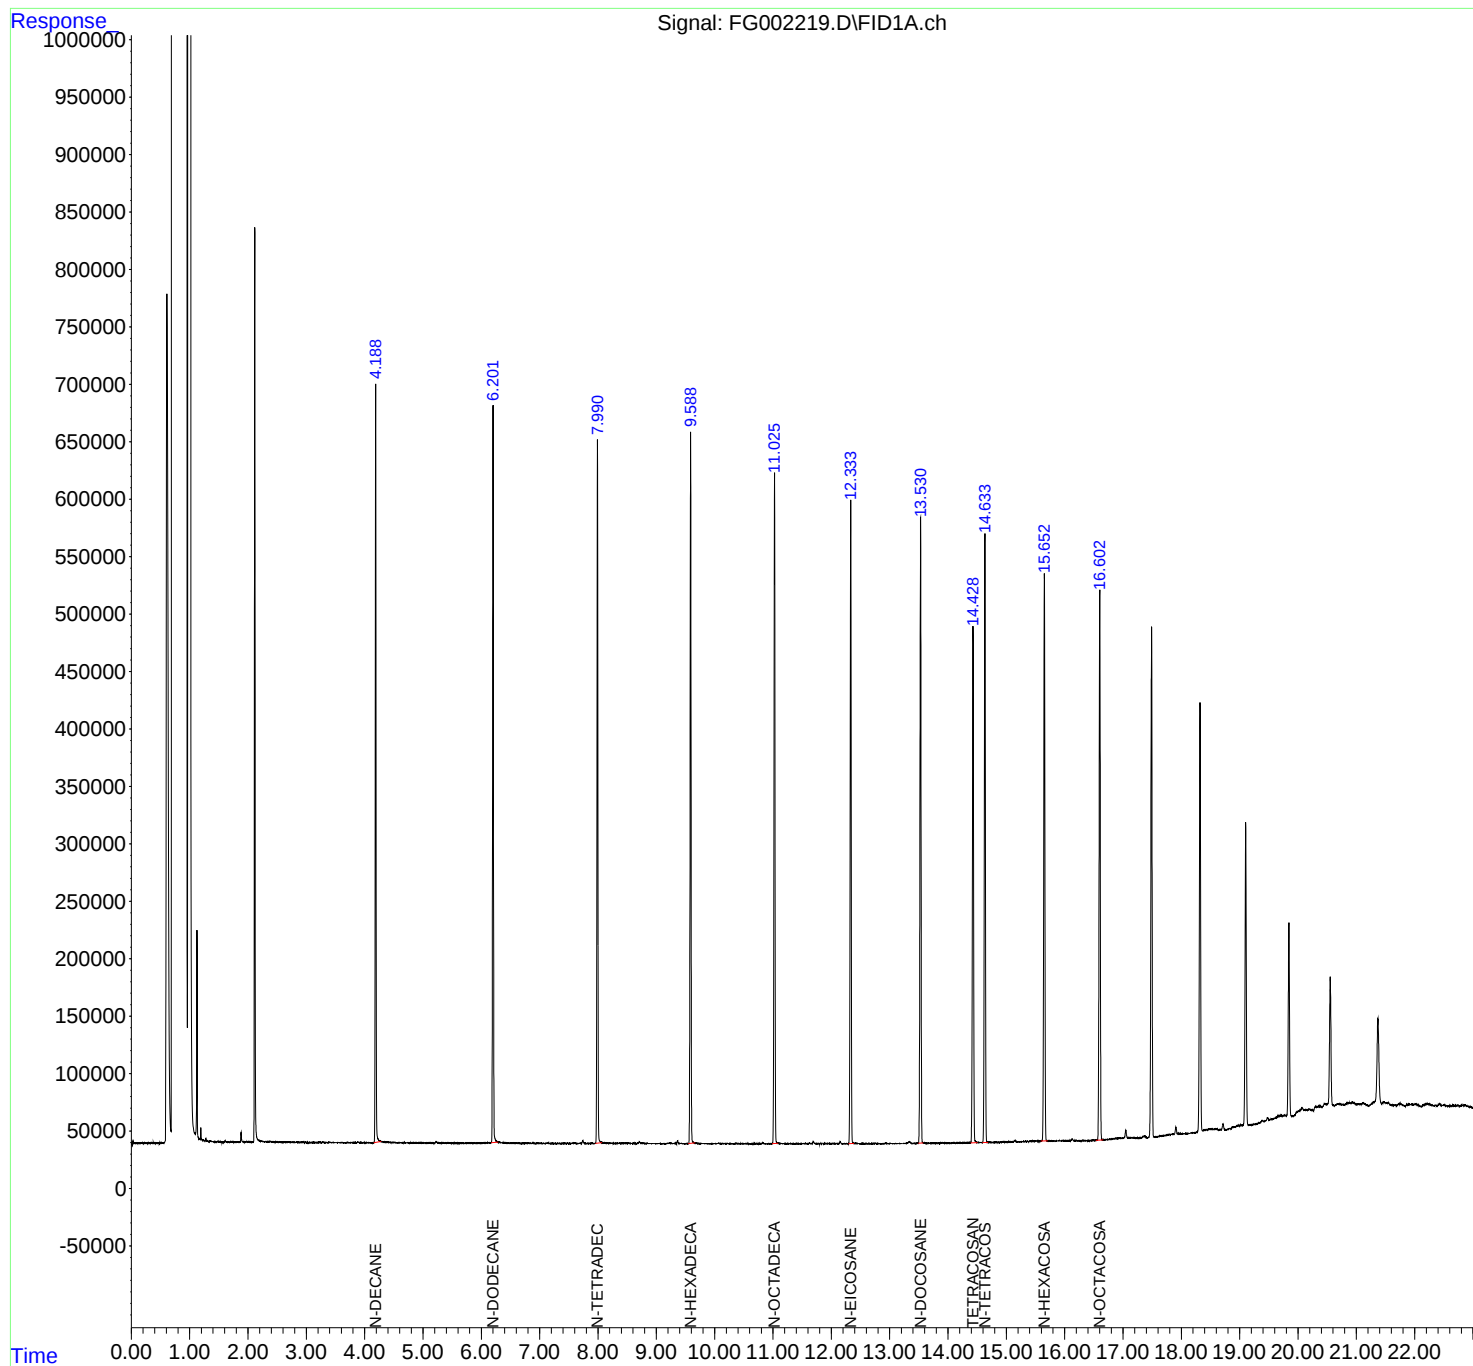


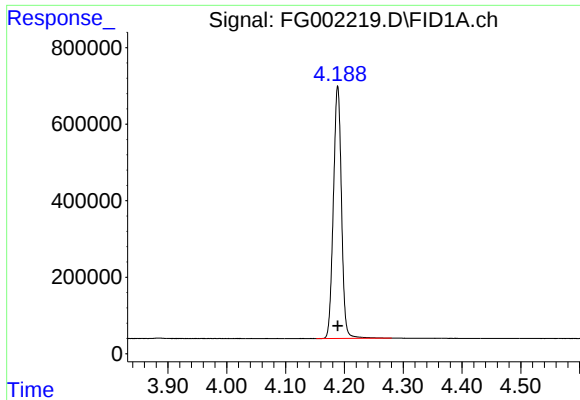

#2 N-DECANE


R.T.: 4.189 min
Delta R.T.: 0.000 min
Response: 6315217
Conc: 52.61 ug/ml

Instrument :
FID_G
ClientSampleId :

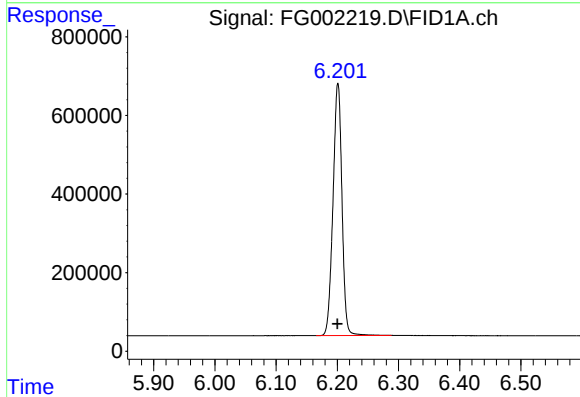


#3 N-DODECANE

R.T.: 6.201 min
Delta R.T.: 0.000 min
Response: 6545206
Conc: 52.01 ug/ml

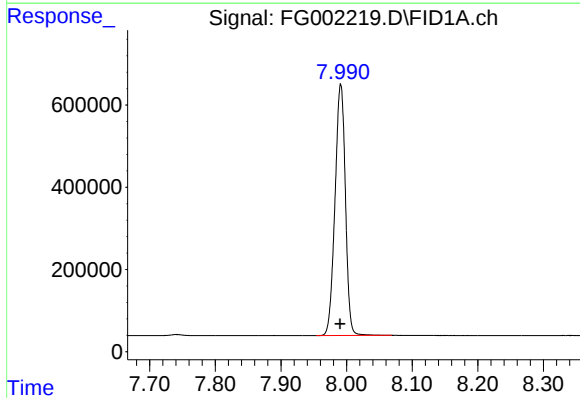


#4 N-TETRADECANE

R.T.: 7.991 min
Delta R.T.: 0.001 min
Response: 6732351
Conc: 51.28 ug/ml

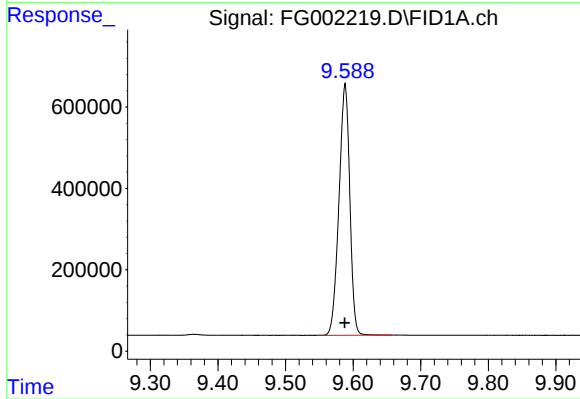

#5 N-HEXADECANE


R.T.: 9.588 min
Delta R.T.: 0.000 min
Response: 6865193
Conc: 50.44 ug/ml

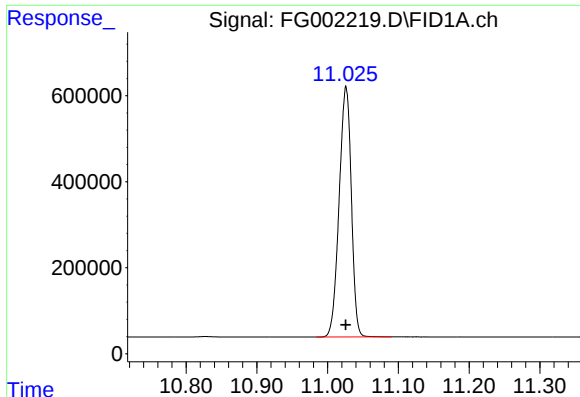

#6 N-OCTADECANE


R.T.: 11.026 min
Delta R.T.: 0.000 min
Response: 6958251
Conc: 49.54 ug/ml

Instrument :
FID_G
ClientSampleId :

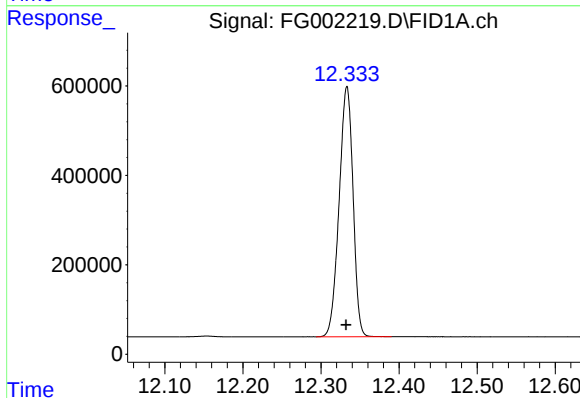


#7 N-EICOSANE

R.T.: 12.333 min
Delta R.T.: 0.001 min
Response: 6937289
Conc: 48.83 ug/ml

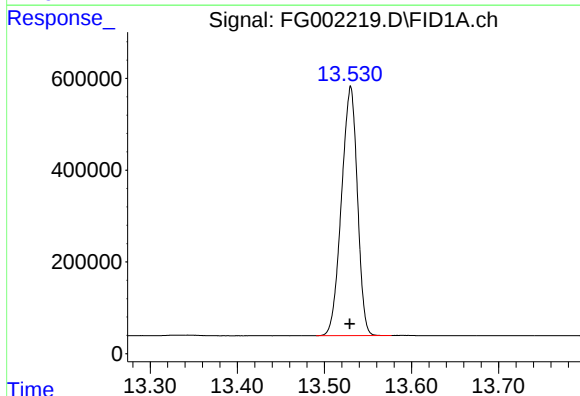


#8 N-DOCOSANE

R.T.: 13.530 min
Delta R.T.: 0.000 min
Response: 6891297
Conc: 48.29 ug/ml

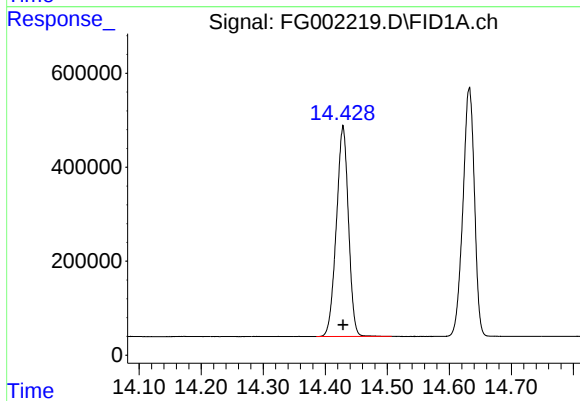

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.429 min
Delta R.T.: 0.000 min
Response: 6063690
Conc: 48.06 ug/ml

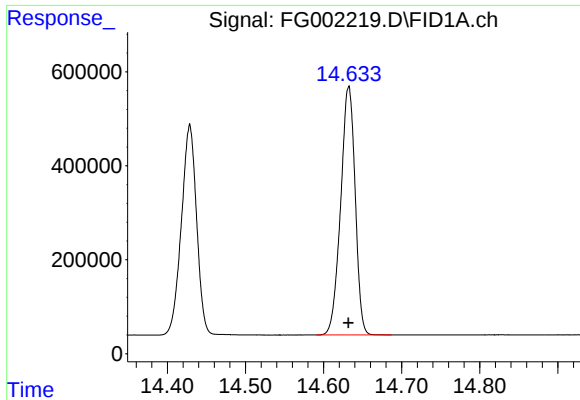

#10 N-TETRACOSANE


R.T.: 14.632 min
Delta R.T.: 0.000 min
Response: 6822390
Conc: 47.72 ug/ml

Instrument :
FID_G
ClientSampleId :

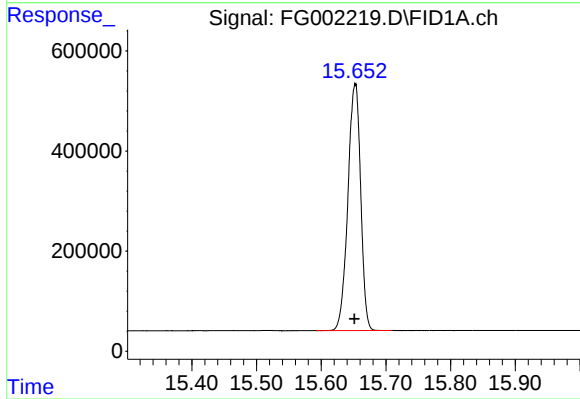

#11 N-HEXACOSANE

R.T.: 15.653 min
Delta R.T.: 0.001 min
Response: 6767454
Conc: 47.14 ug/ml

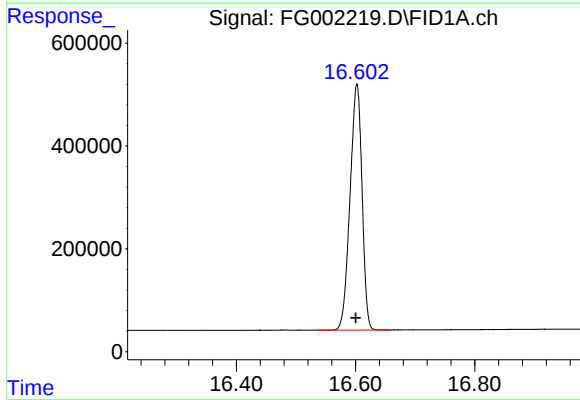

#12 N-OCTACOSANE

R.T.: 16.602 min
Delta R.T.: 0.002 min
Response: 6685555
Conc: 45.69 ug/ml