

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG083118\
Data File : FG002230.D
Signal(s) : FID1A.ch
Acq On : 31 Aug 2018 21:39
Operator : AJ\SJ
Sample : J4720-03 20X
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
BZTRANS-3

Integration File: Sample.e
Quant Time: Aug 31 23:28:28 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG083018.M
Quant Title :
QLast Update : Thu Aug 30 14:49:31 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.430	248923	1.973 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG083118\
Data File : FG002230.D
Signal(s) : FID1A.ch
Acq On : 31 Aug 2018 21:39
Operator : AJ\SJ
Sample : J4720-03 20X
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
BZTRANS-3

Integration File: Sample.e
Quant Time: Aug 31 23:28:28 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG083018.M
Quant Title :
QLast Update : Thu Aug 30 14:49:31 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

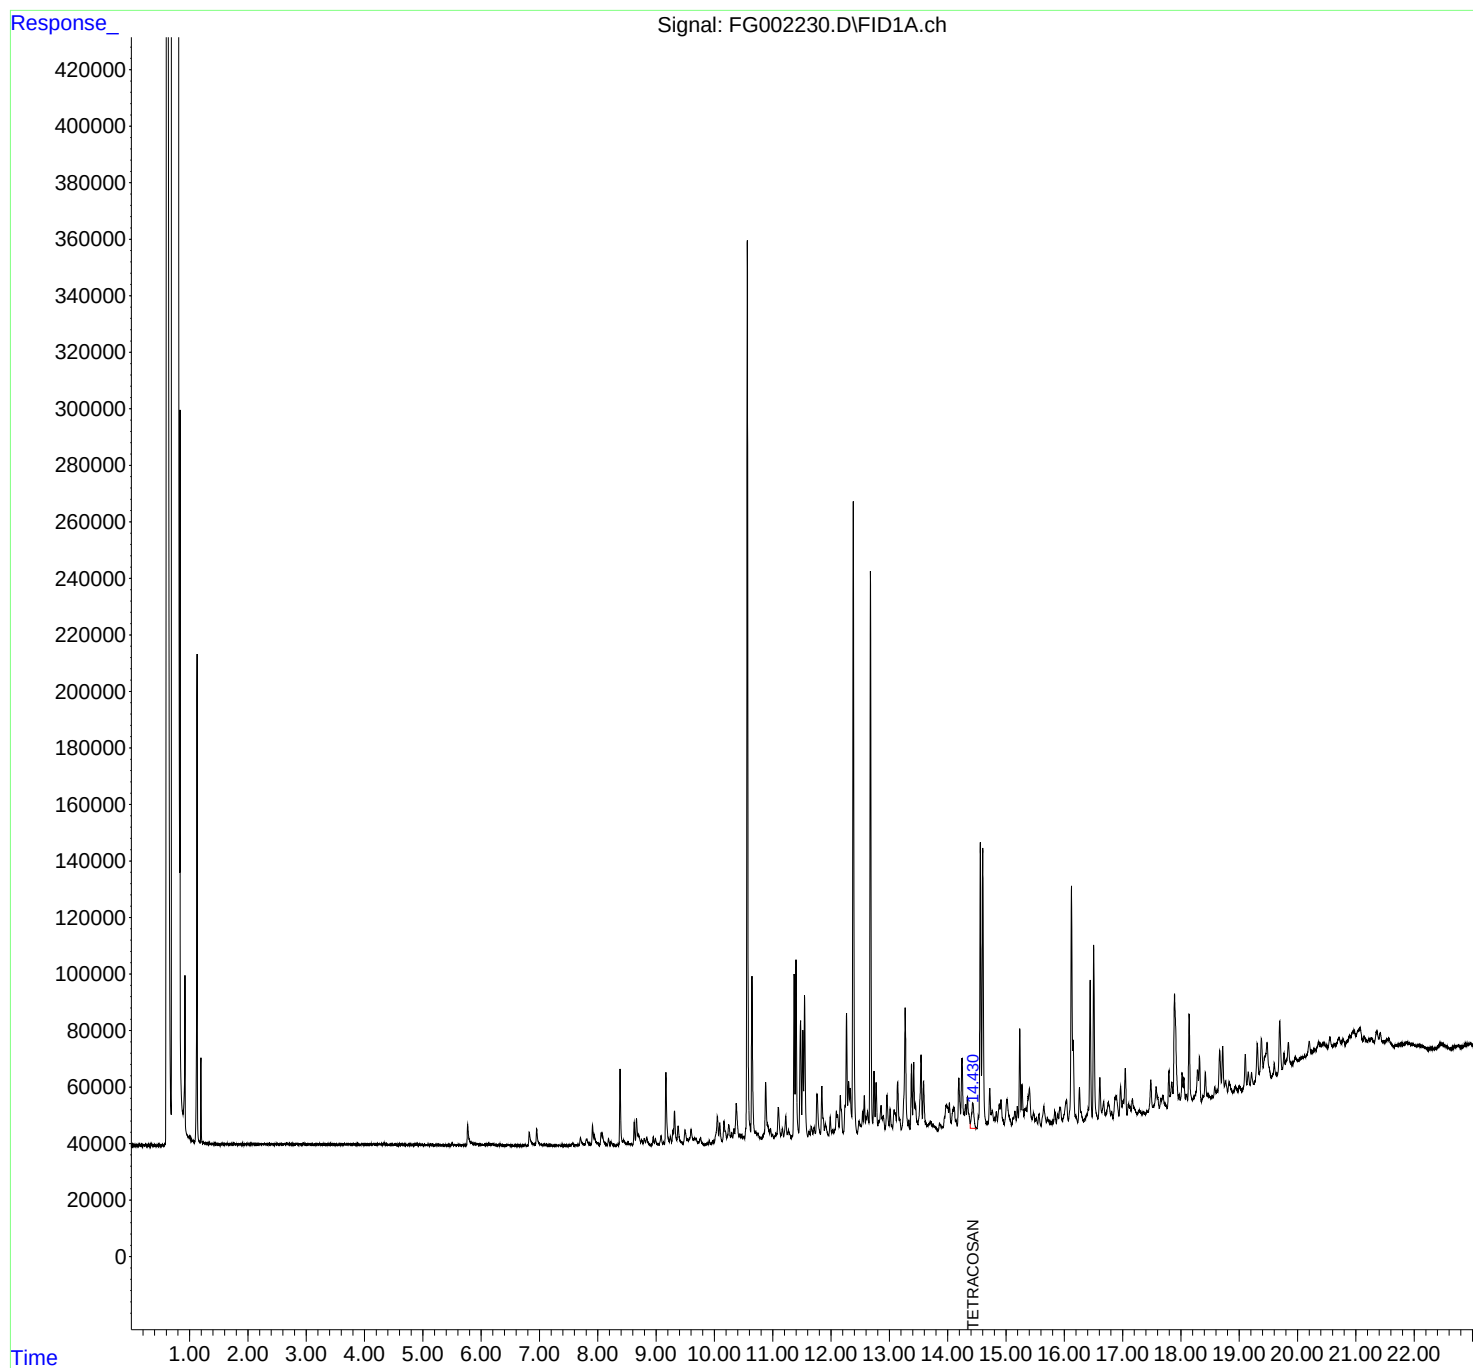

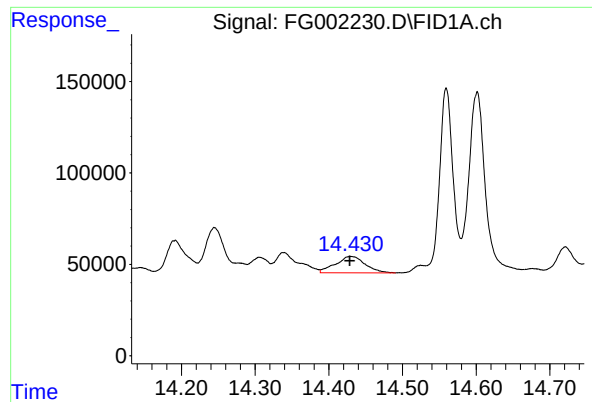

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.430 min
Delta R.T.: 0.002 min
Response: 248923
Conc: 1.97 ug/ml

Instrument :
FID_G
ClientSampleId :
BZTRANS-3