

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG083123\
Data File : FG012839.D
Signal(s) : FID1A.ch
Acq On : 31 Aug 2023 08:25
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 01 00:14:53 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG080223.M
Quant Title :
QLast Update : Wed Aug 02 18:57:31 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
15) N-TETRATRIACONTANE	19.769	42719	0.451 ug/ml
16) N-HEXATRIACONTANE	20.508	4624	0.057 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG083123\
Data File : FG012839.D
Signal(s) : FID1A.ch
Acq On : 31 Aug 2023 08:25
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 01 00:14:53 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG080223.M
Quant Title :
QLast Update : Wed Aug 02 18:57:31 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

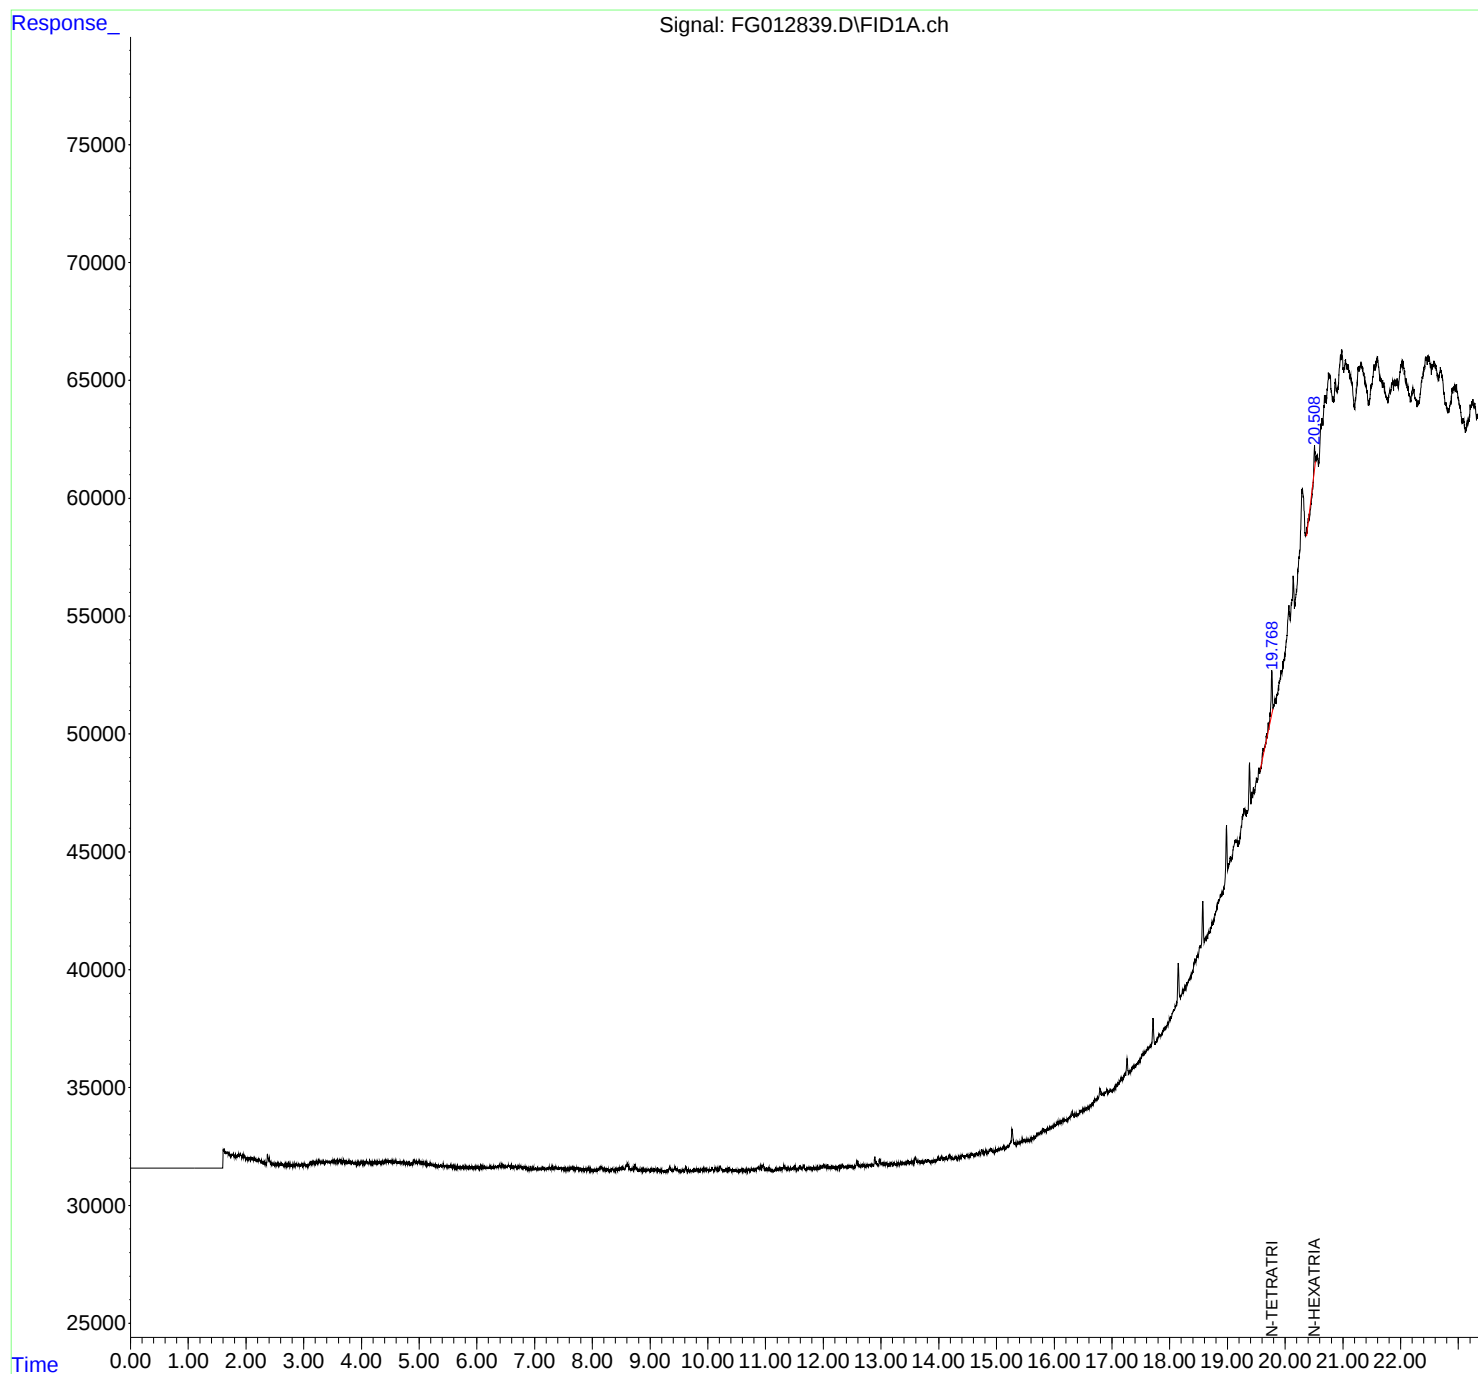


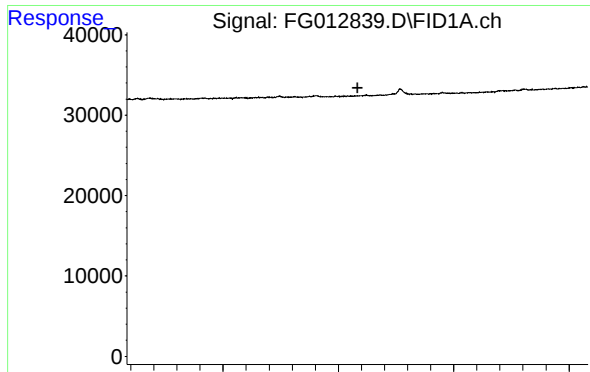

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 15.083 min
Response: 0
Conc: N.D.

Instrument :
FID_G
ClientSampleId :

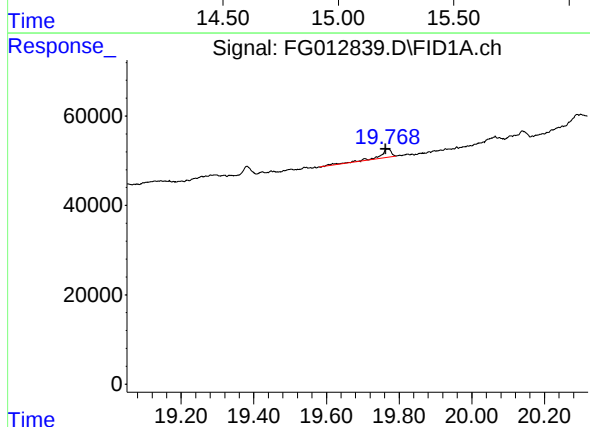

#15 N-TETRATRIACONTANE

R.T.: 19.769 min
Delta R.T.: 0.005 min
Response: 42719
Conc: 0.45 ug/ml

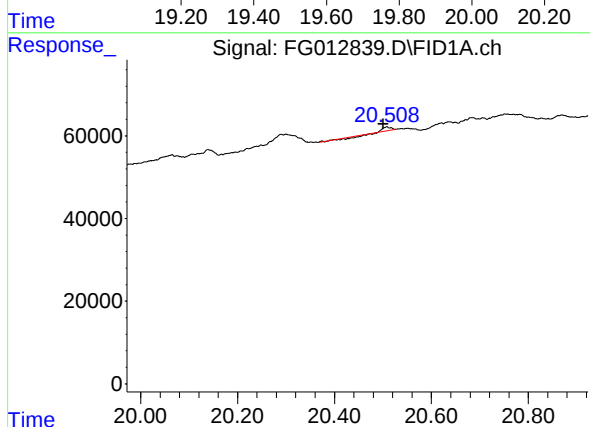

#16 N-HEXATRIACONTANE

R.T.: 20.508 min
Delta R.T.: 0.007 min
Response: 4624
Conc: 0.06 ug/ml