

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG083123\
Data File : FG012840.D
Signal(s) : FID1A.ch
Acq On : 31 Aug 2023 08:55
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
I.BLK

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/01/2023
Supervised By :mohammad ahmed 09/01/2023

Integration File: autoint1.e
Quant Time: Sep 01 00:15:01 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG080223.M
Quant Title :
QLast Update : Wed Aug 02 18:57:31 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.082	1986589	17.759 ug/mlm
Target Compounds			

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG083123\
Data File : FG012840.D
Signal(s) : FID1A.ch
Acq On : 31 Aug 2023 08:55
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1


Instrument :
FID_G
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/01/2023
Supervised By :mohammad ahmed 09/01/2023

Integration File: autoint1.e
Quant Time: Sep 01 00:15:01 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG080223.M
Quant Title :
QLast Update : Wed Aug 02 18:57:31 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

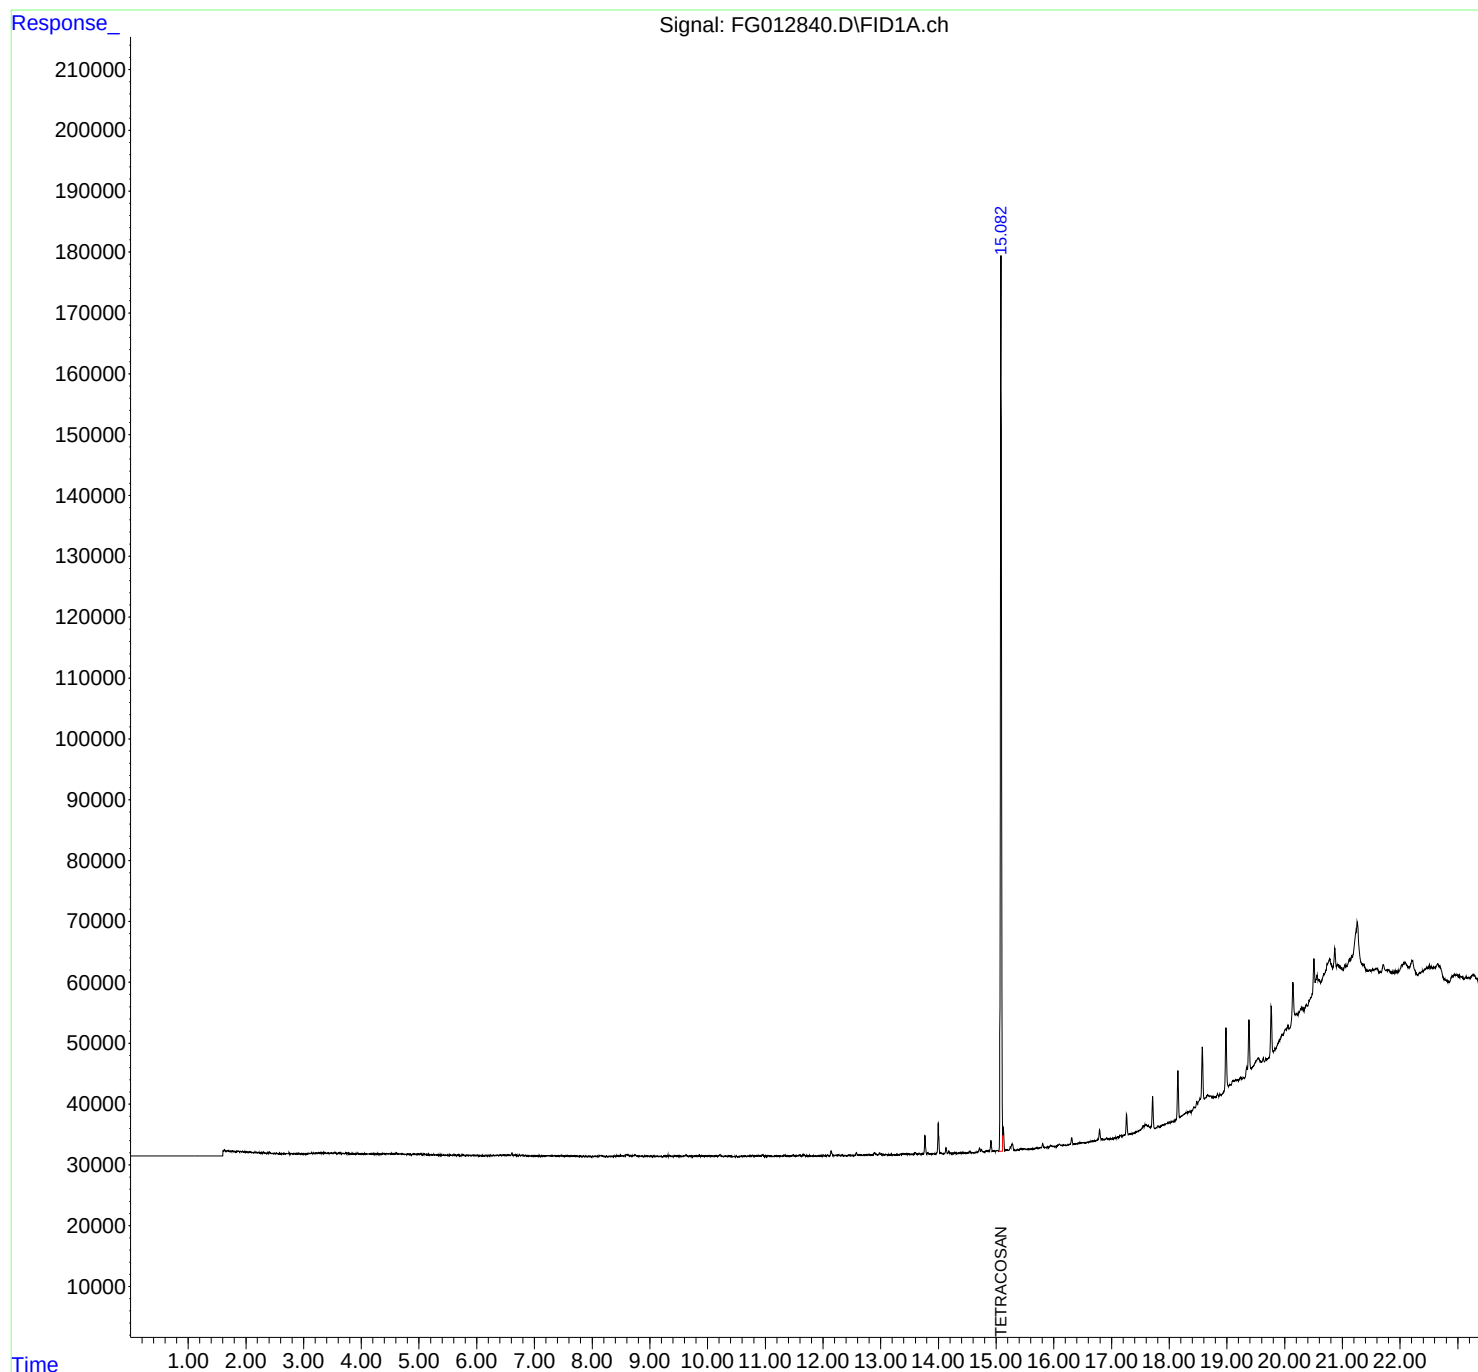

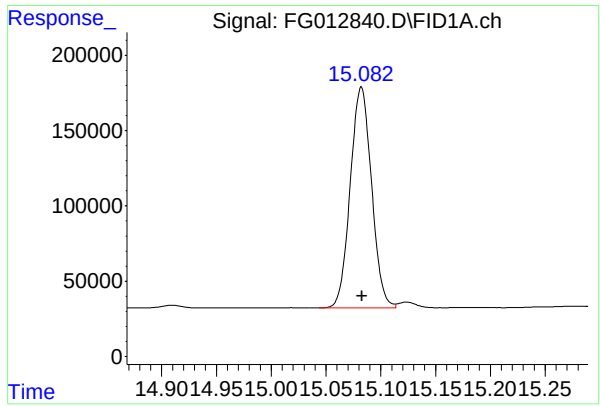

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.082 min
Delta R.T.: 0.000 min
Response: 1986589
Conc: 17.76 ug/ml

Instrument :

FID_G

ClientSampleId :

I.BLK

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 09/01/2023

Supervised By :mohammad ahmed 09/01/2023