

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG090122\
Data File : FG010473.D
Signal(s) : FID1A.ch
Acq On : 01 Sep 2022 12:59
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 02 03:04:02 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG082622.M
Quant Title :
QLast Update : Fri Aug 26 23:48:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.494	2678605	20.353 ug/ml
12)	N-OCTACOSANE	16.960	2658962	20.106 ug/ml
13)	N-TRIACONTANE	17.849	90385	0.698 ug/ml
14)	N-DOTRIACONTANE	18.682	125227	0.979 ug/ml
15)	N-TETRATRIACONTANE	19.464	115120	0.931 ug/ml
16)	N-HEXATRIACONTANE	20.207	83212	0.717 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG090122\
Data File : FG010473.D
Signal(s) : FID1A.ch
Acq On : 01 Sep 2022 12:59
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 02 03:04:02 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG082622.M
Quant Title :
QLast Update : Fri Aug 26 23:48:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

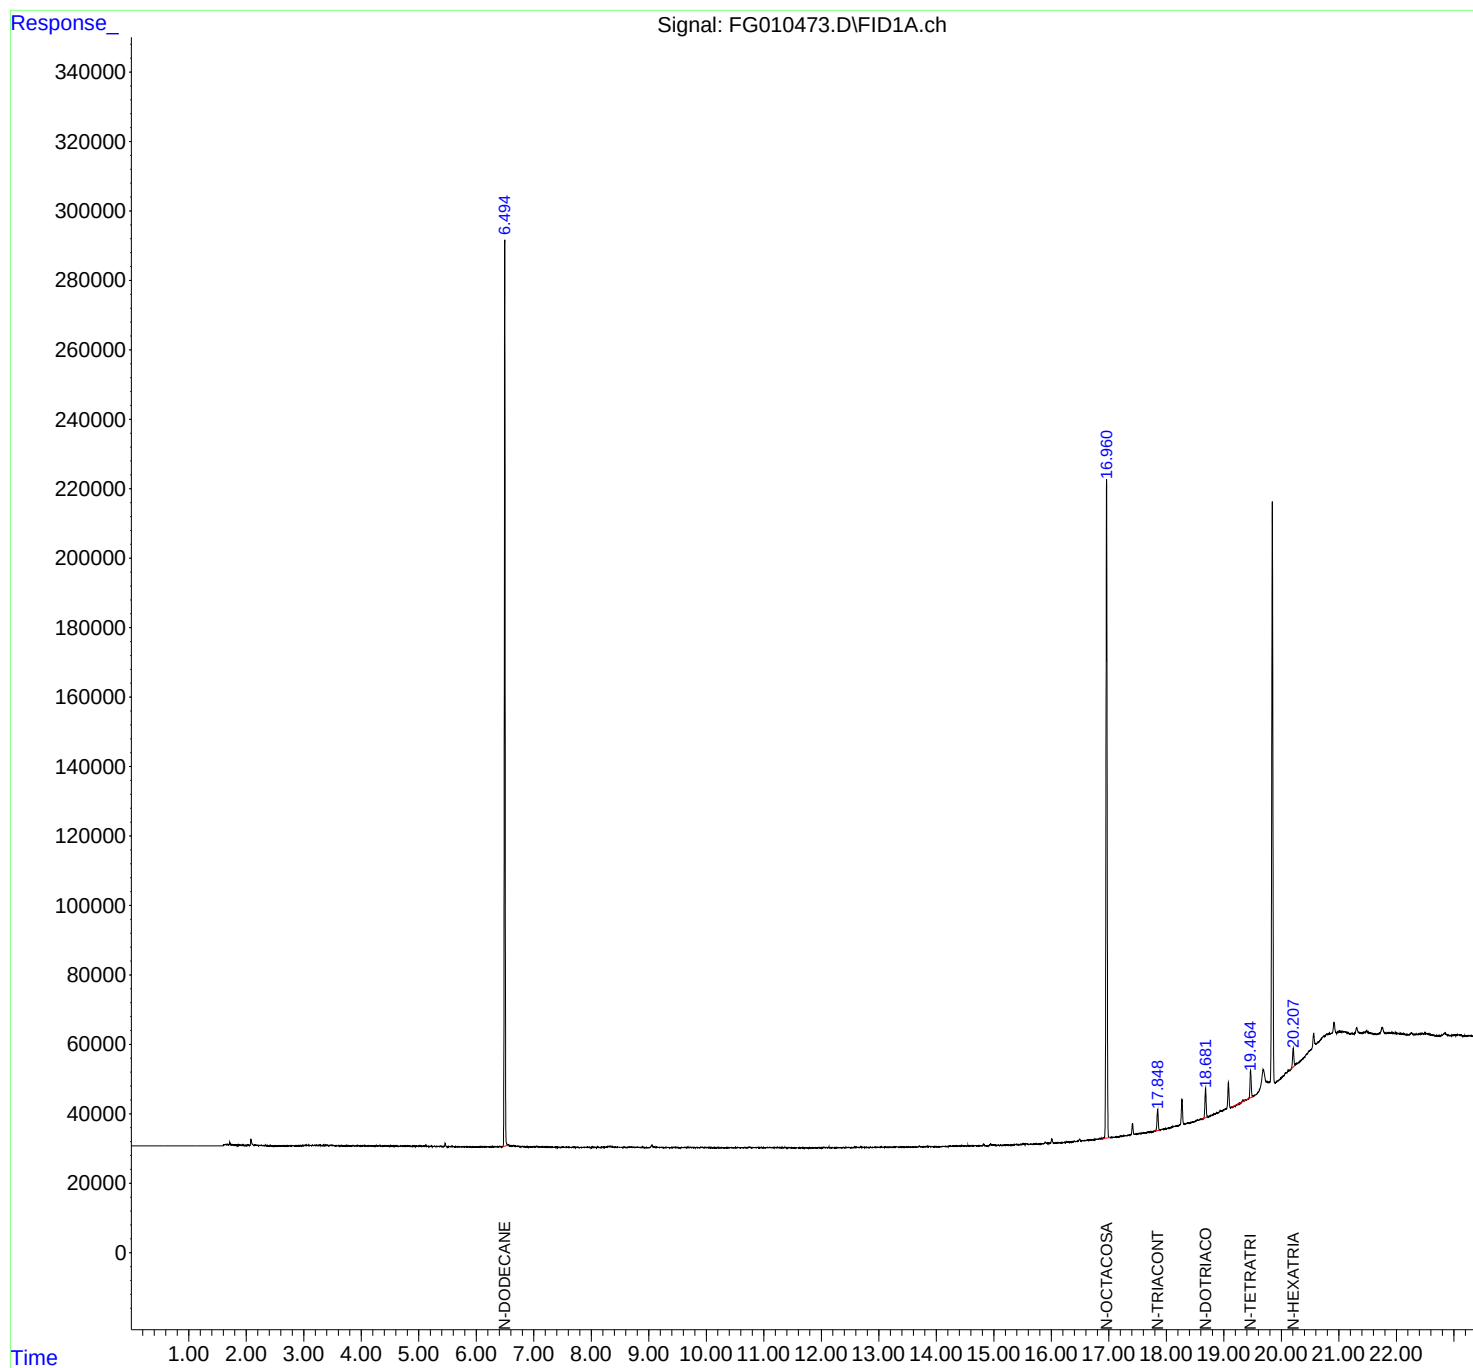


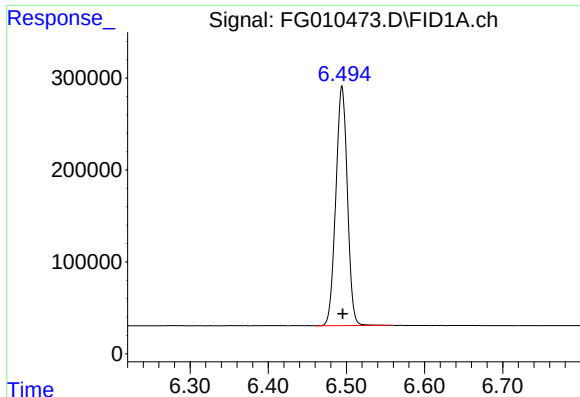

#3 N-DODECANE


R.T.: 6.494 min
Delta R.T.: 0.000 min
Response: 2678605
Conc: 20.35 ug/ml

Instrument :
FID_G
ClientSampleId :

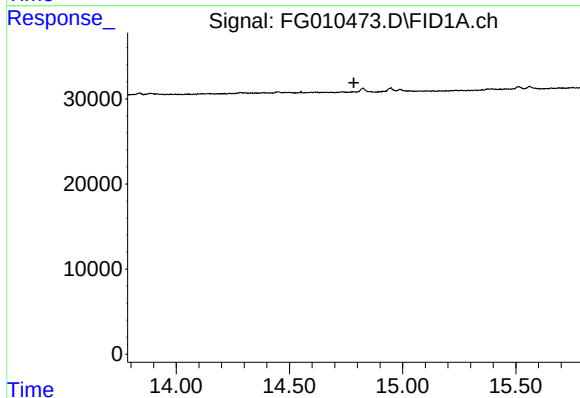


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.785 min
Response: 0
Conc: N.D.

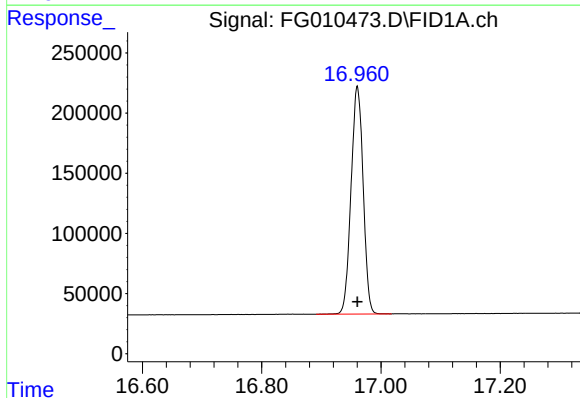


#12 N-OCTACOSANE

R.T.: 16.960 min
Delta R.T.: 0.000 min
Response: 2658962
Conc: 20.11 ug/ml

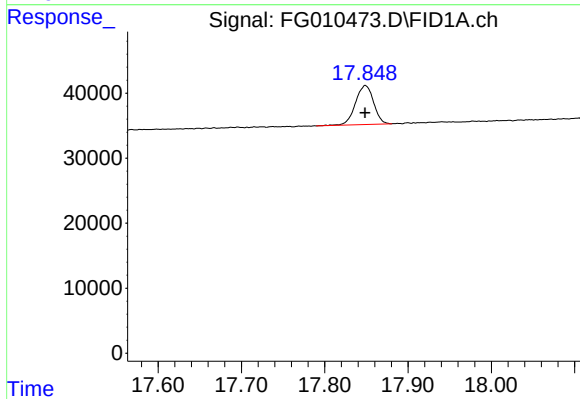

#13 N-TRIACONTANE


R.T.: 17.849 min
Delta R.T.: 0.000 min
Response: 90385
Conc: 0.70 ug/ml

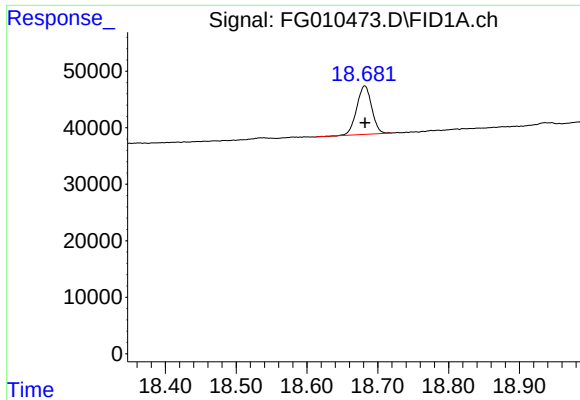

#14 N-DOTRIACONTANE


R.T.: 18.682 min
Delta R.T.: 0.000 min
Response: 125227
Conc: 0.98 ug/ml

Instrument :
FID_G
ClientSampleId :

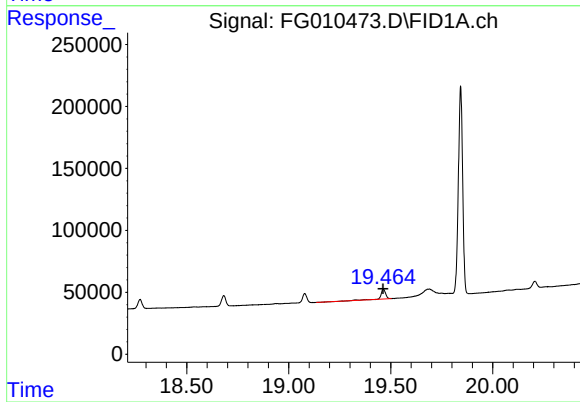

#15 N-TETRATRIACONTANE

R.T.: 19.464 min
Delta R.T.: 0.000 min
Response: 115120
Conc: 0.93 ug/ml

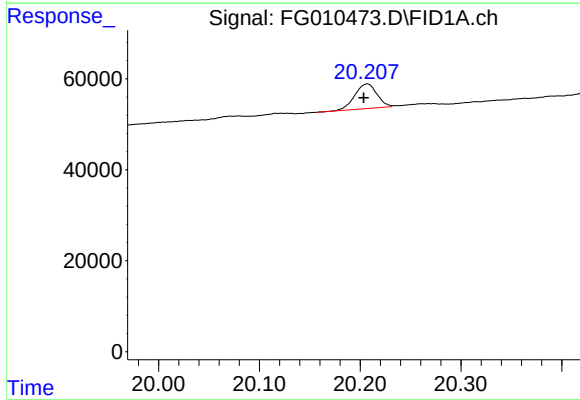

#16 N-HEXATRIACONTANE

R.T.: 20.207 min
Delta R.T.: 0.003 min
Response: 83212
Conc: 0.72 ug/ml