

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG090122\
 Data File : FG010474.D
 Signal(s) : FID1A.ch
 Acq On : 01 Sep 2022 14:26
 Operator : YP\AJ
 Sample : PB147413BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Sep 02 03:04:11 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG082622.M
 Quant Title :
 QLast Update : Fri Aug 26 23:48:05 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.788	2275814	18.596 ug/ml
Target Compounds			
13) N-TRIACONTANE	17.851	49065	0.379 ug/ml
14) N-DOTRIACONTANE	18.683	62266	0.487 ug/ml
15) N-TETRATRIACONTANE	19.466	60682	0.491 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG090122\
Data File : FG010474.D
Signal(s) : FID1A.ch
Acq On : 01 Sep 2022 14:26
Operator : YP\AJ
Sample : PB147413BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 02 03:04:11 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG082622.M
Quant Title :
QLast Update : Fri Aug 26 23:48:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

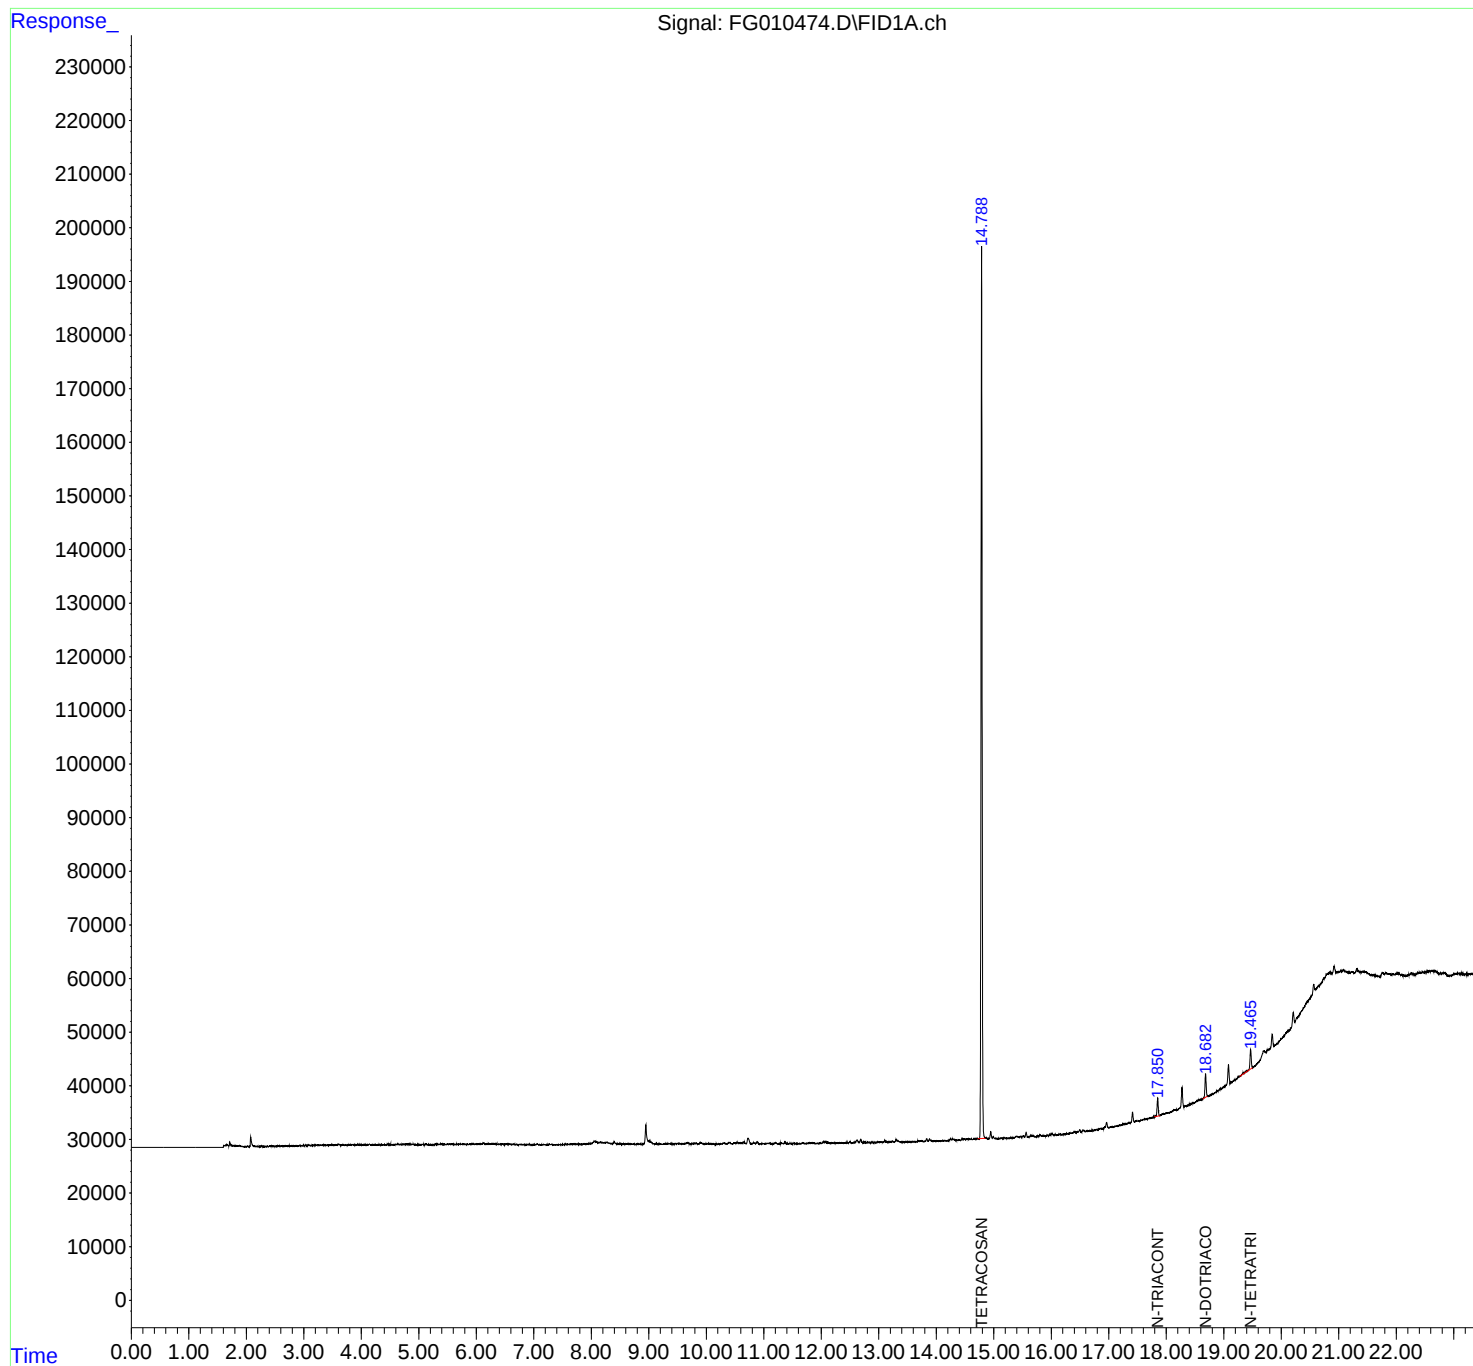


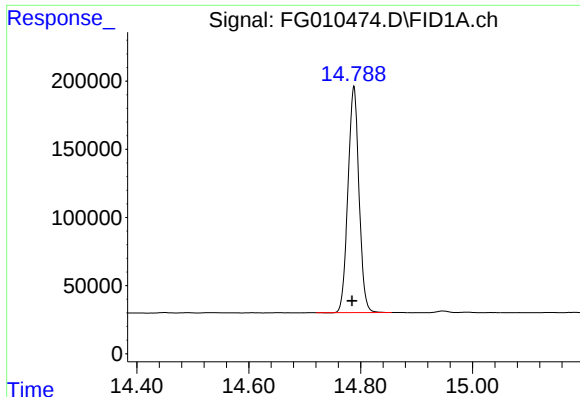

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.788 min
Delta R.T.: 0.003 min
Response: 2275814
Conc: 18.60 ug/ml

Instrument :
FID_G
ClientSampleId :

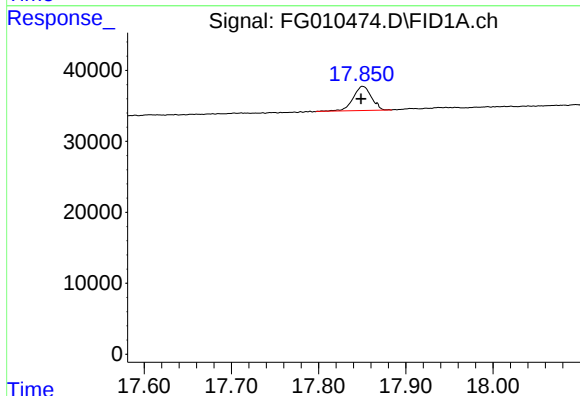


#13 N-TRIACONTANE

R.T.: 17.851 min
Delta R.T.: 0.002 min
Response: 49065
Conc: 0.38 ug/ml

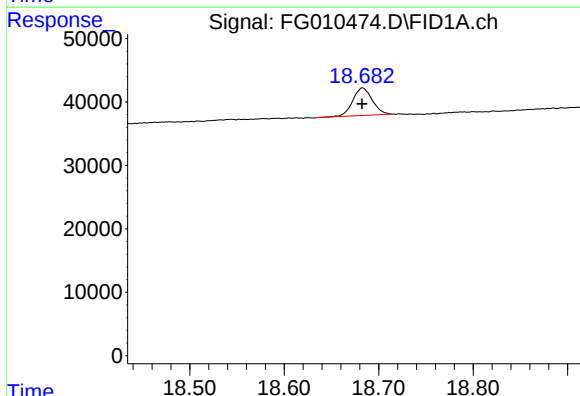

#14 N-DOTRIACONTANE

R.T.: 18.683 min
Delta R.T.: 0.000 min
Response: 62266
Conc: 0.49 ug/ml

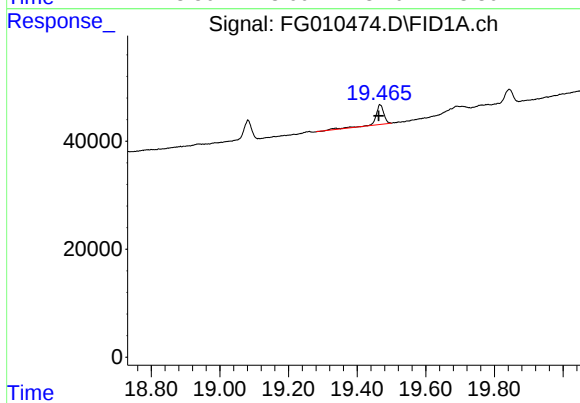

#15 N-TETRATRIACONTANE

R.T.: 19.466 min
Delta R.T.: 0.003 min
Response: 60682
Conc: 0.49 ug/ml