

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG090122\
 Data File : FG010476.D
 Signal(s) : FID1A.ch
 Acq On : 01 Sep 2022 15:25
 Operator : YP\AJ
 Sample : N4453-01 10X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Sep 02 03:04:34 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG082622.M
 Quant Title :
 QLast Update : Fri Aug 26 23:48:05 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.785	150987	1.234 ug/ml
Target Compounds			
7) N-EICOSANE	12.711	320411	2.244 ug/ml
10) N-TETRACOSANE	14.928f	182059	1.314 ug/ml
12) N-OCTACOSANE	16.923	39079	0.296 ug/ml
14) N-DOTRIACONTANE	18.681	66149	0.517 ug/ml
15) N-TETRATRIACONTANE	19.466	21422	0.173 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG090122\
Data File : FG010476.D
Signal(s) : FID1A.ch
Acq On : 01 Sep 2022 15:25
Operator : YP\AJ
Sample : N4453-01 10X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 02 03:04:34 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG082622.M
Quant Title :
QLast Update : Fri Aug 26 23:48:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

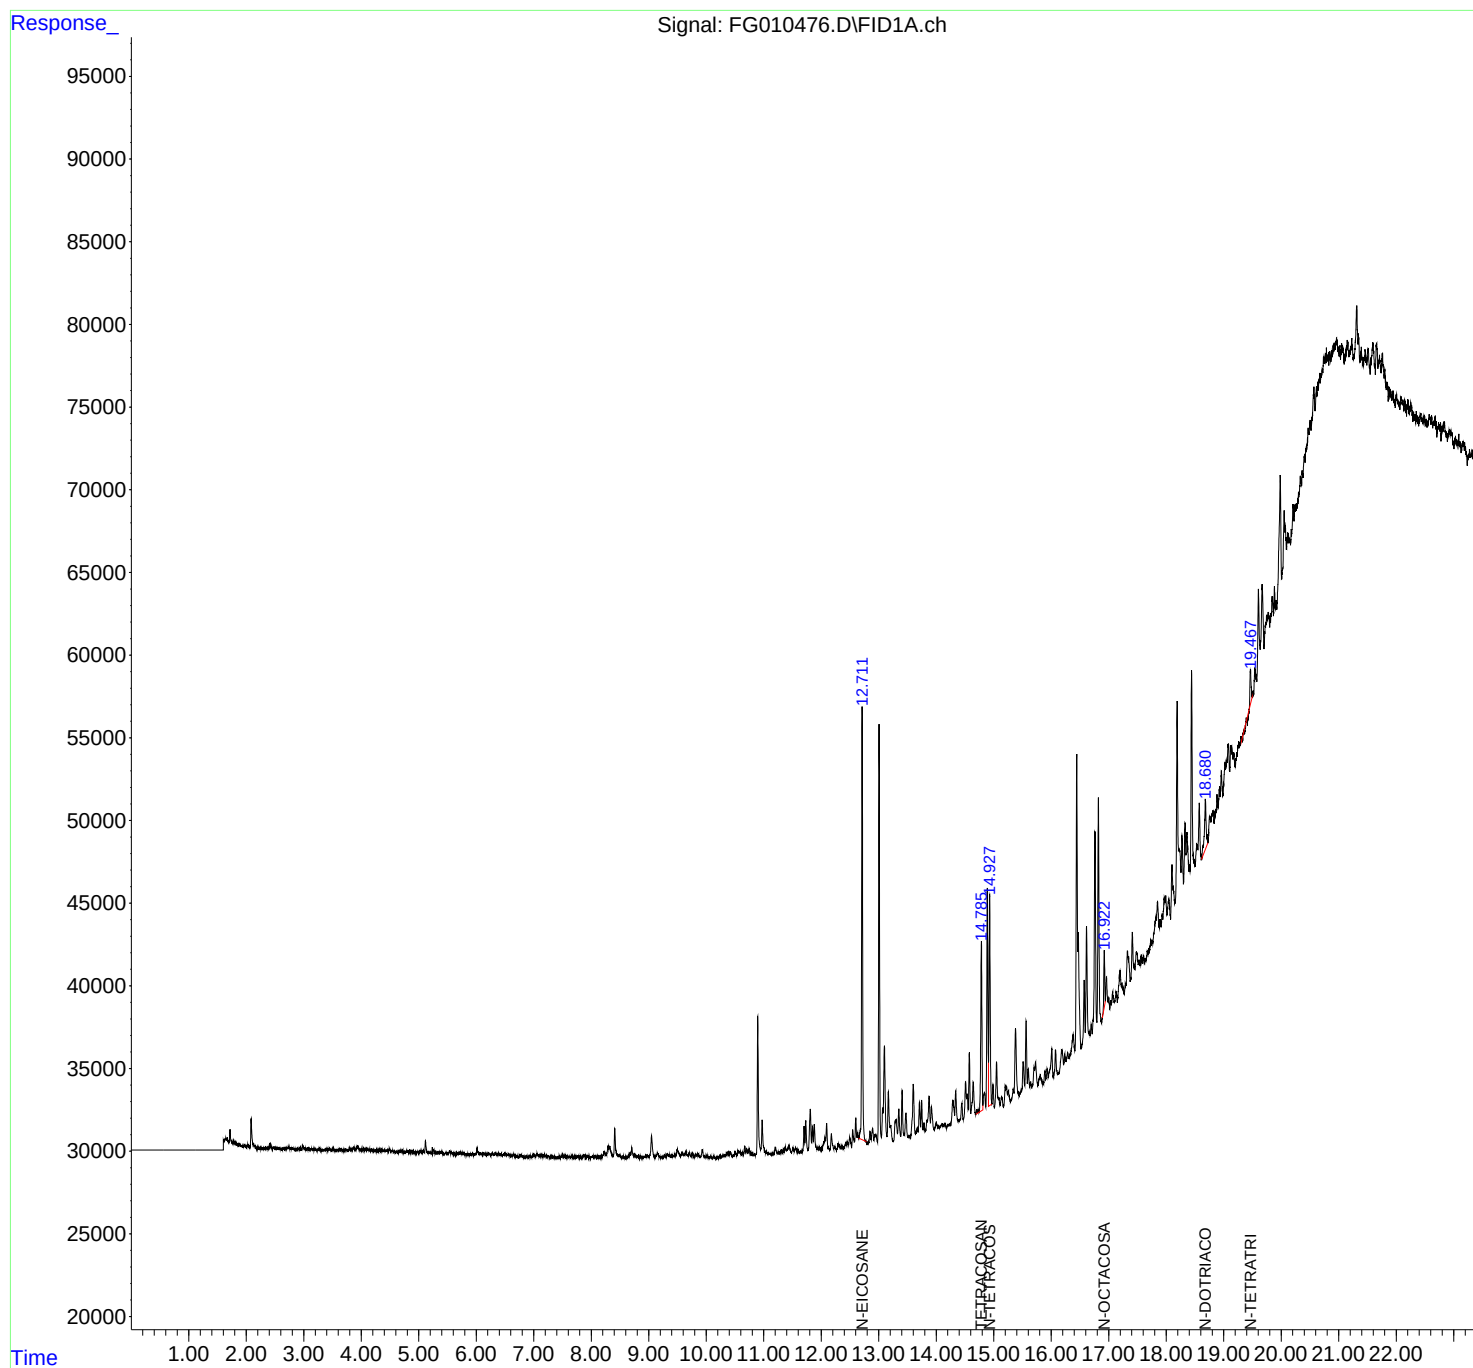


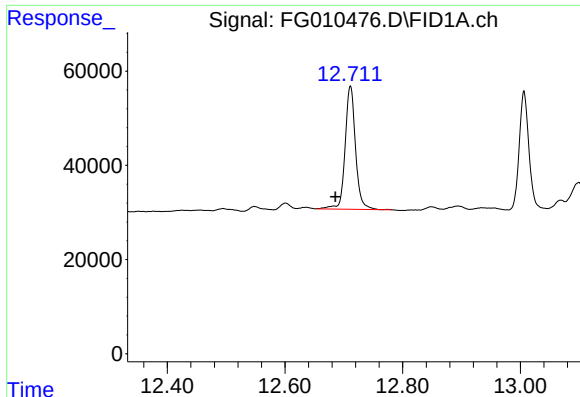

#7 N-EICOSANE


R.T.: 12.711 min
Delta R.T.: 0.026 min
Response: 320411
Conc: 2.24 ug/ml

Instrument :
FID_G
ClientSampleId :

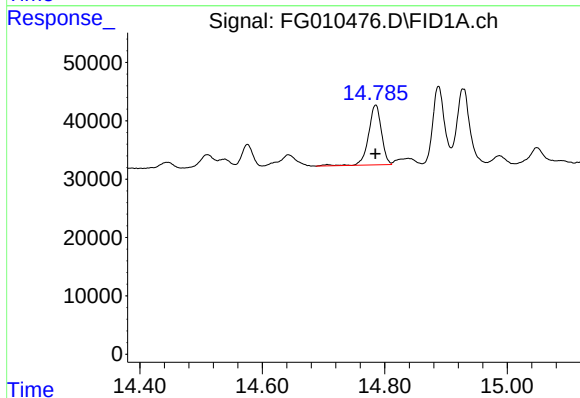


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.785 min
Delta R.T.: 0.000 min
Response: 150987
Conc: 1.23 ug/ml

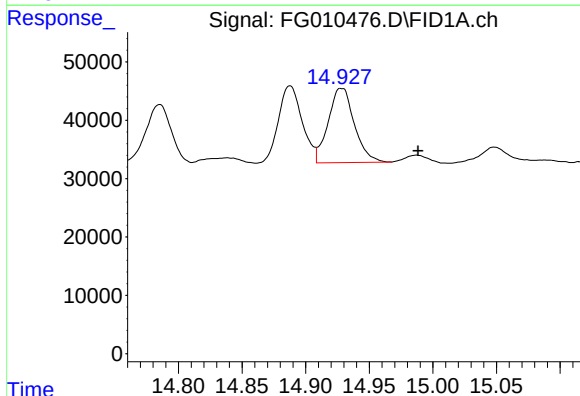


#10 N-TETRACOSANE

R.T.: 14.928 min
Delta R.T.: -0.060 min
Response: 182059
Conc: 1.31 ug/ml

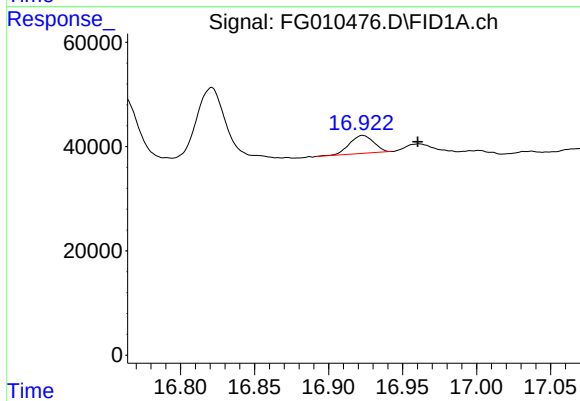

#12 N-OCTACOSANE


R.T.: 16.923 min
Delta R.T.: -0.037 min
Response: 39079
Conc: 0.30 ug/ml

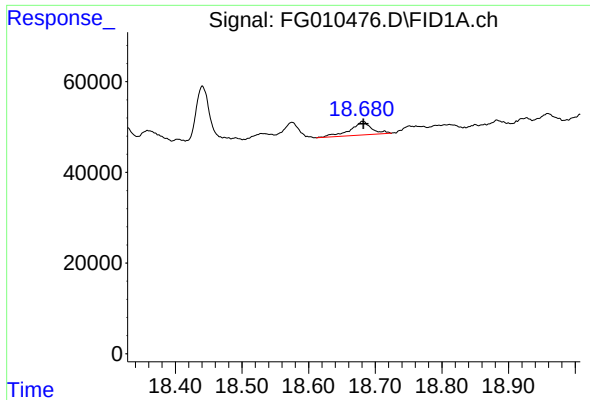

#14 N-DOTRIACONTANE

R.T.: 18.681 min
Delta R.T.: -0.001 min
Response: 66149
Conc: 0.52 ug/ml

Instrument :
FID_G
ClientSampleId :

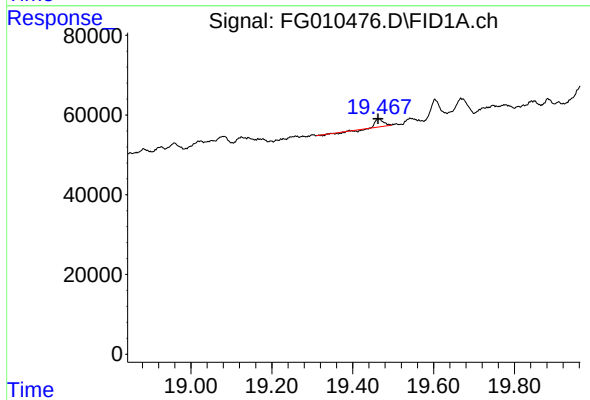

#15 N-TETRATRIACONTANE

R.T.: 19.466 min
Delta R.T.: 0.003 min
Response: 21422
Conc: 0.17 ug/ml