

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG090122\
 Data File : FG010477.D
 Signal(s) : FID1A.ch
 Acq On : 01 Sep 2022 15:55
 Operator : YP\AJ
 Sample : N4453-02
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Sep 02 03:04:45 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG082622.M
 Quant Title :
 QLast Update : Fri Aug 26 23:48:05 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.785	1530395	12.505 ug/ml
Target Compounds			
4) N-TETRADECANE	8.290	108115	0.799 ug/ml
7) N-EICOSANE	12.712	152627	1.069 ug/ml
10) N-TETRACOSANE	14.987	93542	0.675 ug/ml
11) N-HEXACOSANE	16.009	179118	1.320 ug/ml
12) N-OCTACOSANE	16.960	177227	1.340 ug/ml
13) N-TRIACONTANE	17.849	169171	1.306 ug/ml
14) N-DOTRIACONTANE	18.674	235616	1.843 ug/ml
15) N-TETRATRIACONTANE	19.471	60900	0.492 ug/ml
16) N-HEXATRIACONTANE	20.212	51087	0.440 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG090122\
Data File : FG010477.D
Signal(s) : FID1A.ch
Acq On : 01 Sep 2022 15:55
Operator : YP\AJ
Sample : N4453-02
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 02 03:04:45 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG082622.M
Quant Title :
QLast Update : Fri Aug 26 23:48:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

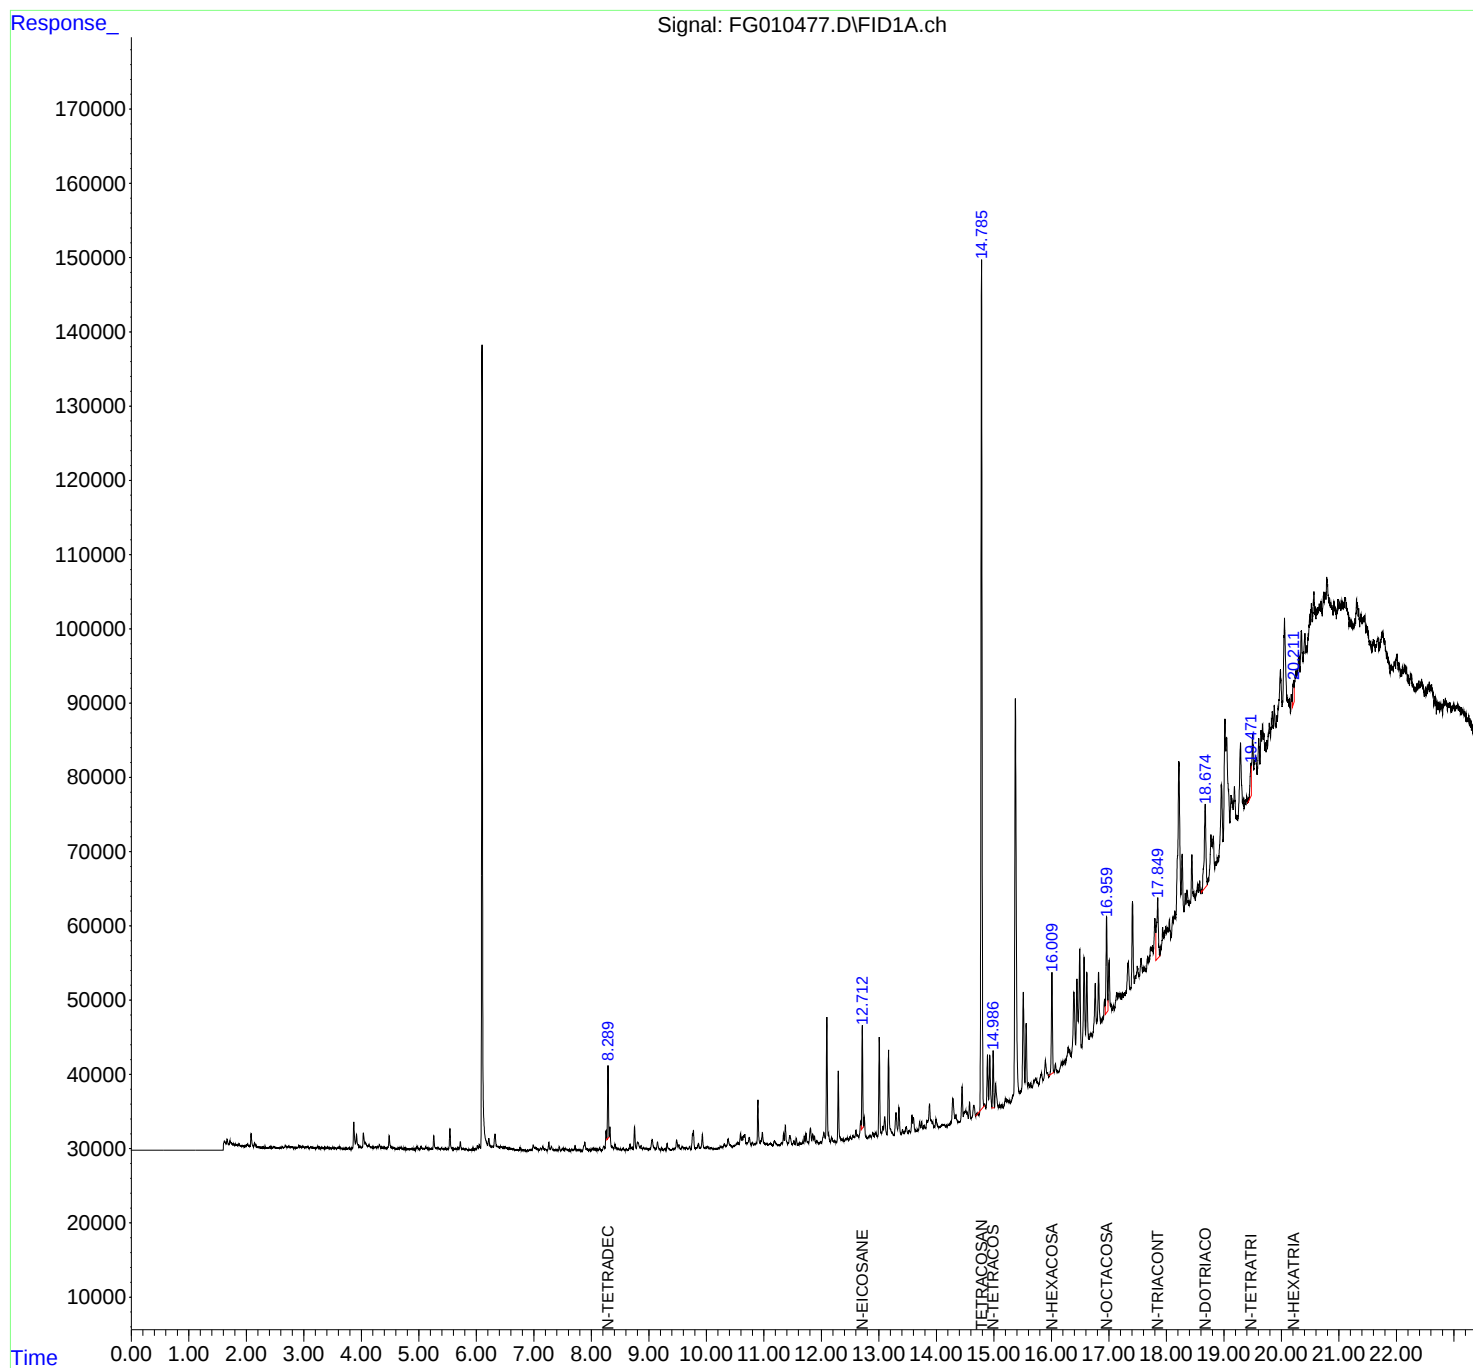


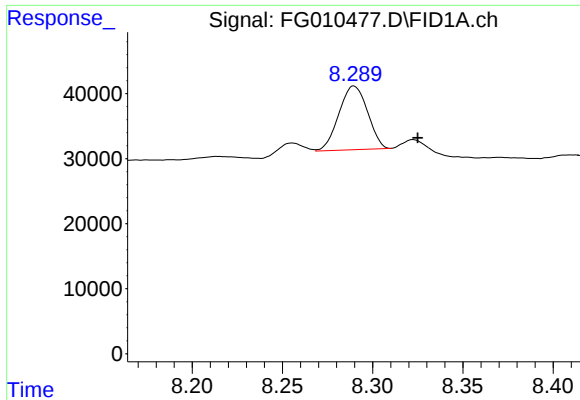

#4 N-TETRADECANE


R.T.: 8.290 min
Delta R.T.: -0.035 min
Response: 108115
Conc: 0.80 ug/ml

Instrument :
FID_G
ClientSampleId :

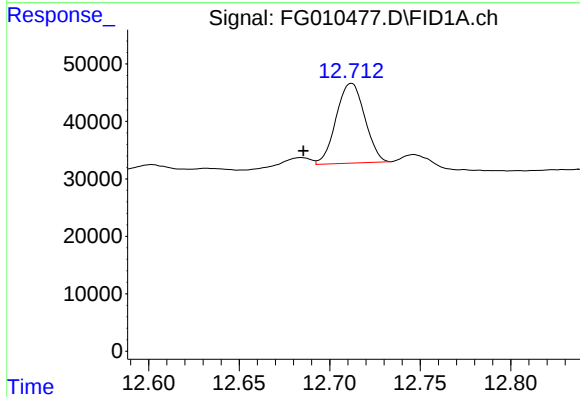


#7 N-EICOSANE

R.T.: 12.712 min
Delta R.T.: 0.026 min
Response: 152627
Conc: 1.07 ug/ml

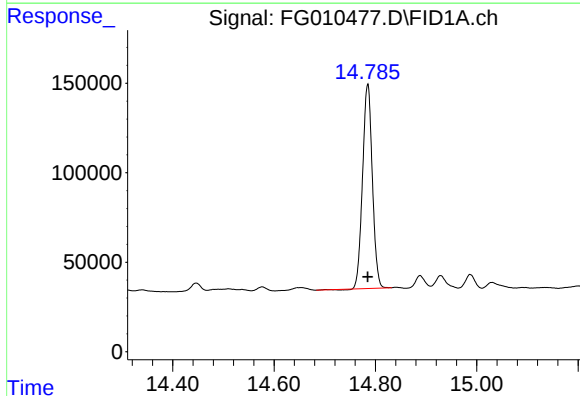


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.785 min
Delta R.T.: 0.000 min
Response: 1530395
Conc: 12.50 ug/ml

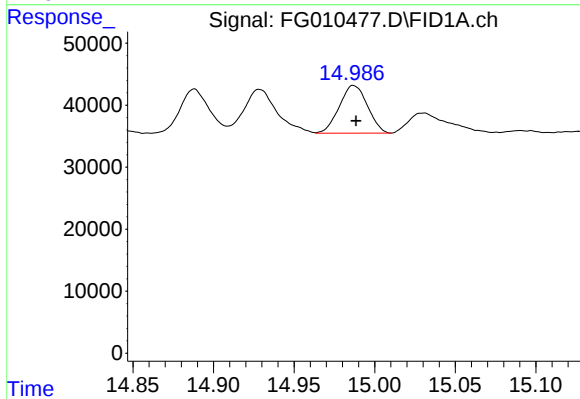

#10 N-TETRACOSANE


R.T.: 14.987 min
Delta R.T.: -0.001 min
Response: 93542
Conc: 0.68 ug/ml

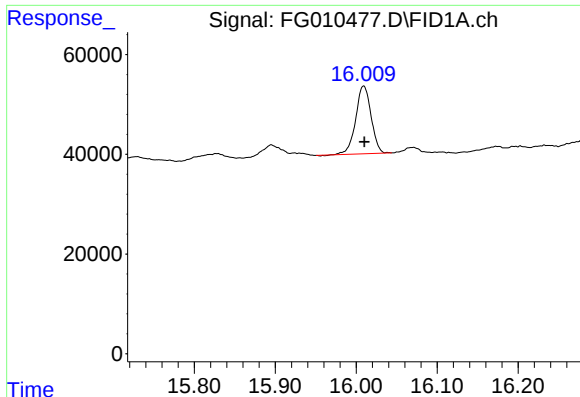

#11 N-HEXACOSANE


R.T.: 16.009 min
Delta R.T.: 0.000 min
Response: 179118
Conc: 1.32 ug/ml

Instrument :
FID_G
ClientSampleId :

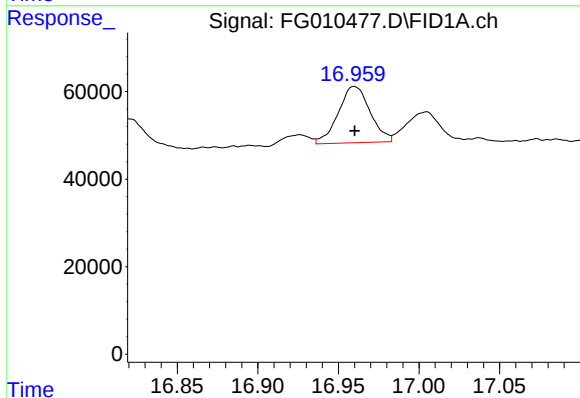


#12 N-OCTACOSANE

R.T.: 16.960 min
Delta R.T.: 0.000 min
Response: 177227
Conc: 1.34 ug/ml

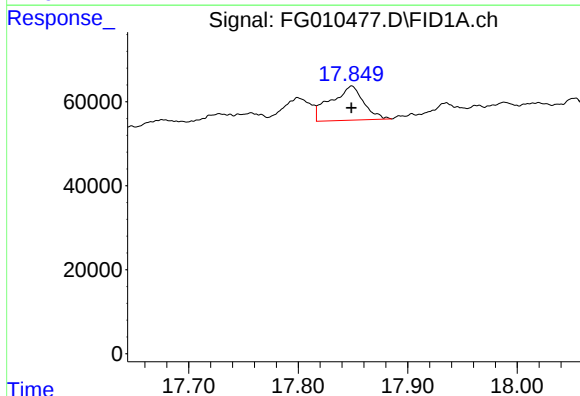


#13 N-TRIACONTANE

R.T.: 17.849 min
Delta R.T.: 0.000 min
Response: 169171
Conc: 1.31 ug/ml

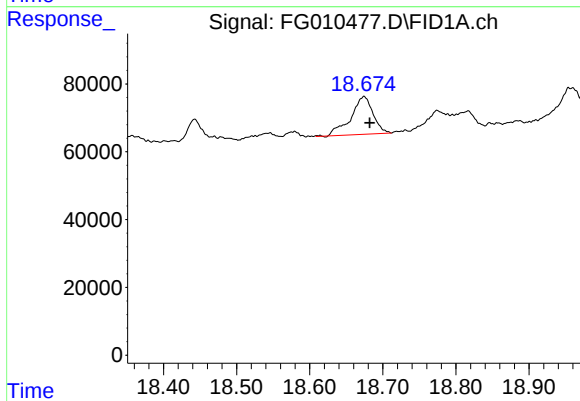

#14 N-DOTRIACONTANE


R.T.: 18.674 min
Delta R.T.: -0.008 min
Response: 235616
Conc: 1.84 ug/ml

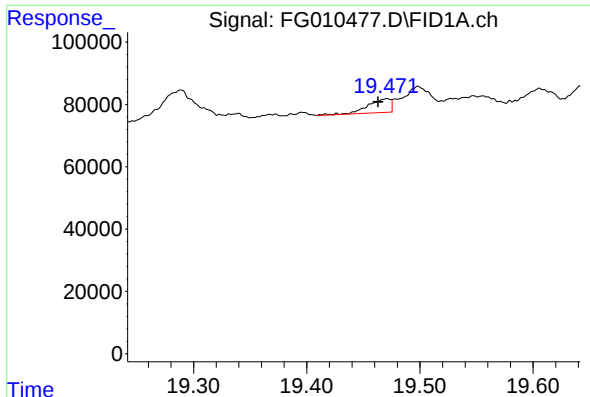

#15 N-TETRATRIACONTANE

R.T.: 19.471 min
Delta R.T.: 0.008 min
Response: 60900
Conc: 0.49 ug/ml

Instrument :
FID_G
ClientSampleId :

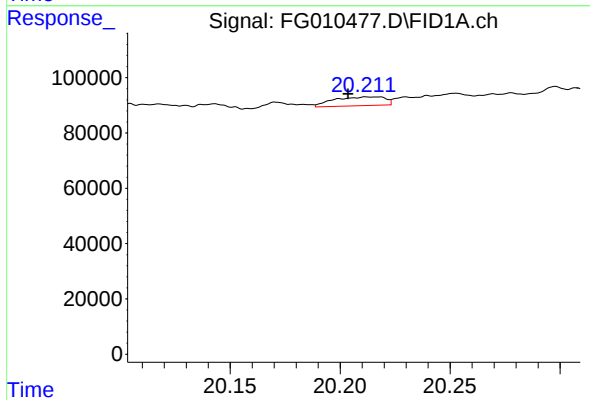

#16 N-HEXATRIACONTANE

R.T.: 20.212 min
Delta R.T.: 0.009 min
Response: 51087
Conc: 0.44 ug/ml