

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG090122\
Data File : FG010478.D
Signal(s) : FID1A.ch
Acq On : 01 Sep 2022 16:25
Operator : YP\AJ
Sample : N4466-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
SASP2-T-5-(10-17)

Integration File: autoint1.e
Quant Time: Sep 02 03:04:58 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG082622.M
Quant Title :
QLast Update : Fri Aug 26 23:48:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.786	1577953	12.893 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG090122\
Data File : FG010478.D
Signal(s) : FID1A.ch
Acq On : 01 Sep 2022 16:25
Operator : YP\AJ
Sample : N4466-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
SASP2-T-5-(10-17)

Integration File: autoint1.e
Quant Time: Sep 02 03:04:58 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG082622.M
Quant Title :
QLast Update : Fri Aug 26 23:48:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

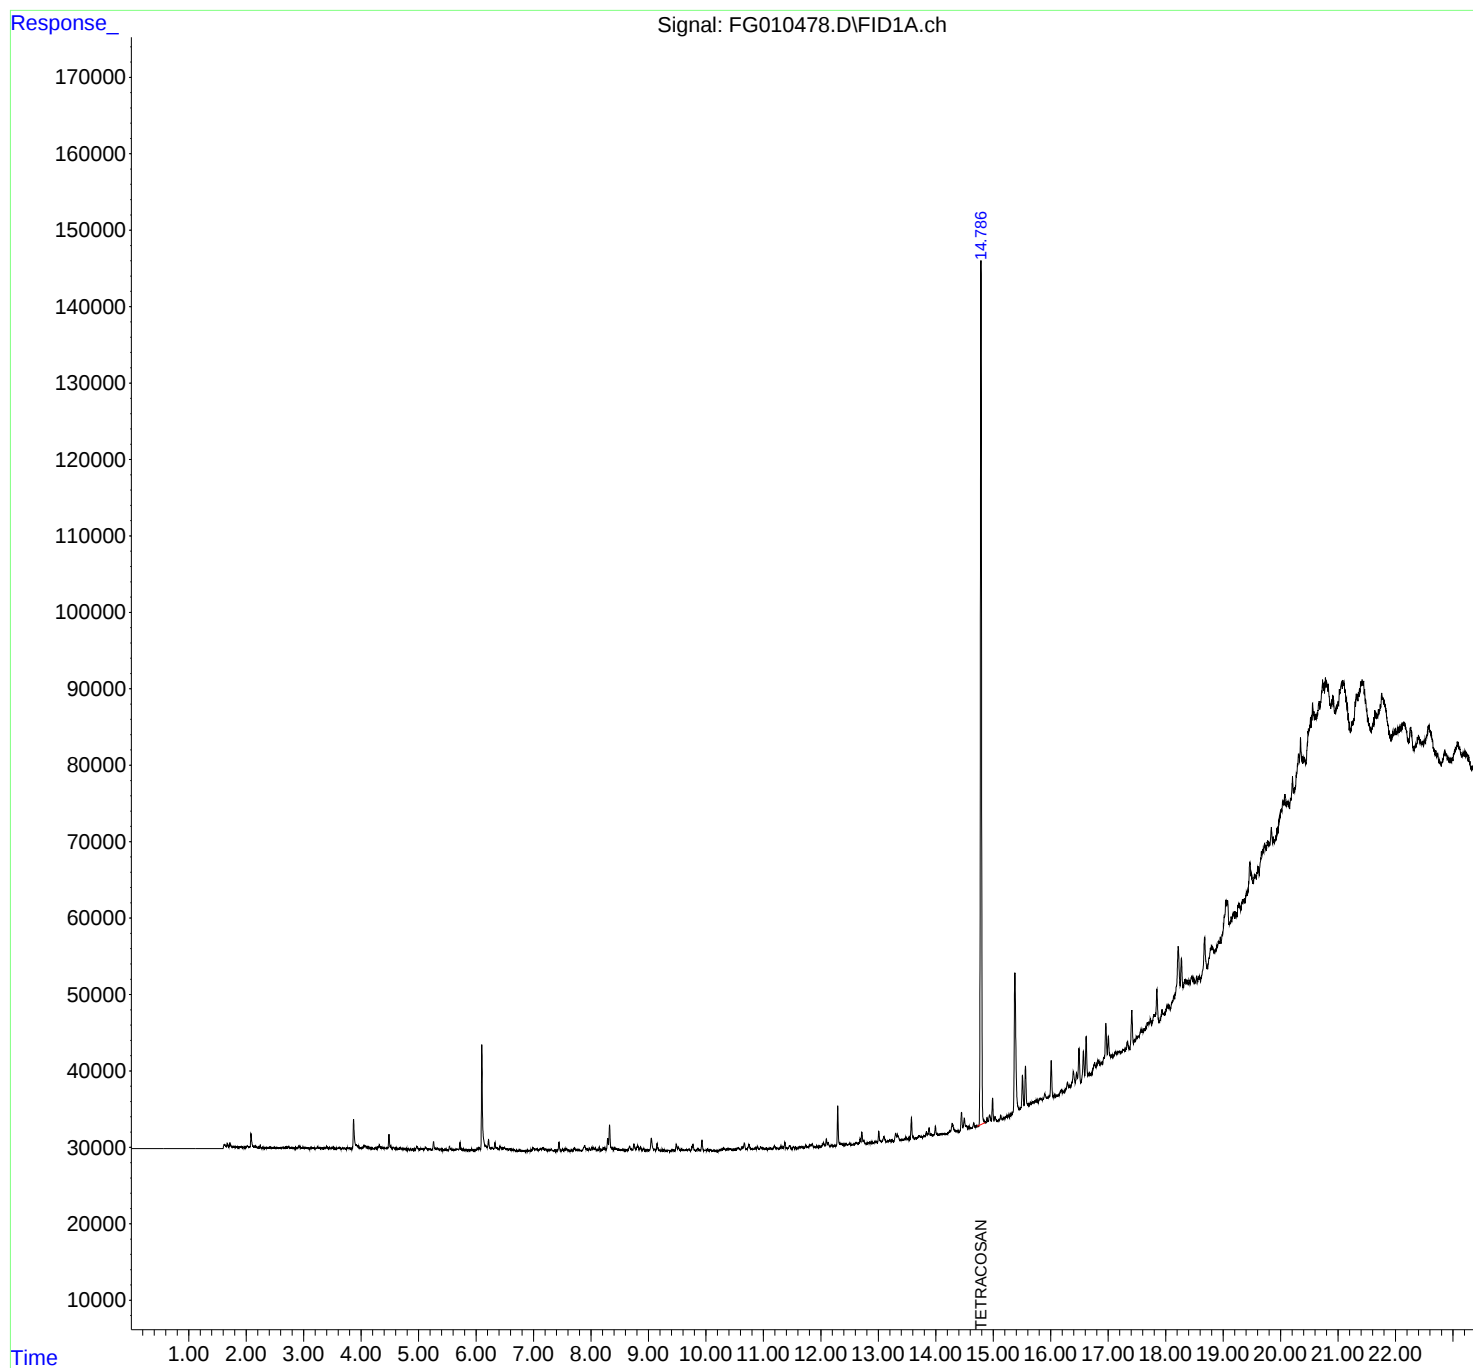

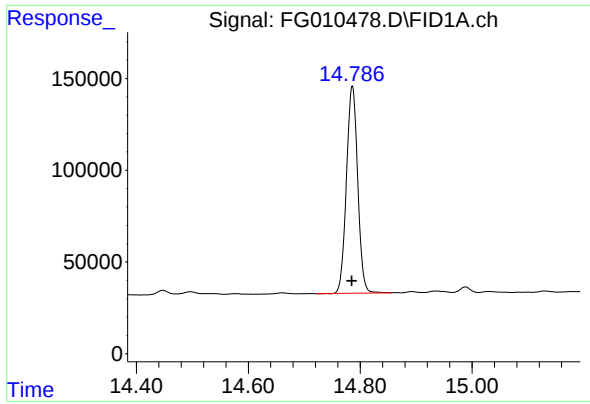

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.786 min
Delta R.T.: 0.001 min
Response: 1577953
Conc: 12.89 ug/ml

Instrument :
FID_G
ClientSampleId :
SASP2-T-5-(10-17)