

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG090622\
 Data File : FG010493.D
 Signal(s) : FID1A.ch
 Acq On : 06 Sep 2022 12:23
 Operator : YP\AJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Sep 07 04:02:27 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG082622.M
 Quant Title :
 QLast Update : Fri Aug 26 23:48:05 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.491	2026125	15.395 ug/ml
12)	N-OCTACOSANE	16.956	2041993	15.441 ug/ml
13)	N-TRIACONTANE	17.844	204585	1.579 ug/ml
14)	N-DOTRIACONTANE	18.675	278070	2.175 ug/ml
15)	N-TETRATRIACONTANE	19.459	250183	2.022 ug/ml
16)	N-HEXATRIACONTANE	20.200	177005	1.525 ug/ml
17)	N-OCTATRIACONTANE	20.909	121548	1.058 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG090622\
Data File : FG010493.D
Signal(s) : FID1A.ch
Acq On : 06 Sep 2022 12:23
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 07 04:02:27 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG082622.M
Quant Title :
QLast Update : Fri Aug 26 23:48:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

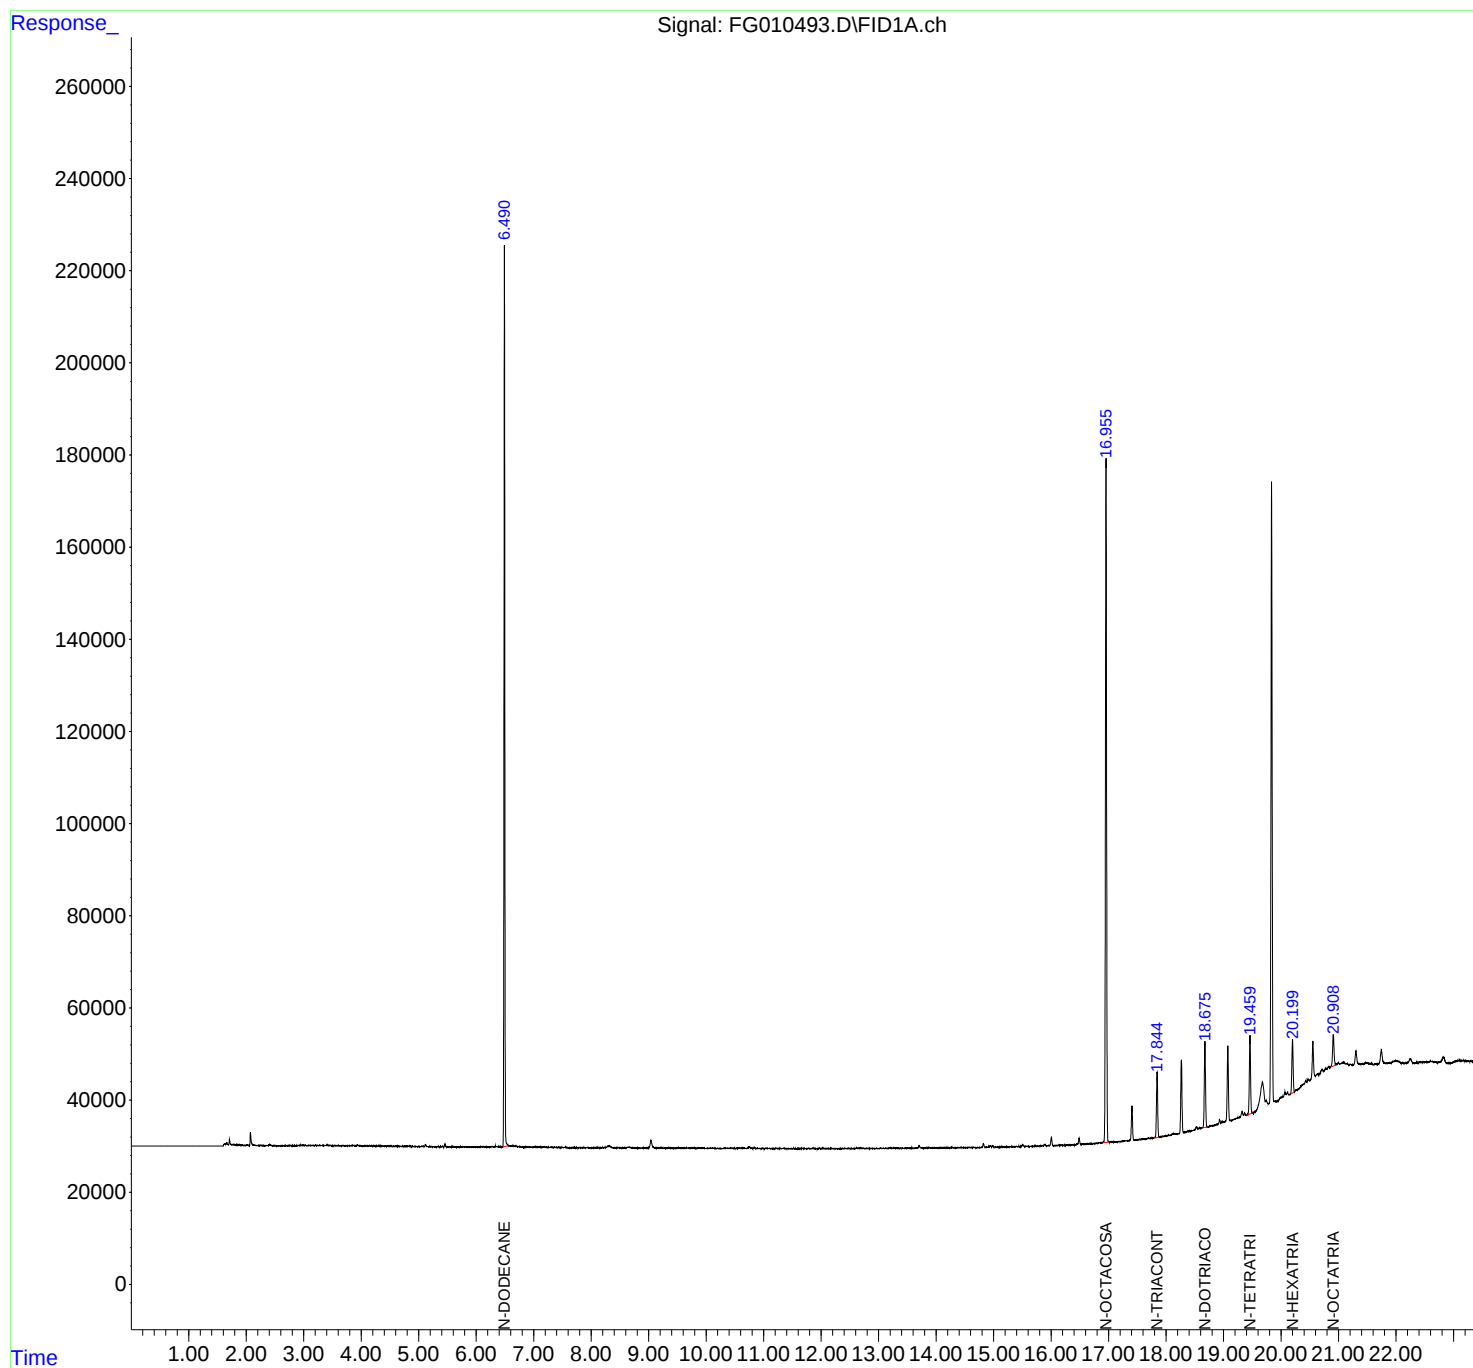


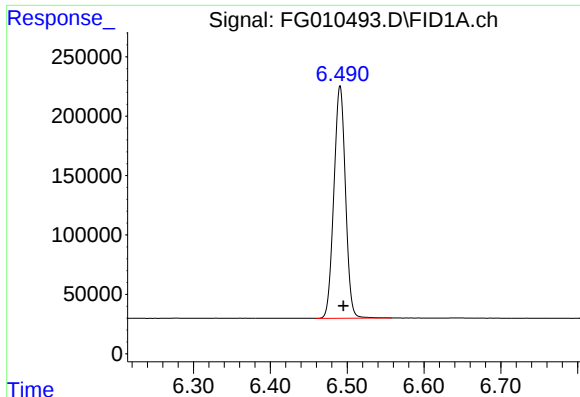

#3 N-DODECANE


R.T.: 6.491 min
Delta R.T.: -0.004 min
Response: 2026125
Conc: 15.39 ug/ml

Instrument :
FID_G
ClientSampleId :

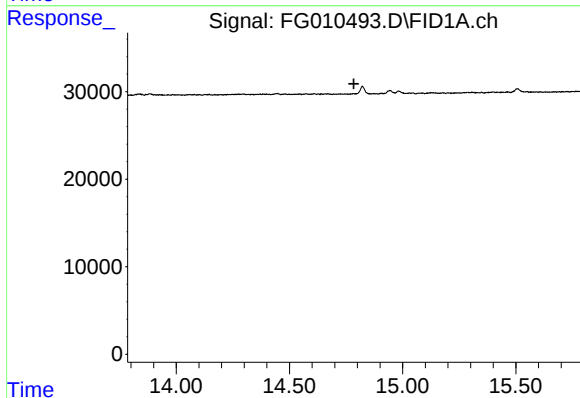


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.785 min
Response: 0
Conc: N.D.

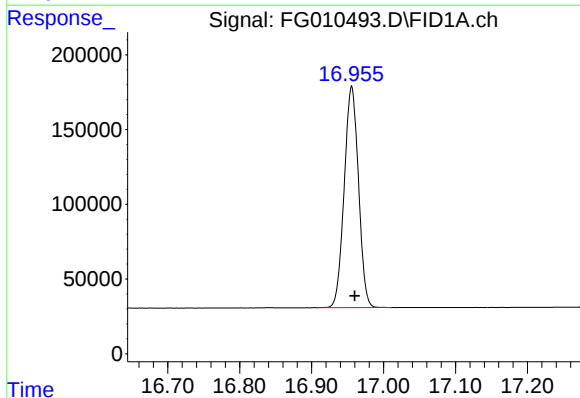


#12 N-OCTACOSANE

R.T.: 16.956 min
Delta R.T.: -0.004 min
Response: 2041993
Conc: 15.44 ug/ml

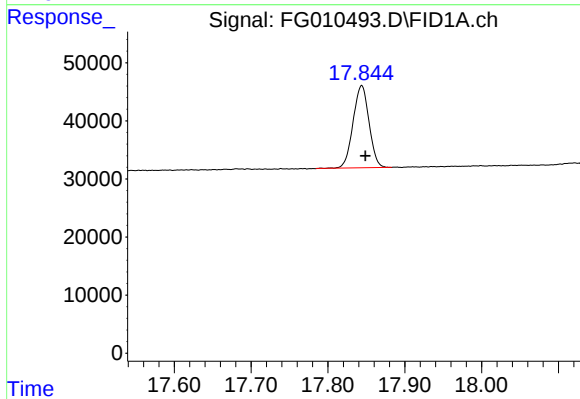

#13 N-TRIACONTANE


R.T.: 17.844 min
Delta R.T.: -0.005 min
Response: 204585
Conc: 1.58 ug/ml

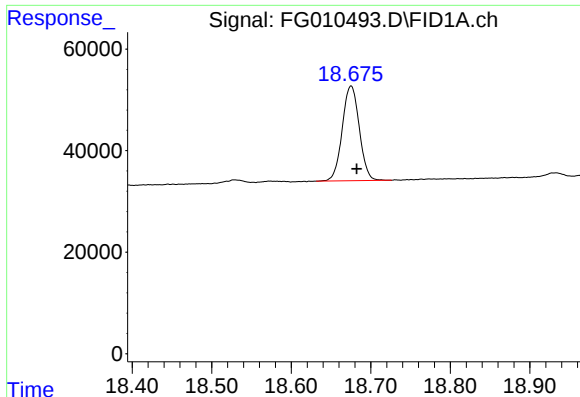

#14 N-DOTRIACONTANE


R.T.: 18.675 min
Delta R.T.: -0.007 min
Response: 278070
Conc: 2.17 ug/ml

Instrument :
FID_G
ClientSampleId :

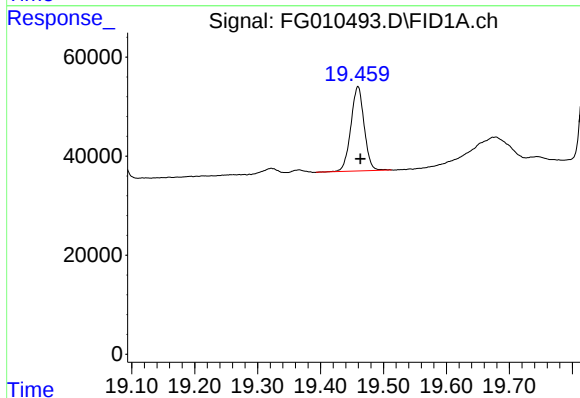


#15 N-TETRATRIACONTANE

R.T.: 19.459 min
Delta R.T.: -0.004 min
Response: 250183
Conc: 2.02 ug/ml

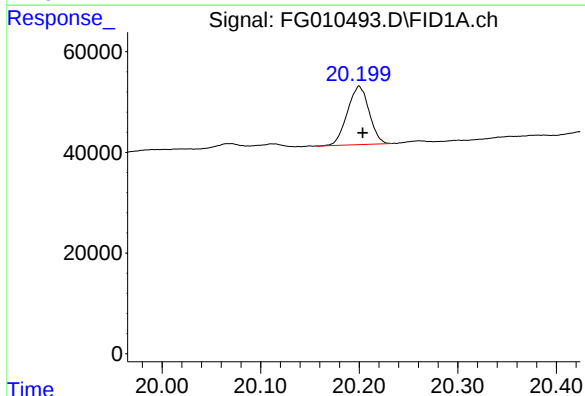

#16 N-HEXATRIACONTANE

R.T.: 20.200 min
Delta R.T.: -0.004 min
Response: 177005
Conc: 1.53 ug/ml

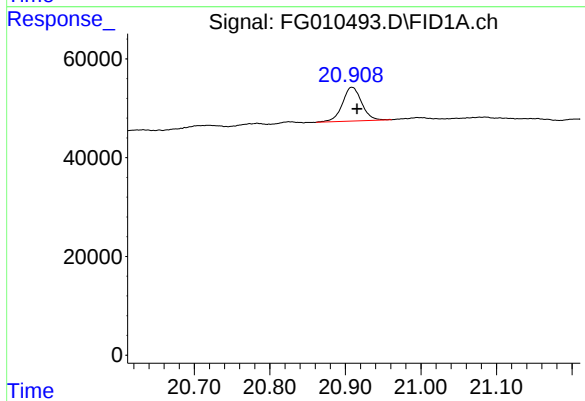

#17 N-OCTATRIACONTANE

R.T.: 20.909 min
Delta R.T.: -0.007 min
Response: 121548
Conc: 1.06 ug/ml