

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG090622\
Data File : FG010505.D
Signal(s) : FID1A.ch
Acq On : 06 Sep 2022 22:12
Operator : YP\AJ
Sample : N4501-06
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 07 04:03:56 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG082622.M
Quant Title :
QLast Update : Fri Aug 26 23:48:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.779	1478153	12.078 ug/ml
Target Compounds				
10)	N-TETRACOSANE	14.981	42509	0.307 ug/ml
11)	N-HEXACOSANE	16.003	55019	0.406 ug/ml
12)	N-OCTACOSANE	16.953	45344	0.343 ug/ml
14)	N-DOTRIACONTANE	18.670	65636	0.513 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG090622\
Data File : FG010505.D
Signal(s) : FID1A.ch
Acq On : 06 Sep 2022 22:12
Operator : YP\AJ
Sample : N4501-06
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 07 04:03:56 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG082622.M
Quant Title :
QLast Update : Fri Aug 26 23:48:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

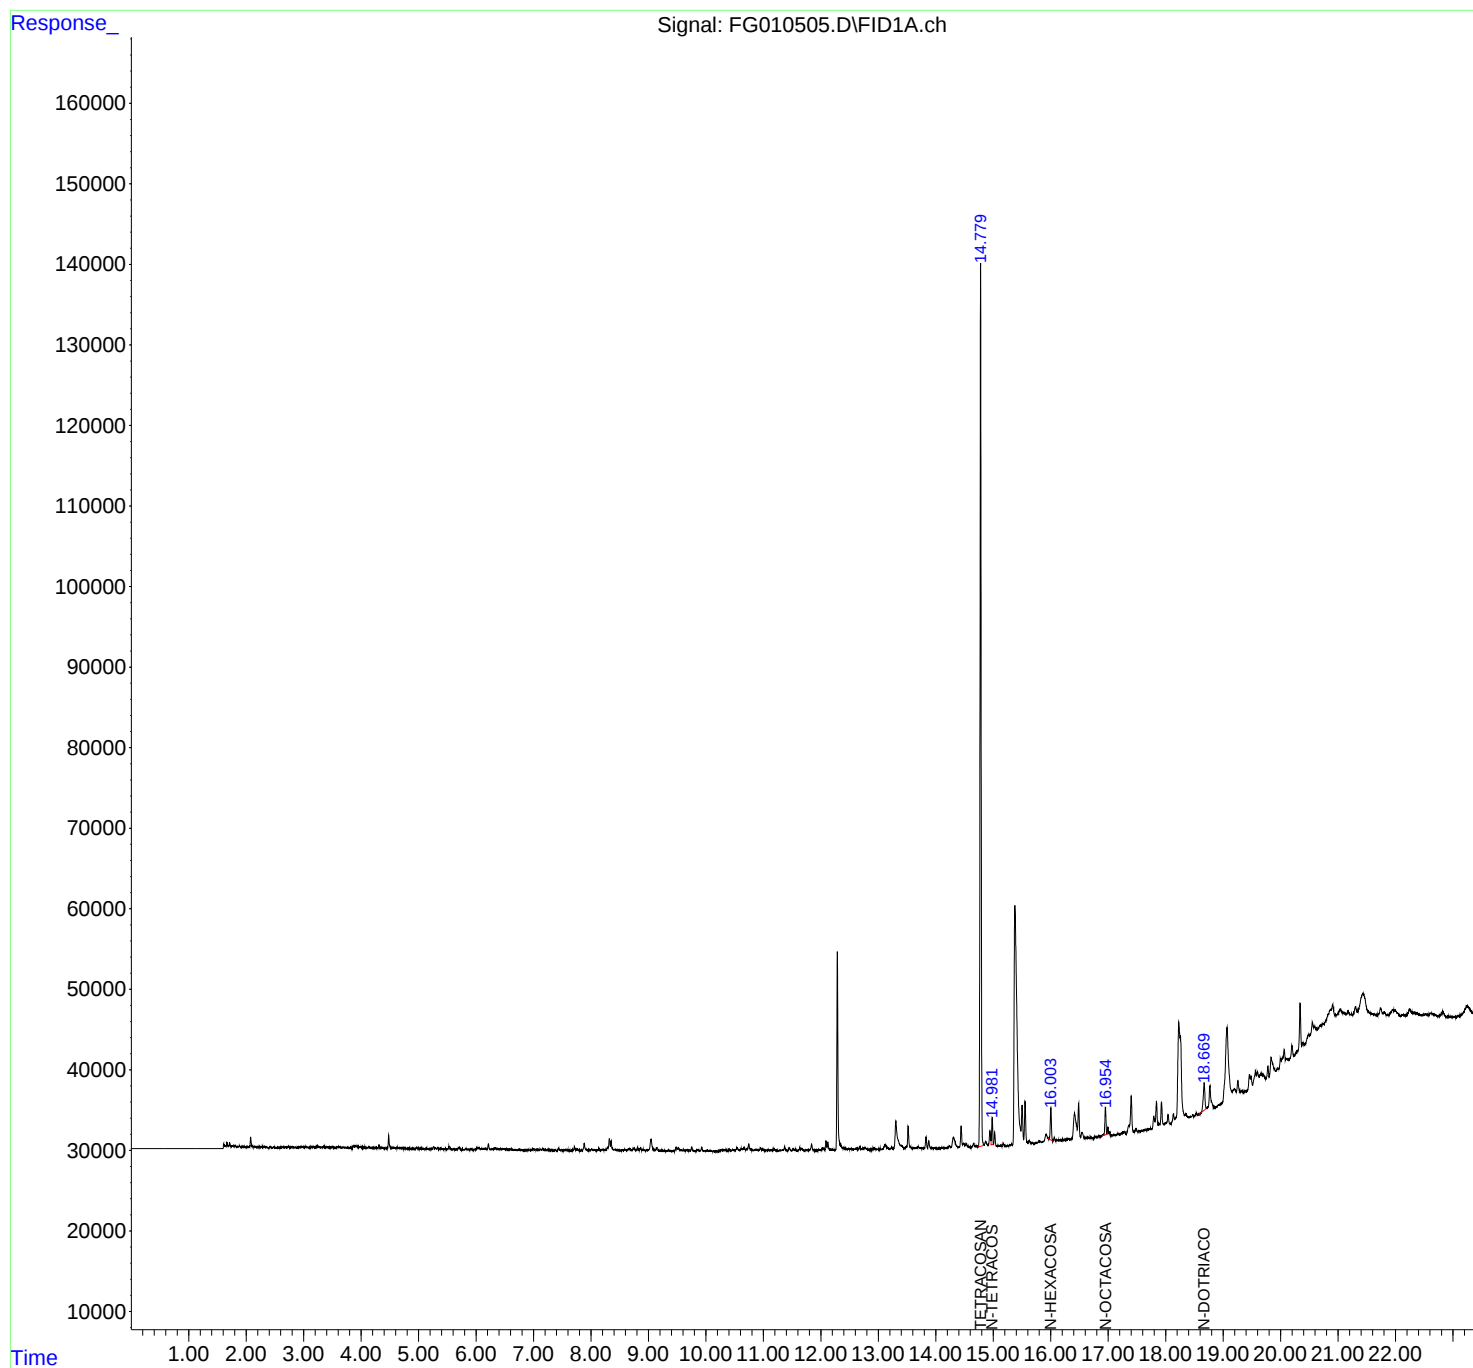


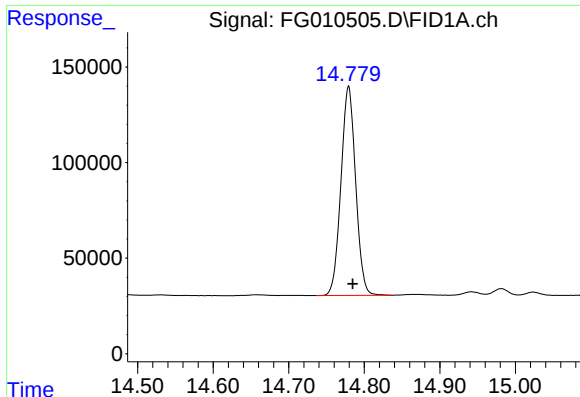

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.779 min
Delta R.T.: -0.005 min
Response: 1478153
Conc: 12.08 ug/ml

Instrument :
FID_G
ClientSampleId :

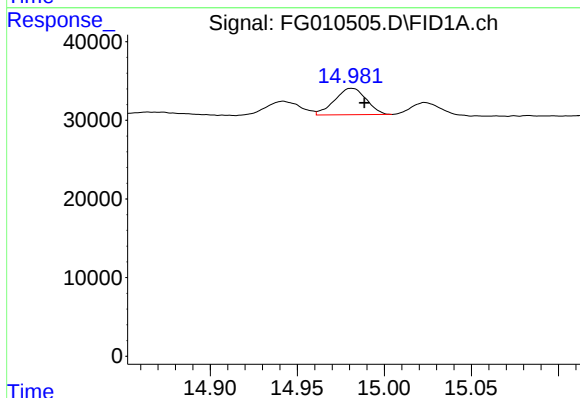


#10 N-TETRACOSANE

R.T.: 14.981 min
Delta R.T.: -0.007 min
Response: 42509
Conc: 0.31 ug/ml

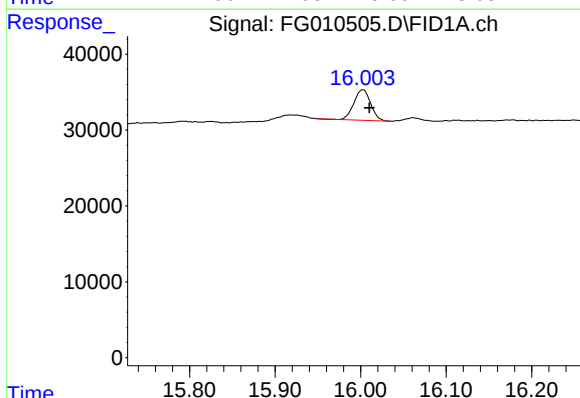


#11 N-HEXACOSANE

R.T.: 16.003 min
Delta R.T.: -0.008 min
Response: 55019
Conc: 0.41 ug/ml

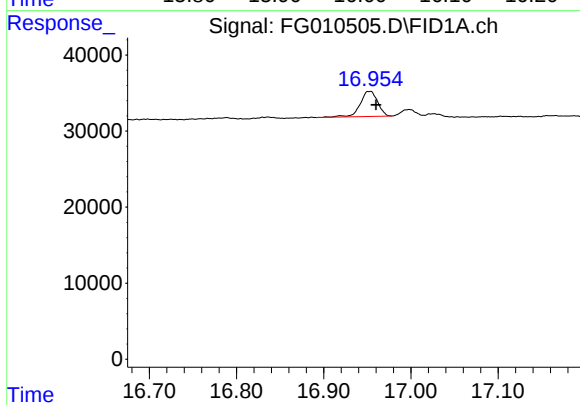

#12 N-OCTACOSANE

R.T.: 16.953 min
Delta R.T.: -0.007 min
Response: 45344
Conc: 0.34 ug/ml

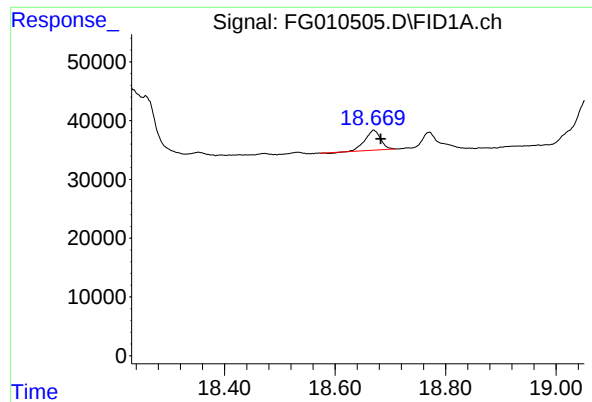

#14 N-DOTRIACONTANE

R.T.: 18.670 min
Delta R.T.: -0.013 min
Response: 65636
Conc: 0.51 ug/ml

Instrument :

FID_G

ClientSampleId :