

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG090623\
Data File : FG012855.D
Signal(s) : FID1A.ch
Acq On : 06 Sep 2023 11:04
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 07 01:42:12 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG090123.M
Quant Title :
QLast Update : Thu Aug 31 16:39:19 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
18) N-TETRACONTANE	22.207	39729	0.511 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG090623\
Data File : FG012855.D
Signal(s) : FID1A.ch
Acq On : 06 Sep 2023 11:04
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 07 01:42:12 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG090123.M
Quant Title :
QLast Update : Thu Aug 31 16:39:19 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

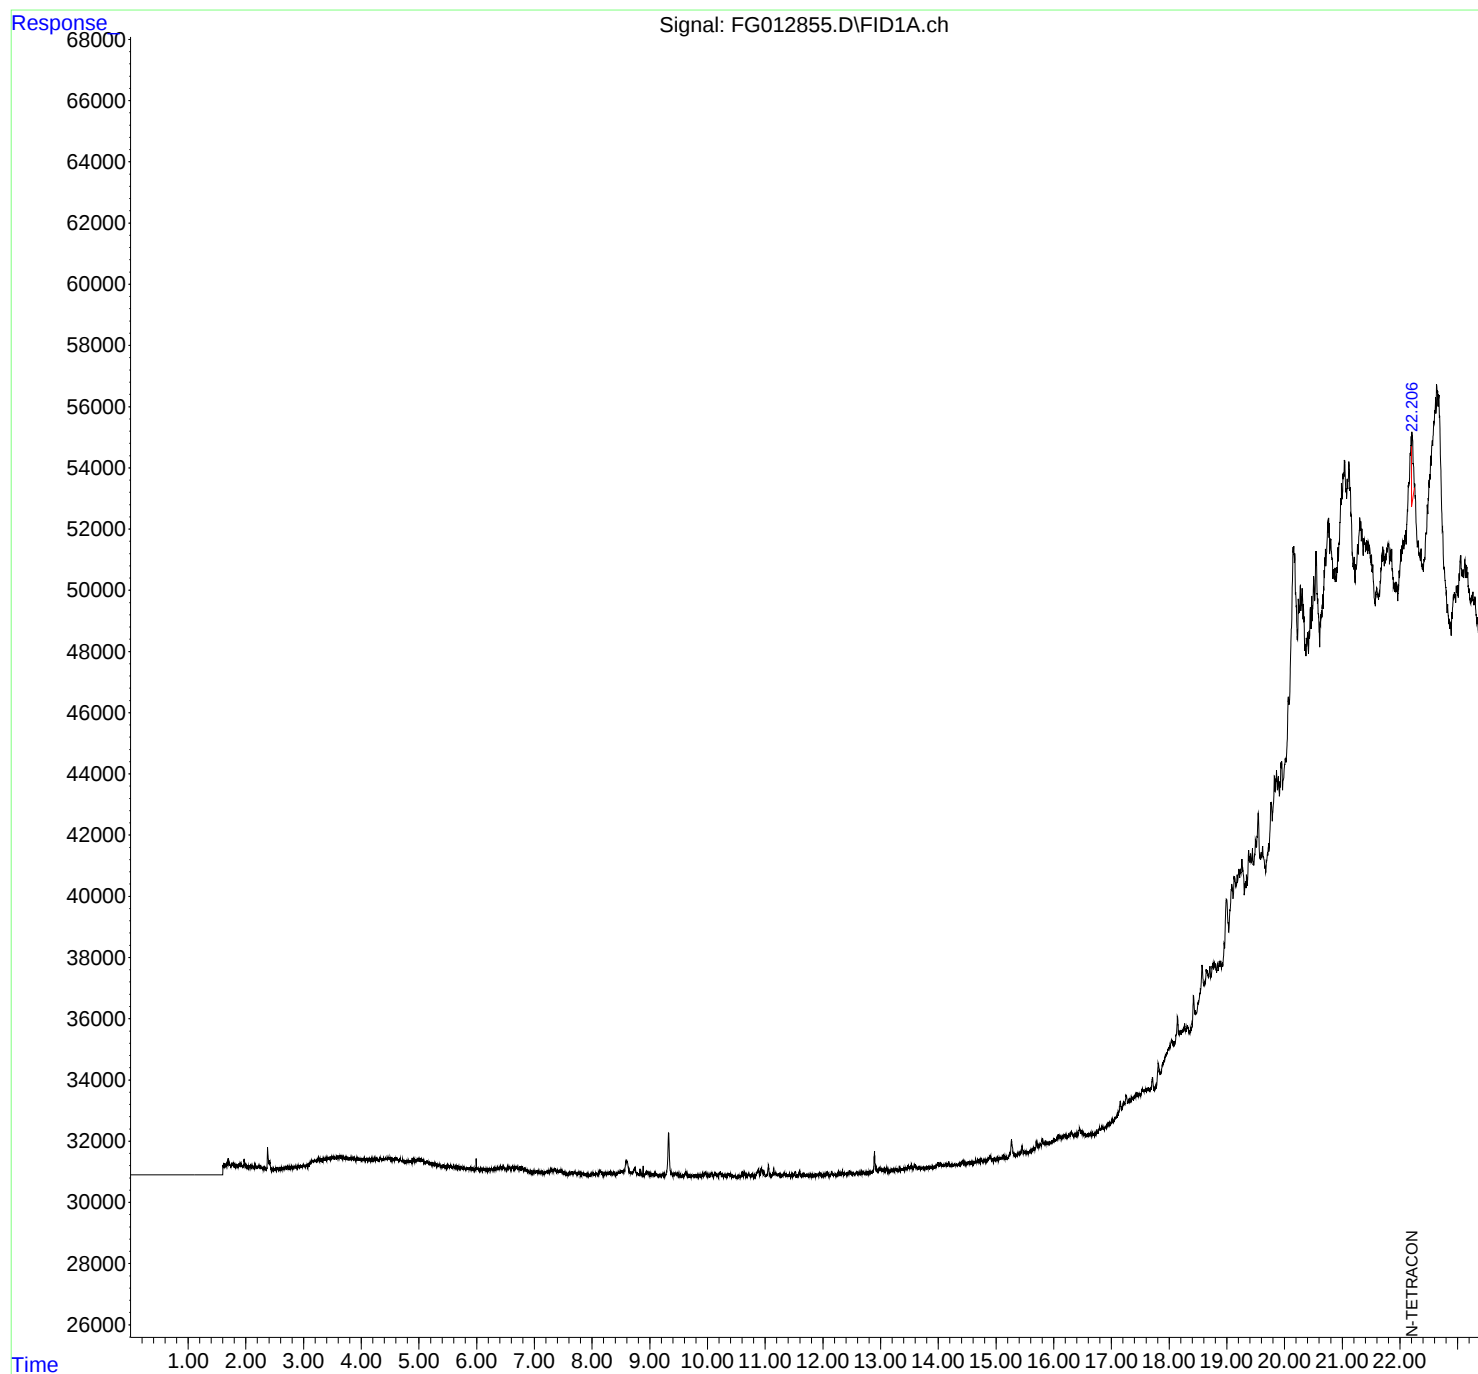


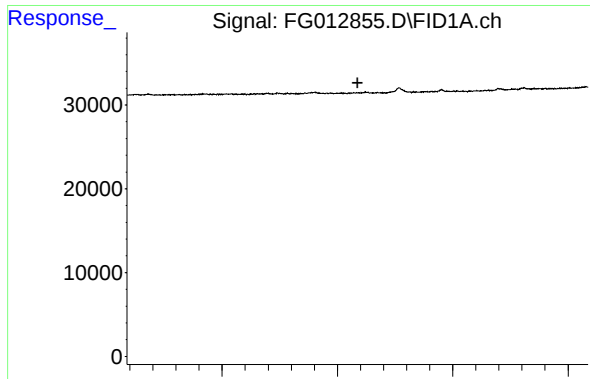

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T.: 15.087 min
Response: 0
Conc: N.D.

Instrument :
FID_G
ClientSampleId :

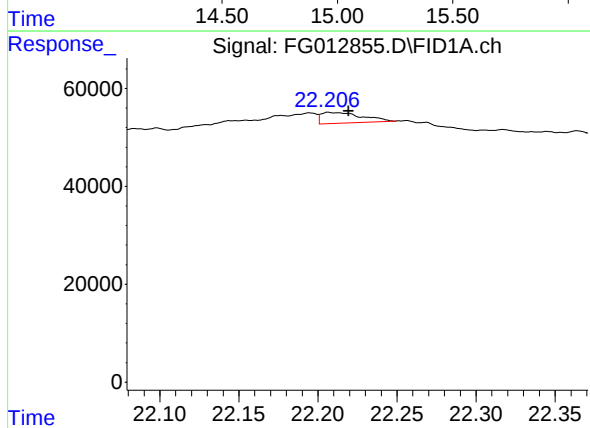

#18 N-TETRACONTANE

R.T.: 22.207 min
Delta R.T.: -0.012 min
Response: 39729
Conc: 0.51 ug/ml