

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG090623\
Data File : FG012858.D
Signal(s) : FID1A.ch
Acq On : 06 Sep 2023 13:55
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Sep 07 01:42:33 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG090123.M
Quant Title :
QLast Update : Thu Aug 31 16:39:19 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) N-DODECANE	6.770	1909906	14.111 ug/ml
12) N-OCTACOSANE	17.261	2012052	17.175 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG090623\
Data File : FG012858.D
Signal(s) : FID1A.ch
Acq On : 06 Sep 2023 13:55
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Sep 07 01:42:33 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG090123.M
Quant Title :
QLast Update : Thu Aug 31 16:39:19 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

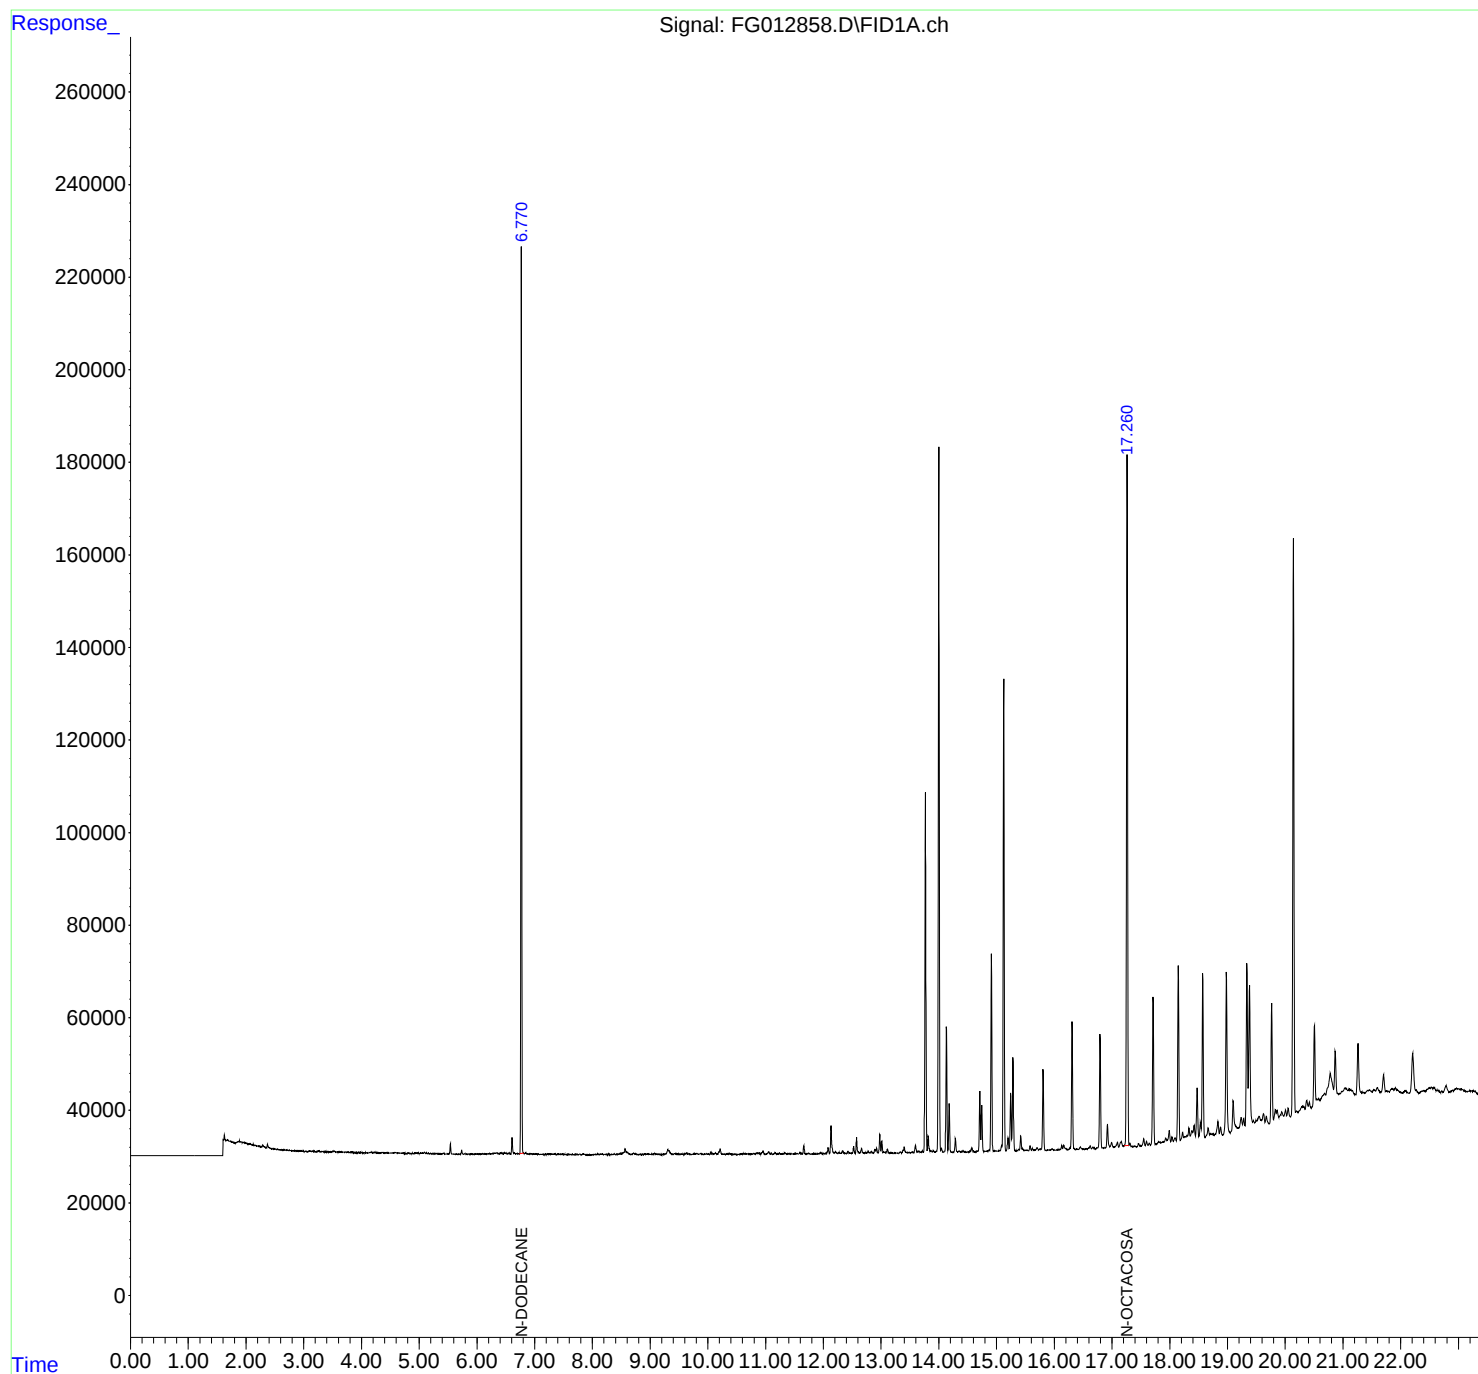


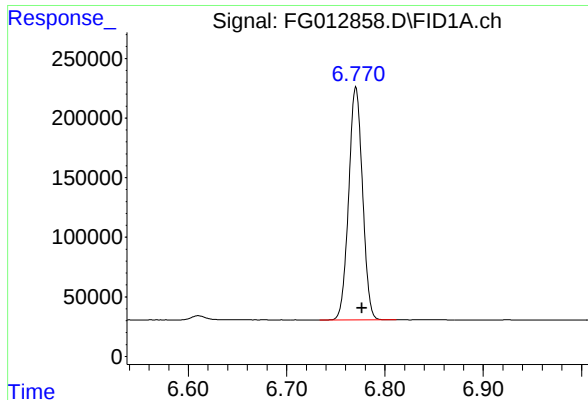

#3 N-DODECANE


R.T.: 6.770 min
Delta R.T.: -0.006 min
Response: 1909906
Conc: 14.11 ug/ml

Instrument :
FID_G
ClientSampleId :
RT MARKER

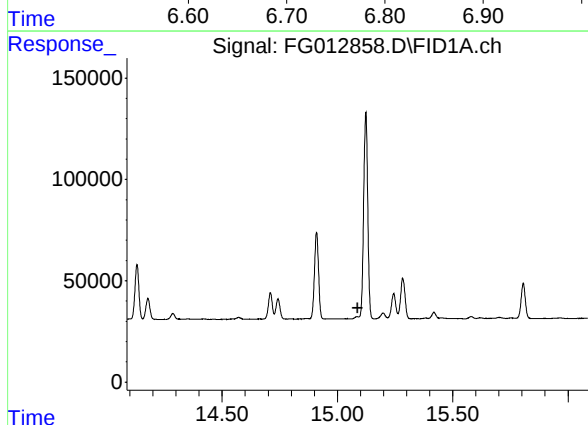

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 15.087 min
Response: 0
Conc: N.D.

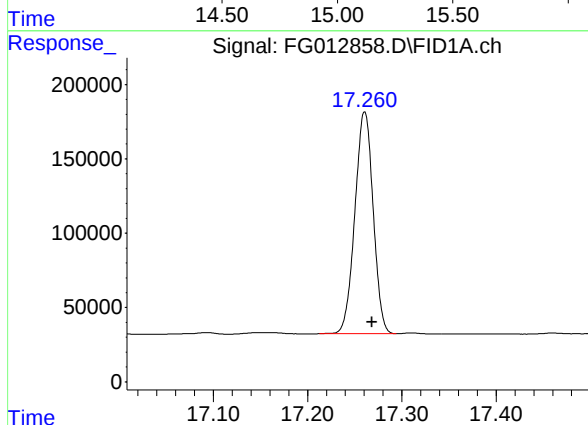

#12 N-OCTACOSANE

R.T.: 17.261 min
Delta R.T.: -0.007 min
Response: 2012052
Conc: 17.17 ug/ml