

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG090719\
Data File : FG005870.D
Signal(s) : FID1A.ch
Acq On : 07 Sep 2019 23:58
Operator : DD\AJ
Sample : 10 TRPH STD
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 09 04:33:05 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG090719.M
Quant Title :
QLast Update : Mon Sep 09 04:30:48 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
1) N-OCTANE	2.333	1313663	9.285 ug/ml
2) N-DECANE	4.435	1319946	9.190 ug/ml
3) N-DODECANE	6.462	1336560	9.230 ug/ml
4) N-TETRADECANE	8.264	1344807	9.347 ug/ml
5) N-HEXADECANE	9.869	1340095	9.396 ug/ml
6) N-OCTADECANE	11.315	1312669	9.467 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG090719\
Data File : FG005870.D
Signal(s) : FID1A.ch
Acq On : 07 Sep 2019 23:58
Operator : DD\AJ
Sample : 10 TRPH STD
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 09 04:33:05 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG090719.M
Quant Title :
QLast Update : Mon Sep 09 04:30:48 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

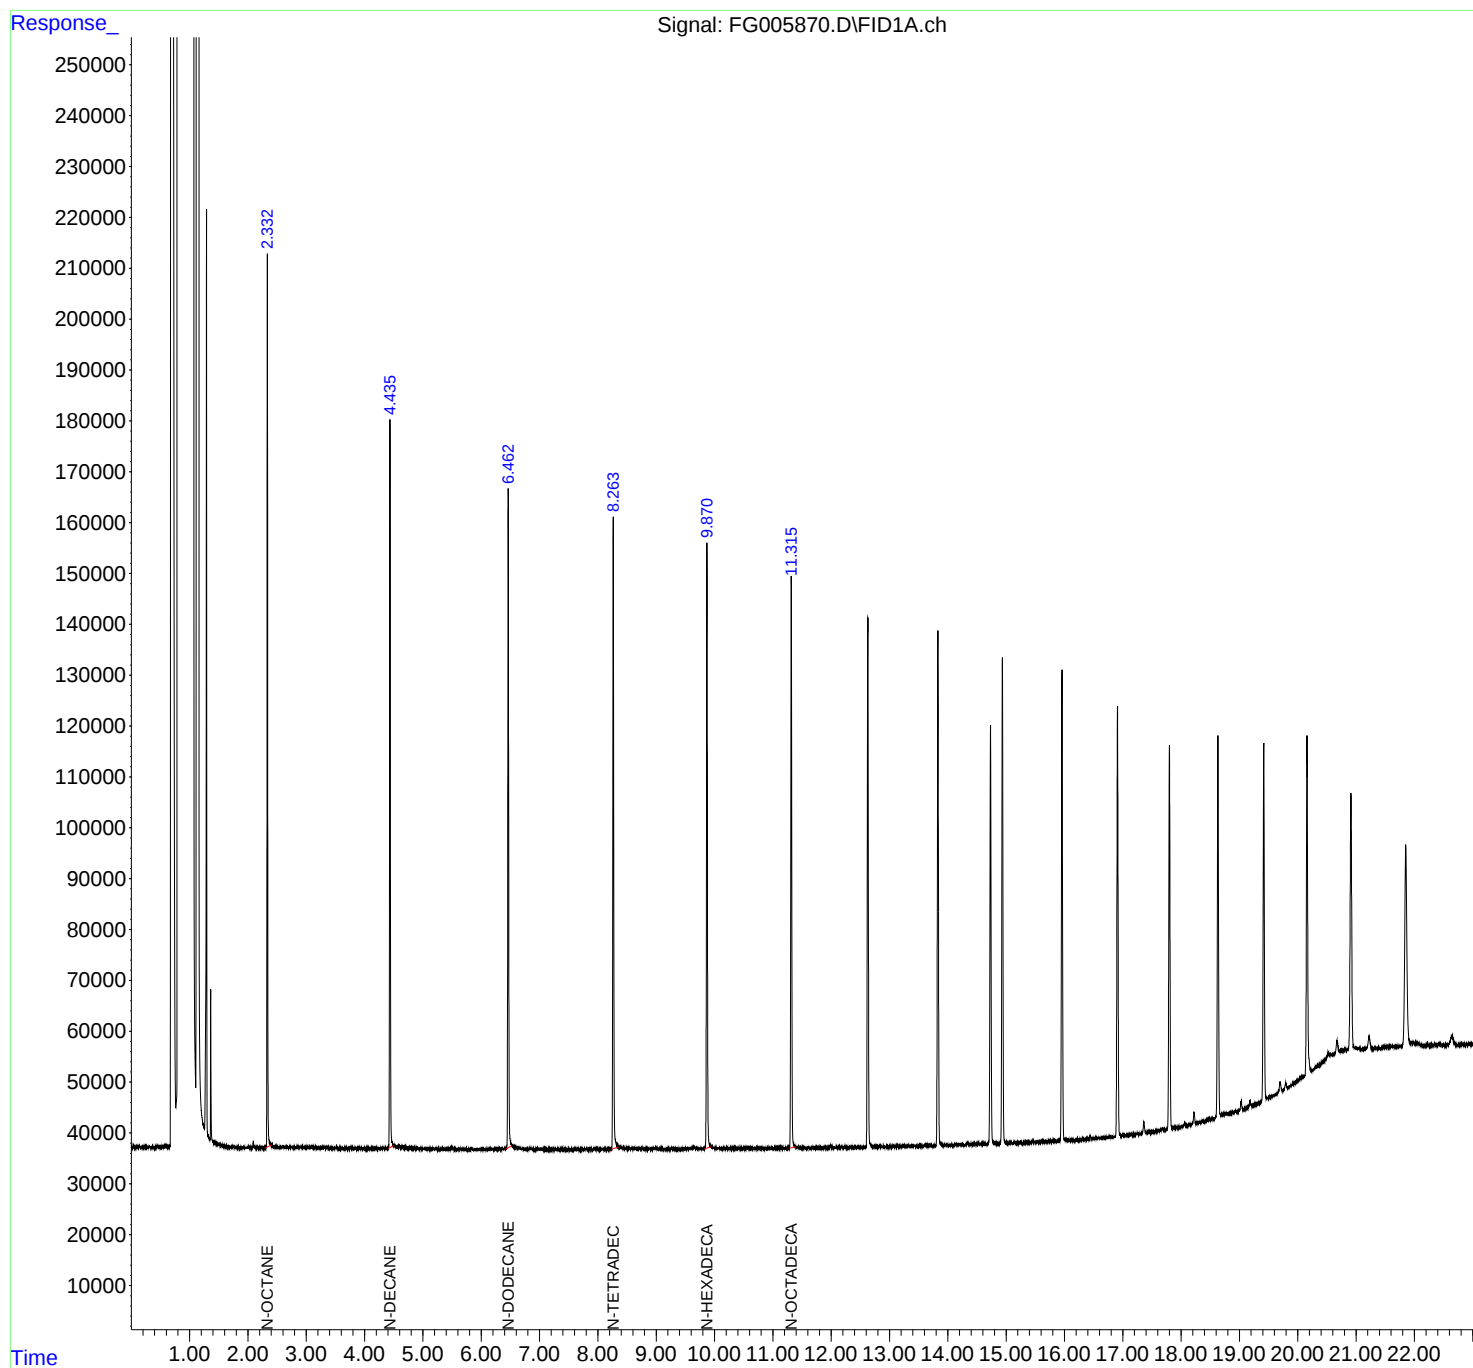


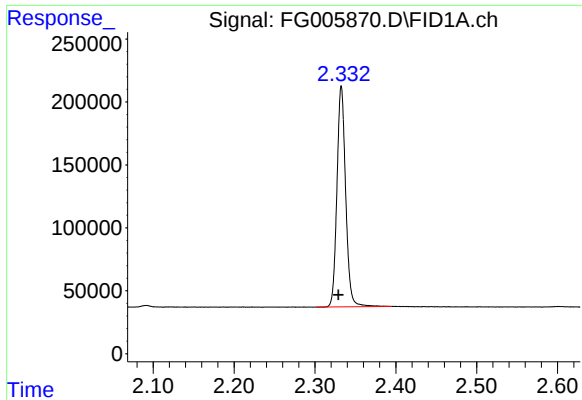

#1 N-OCTANE


R.T.: 2.333 min
Delta R.T.: 0.004 min
Response: 1313663
Conc: 9.28 ug/ml

Instrument :
FID_G
ClientSampleId :

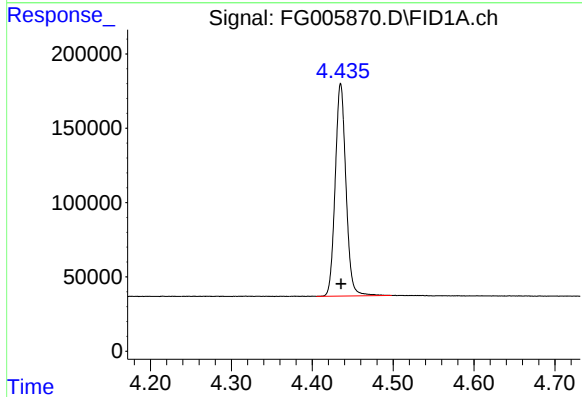


#2 N-DECANE

R.T.: 4.435 min
Delta R.T.: 0.000 min
Response: 1319946
Conc: 9.19 ug/ml

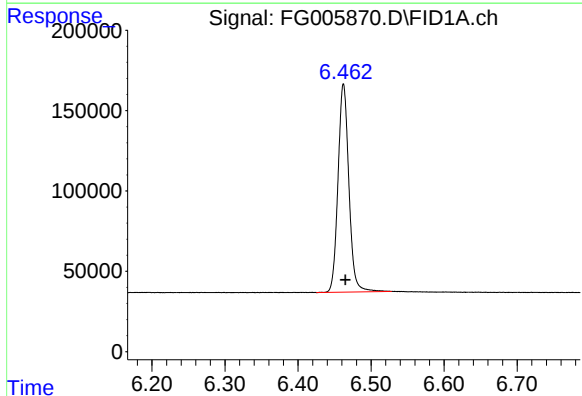


#3 N-DODECANE

R.T.: 6.462 min
Delta R.T.: -0.003 min
Response: 1336560
Conc: 9.23 ug/ml

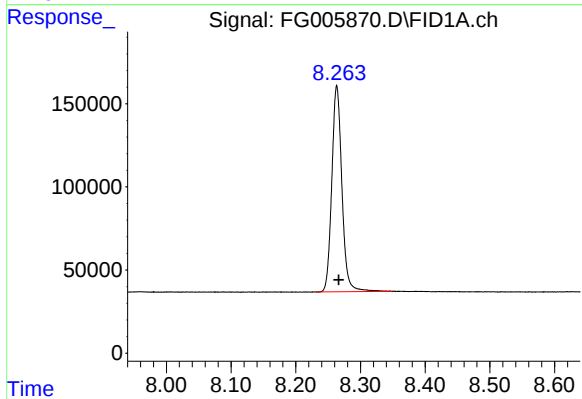

#4 N-TETRADECANE


R.T.: 8.264 min
Delta R.T.: -0.003 min
Response: 1344807
Conc: 9.35 ug/ml

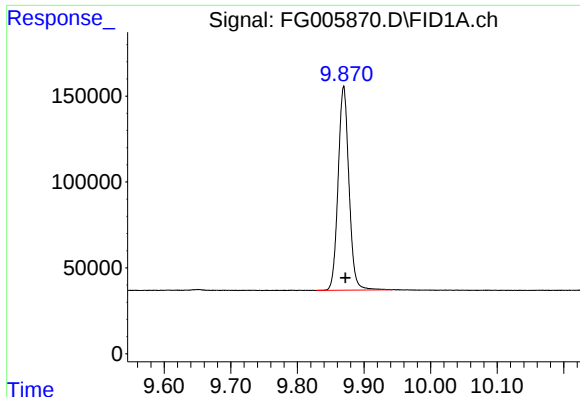

#5 N-HEXADECANE


R.T.: 9.869 min
Delta R.T.: -0.003 min
Response: 1340095
Conc: 9.40 ug/ml

Instrument :
FID_G
ClientSampleId :

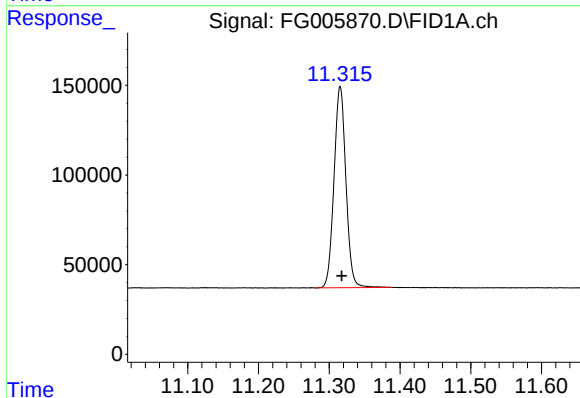

#6 N-OCTADECANE

R.T.: 11.315 min
Delta R.T.: -0.002 min
Response: 1312669
Conc: 9.47 ug/ml

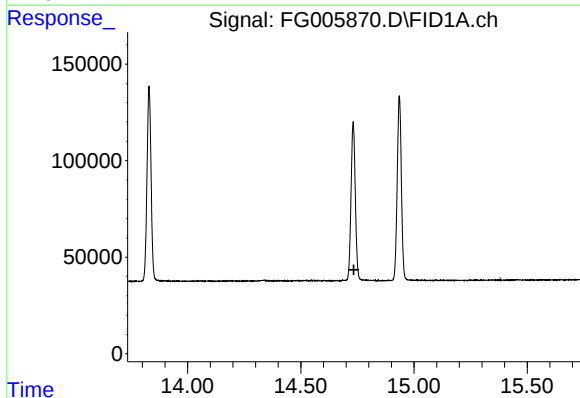

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.734 min
Response: 0
Conc: N.D.