

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG090722\
Data File : FG010518.D
Signal(s) : FID1A.ch
Acq On : 07 Sep 2022 15:58
Operator : YP\AJ
Sample : N4509-08
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
S1-SO_UNK-20220902

Integration File: autoint1.e
Quant Time: Sep 08 02:47:07 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG082622.M
Quant Title :
QLast Update : Fri Aug 26 23:48:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.779	1570232	12.830 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG090722\
Data File : FG010518.D
Signal(s) : FID1A.ch
Acq On : 07 Sep 2022 15:58
Operator : YP\AJ
Sample : N4509-08
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
S1-SO_UNK-20220902

Integration File: autoint1.e
Quant Time: Sep 08 02:47:07 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG082622.M
Quant Title :
QLast Update : Fri Aug 26 23:48:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

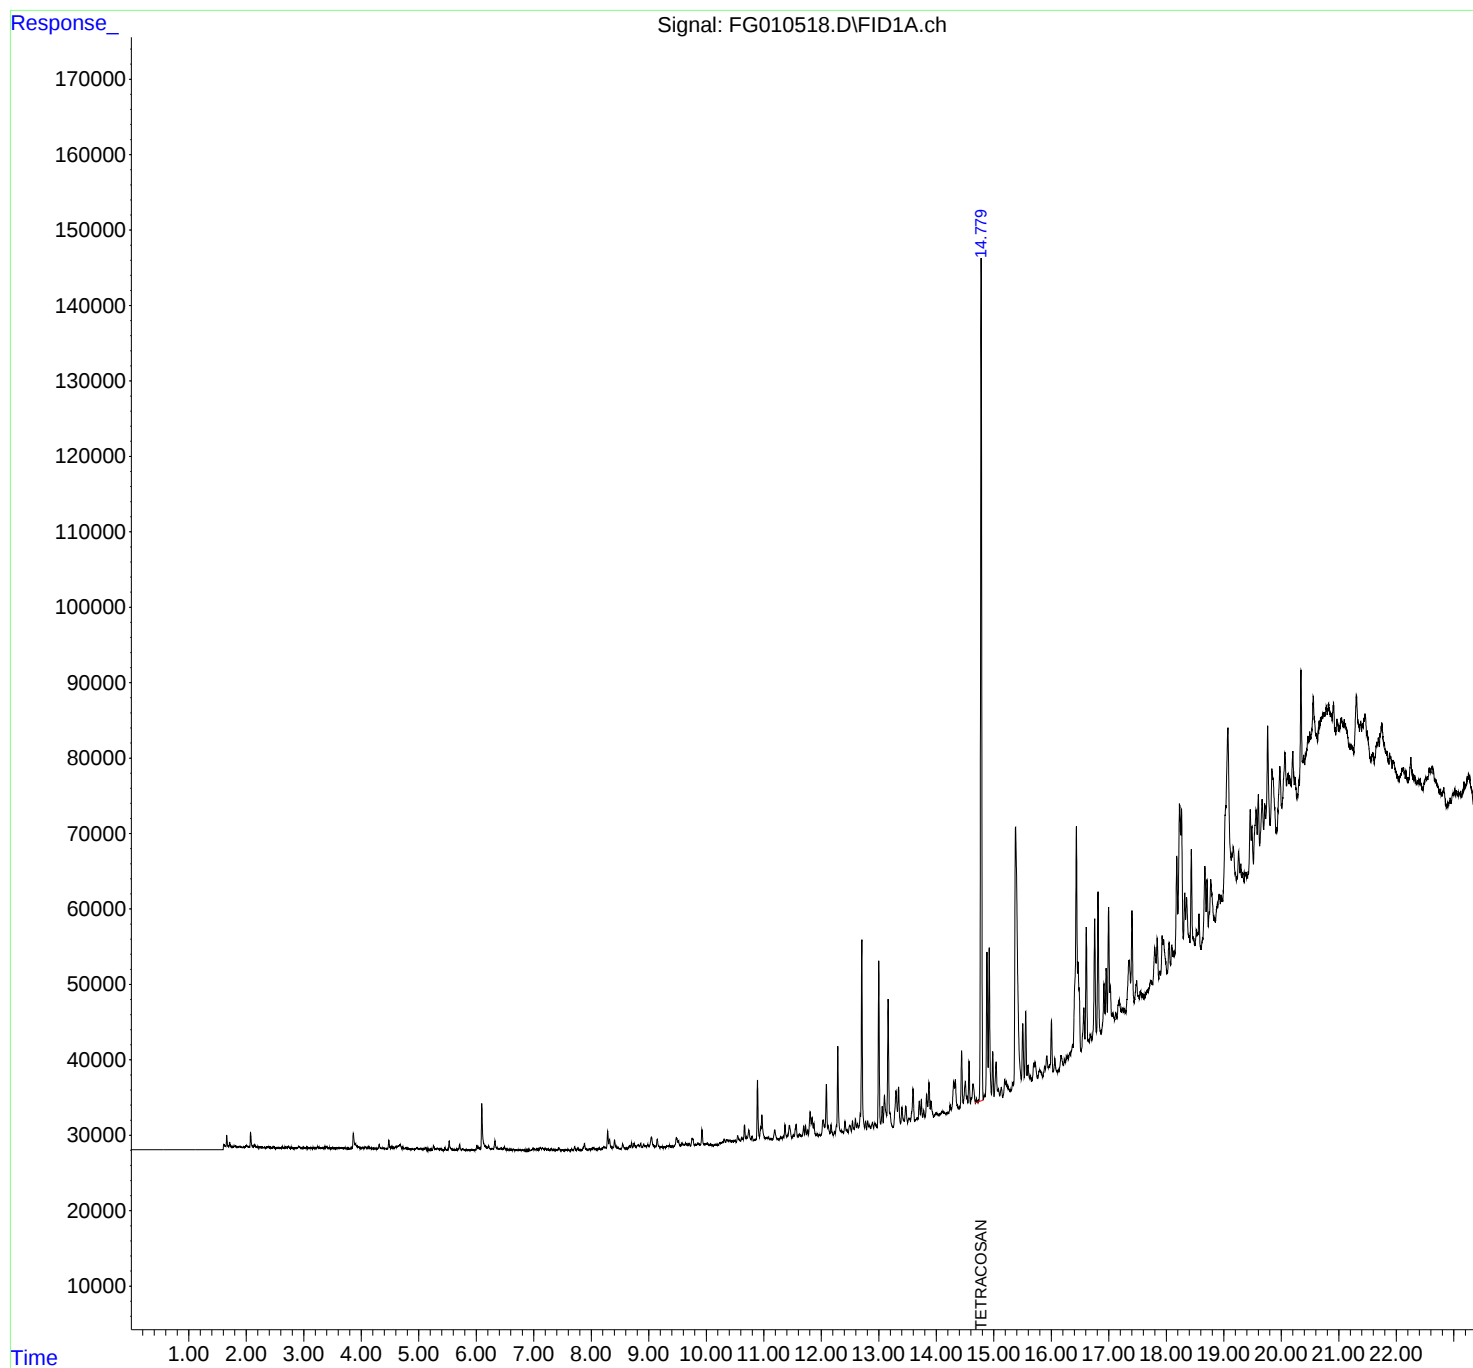

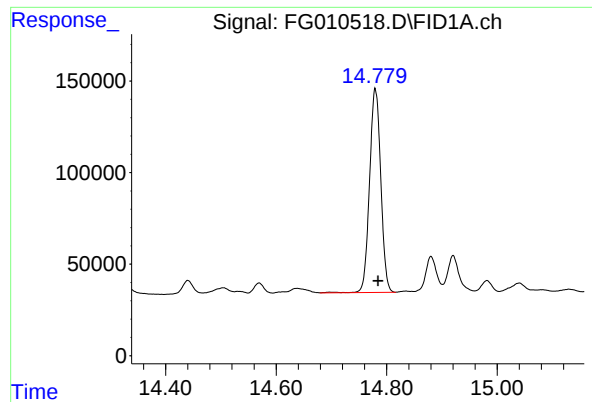

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.779 min
Delta R.T.: -0.005 min
Response: 1570232
Conc: 12.83 ug/ml

Instrument :

FID_G

ClientSampleId :

S1-SO_UNK-20220902