

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG090821\
Data File : FG008738.D
Signal(s) : FID1A.ch
Acq On : 08 Sep 2021 13:21
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 09 01:38:06 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG090721.M
Quant Title :
QLast Update : Wed Sep 08 09:33:21 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) N-DODECANE	6.473	2581288	19.057 ug/ml
12) N-OCTACOSANE	16.928	2316775	19.292 ug/ml
13) N-TRIACONTANE	17.816	60674	0.526 ug/ml
14) N-DOTRIACONTANE	18.649	77344	0.724 ug/ml
15) N-TETRATRIACONTANE	19.433	57211	0.586 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG090821\
Data File : FG008738.D
Signal(s) : FID1A.ch
Acq On : 08 Sep 2021 13:21
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 09 01:38:06 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG090721.M
Quant Title :
QLast Update : Wed Sep 08 09:33:21 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

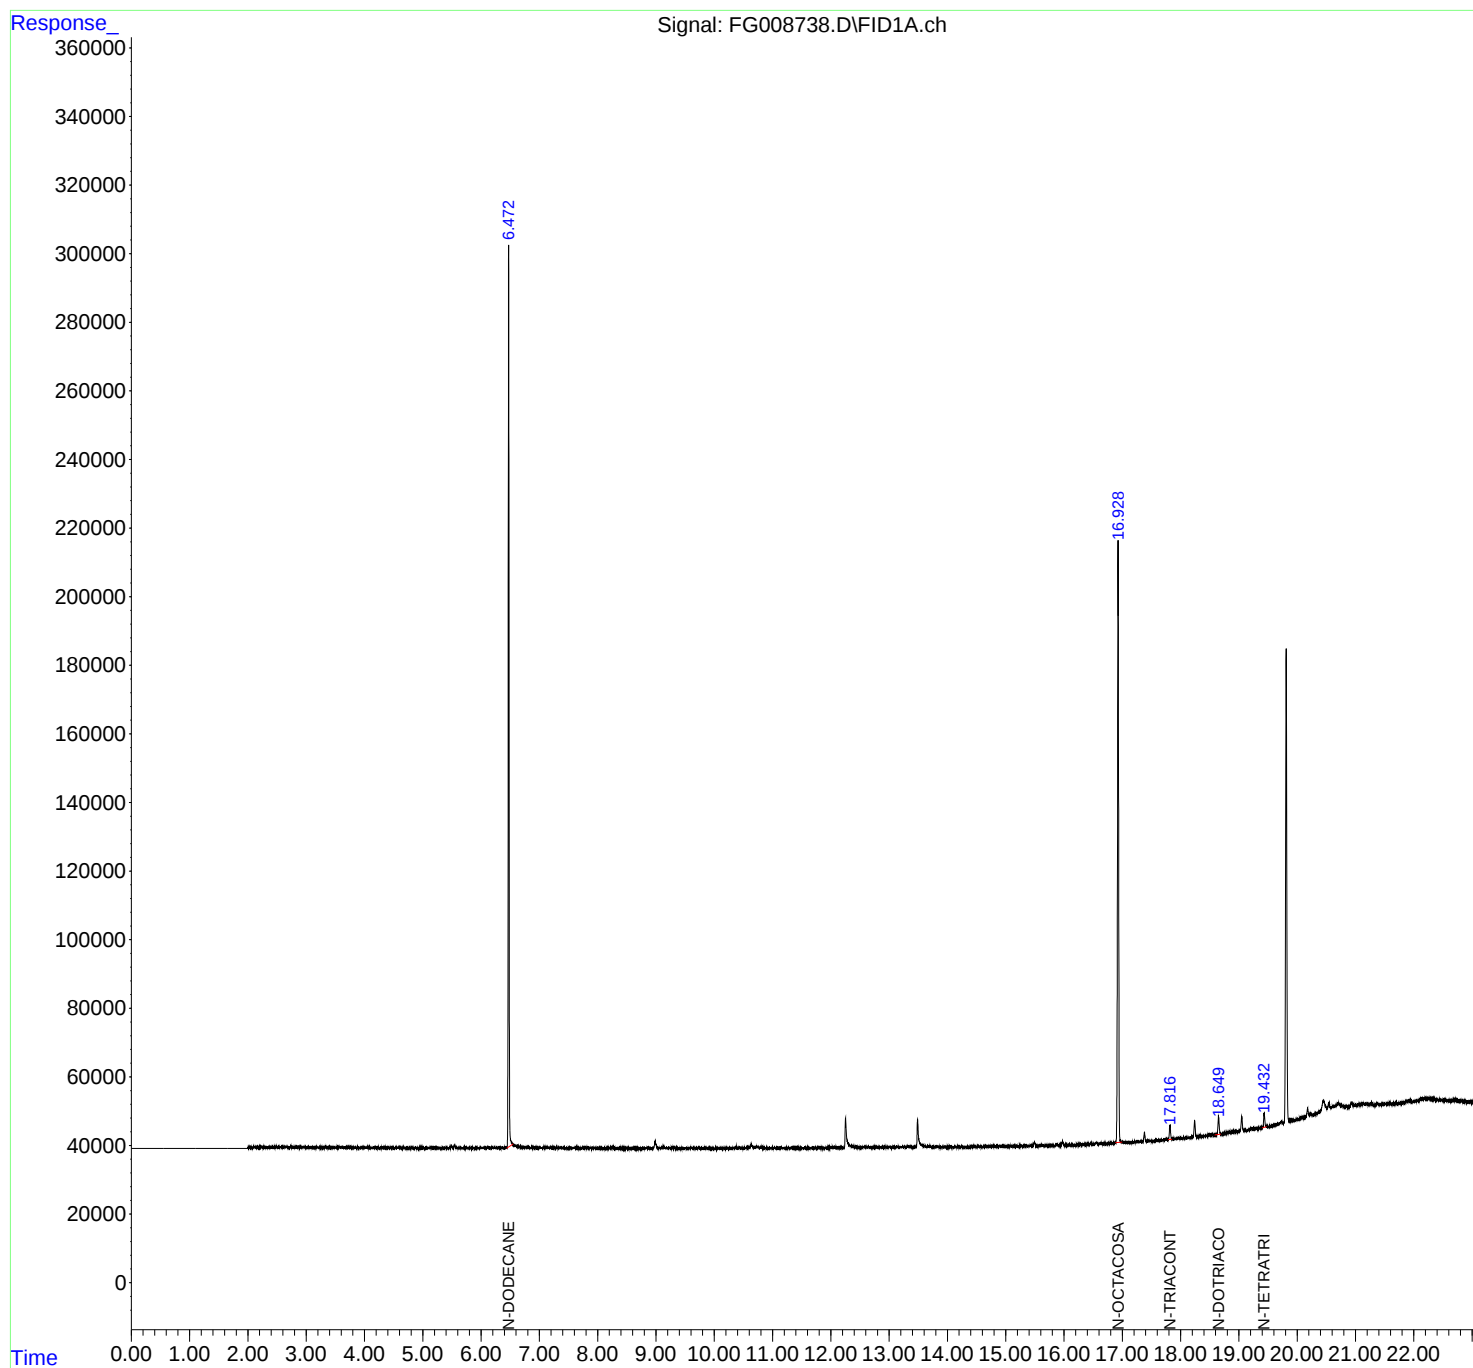


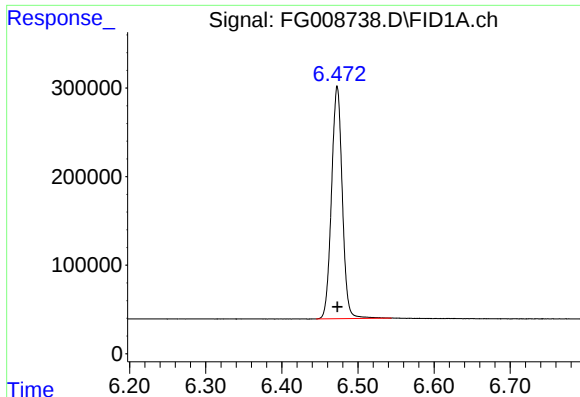

#3 N-DODECANE


R.T.: 6.473 min
Delta R.T.: 0.000 min
Response: 2581288
Conc: 19.06 ug/ml

Instrument :
FID_G
ClientSampleId :

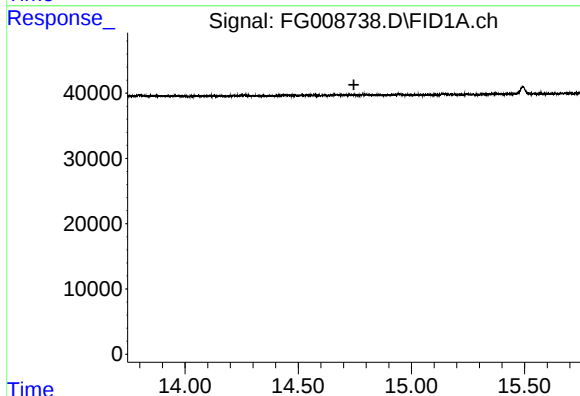


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.746 min
Response: 0
Conc: N.D.

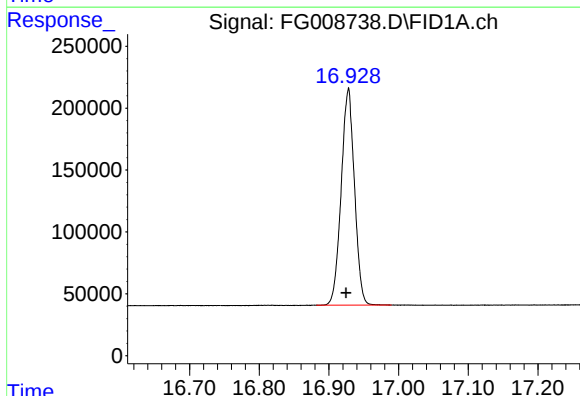


#12 N-OCTACOSANE

R.T.: 16.928 min
Delta R.T.: 0.004 min
Response: 2316775
Conc: 19.29 ug/ml

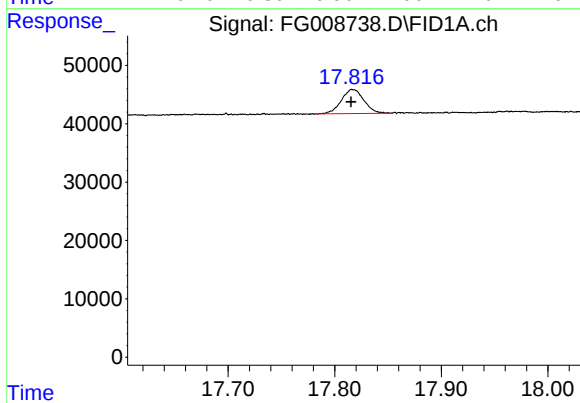

#13 N-TRIACONTANE


R.T.: 17.816 min
Delta R.T.: 0.000 min
Response: 60674
Conc: 0.53 ug/ml

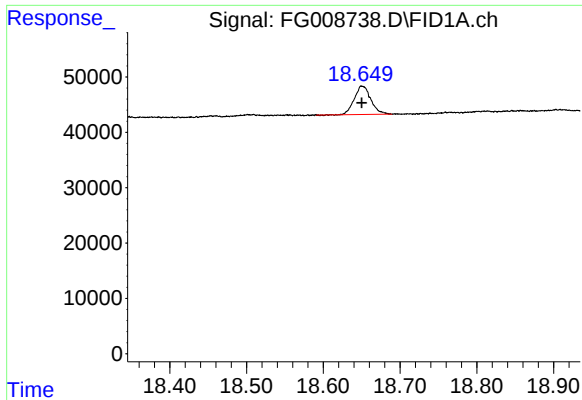

#14 N-DOTRIACONTANE

R.T.: 18.649 min
Delta R.T.: 0.000 min
Response: 77344
Conc: 0.72 ug/ml

Instrument :
FID_G
ClientSampleId :

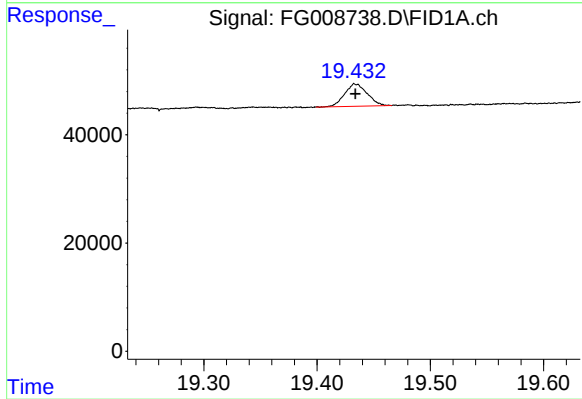

#15 N-TETRATRIACONTANE

R.T.: 19.433 min
Delta R.T.: -0.001 min
Response: 57211
Conc: 0.59 ug/ml