

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG090821\
Data File : FG008739.D
Signal(s) : FID1A.ch
Acq On : 08 Sep 2021 13:52
Operator : DD\AJ
Sample : PB138975BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
PB138975BL

Integration File: autoint1.e
Quant Time: Sep 09 01:38:17 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG090721.M
Quant Title :
QLast Update : Wed Sep 08 09:33:21 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.745	1744516	15.707 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG090821\
Data File : FG008739.D
Signal(s) : FID1A.ch
Acq On : 08 Sep 2021 13:52
Operator : DD\AJ
Sample : PB138975BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
PB138975BL

Integration File: autoint1.e
Quant Time: Sep 09 01:38:17 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG090721.M
Quant Title :
QLast Update : Wed Sep 08 09:33:21 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

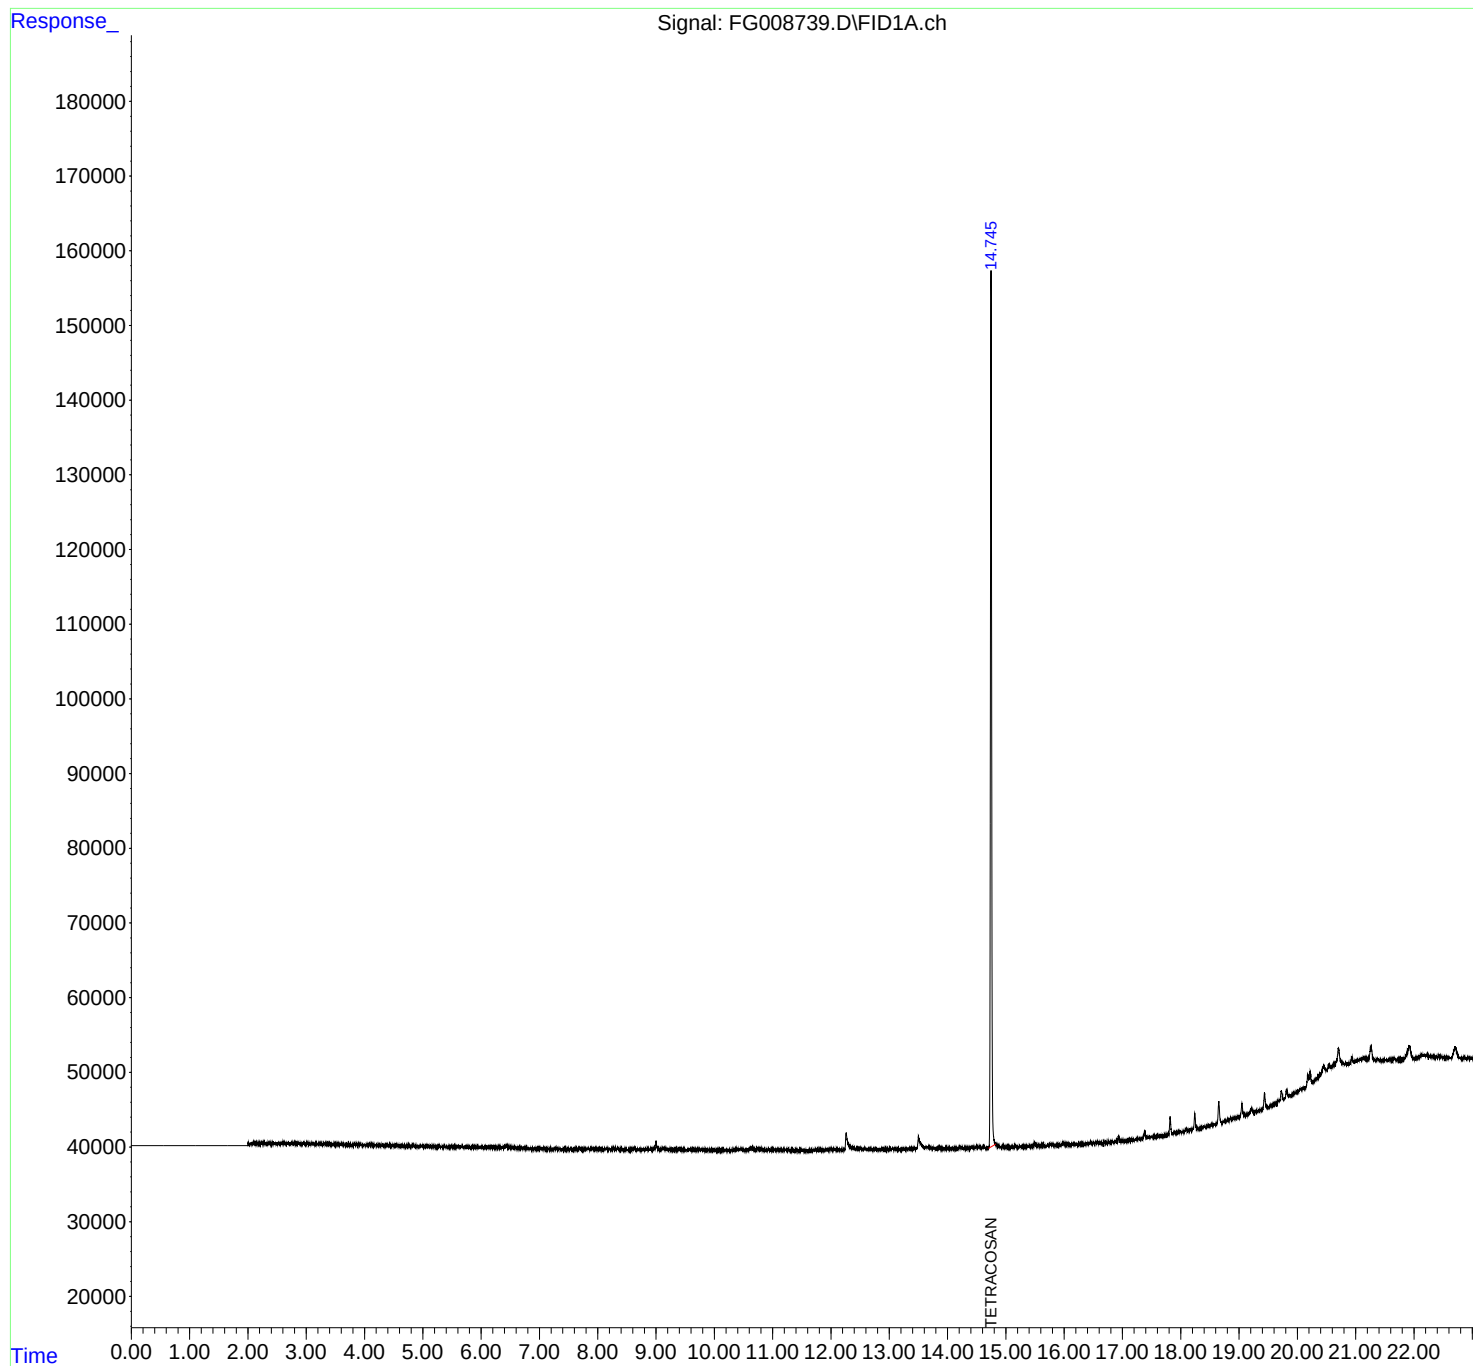

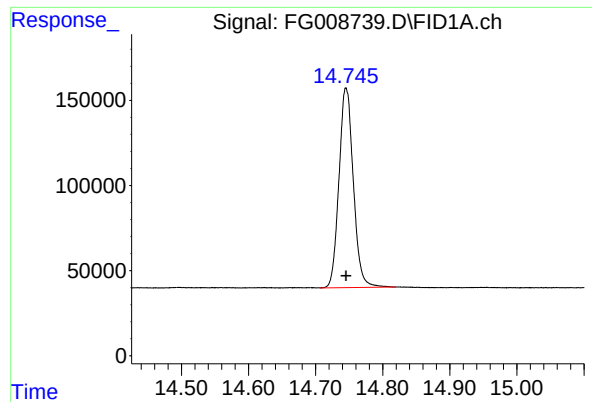

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.745 min
Delta R.T.: 0.000 min
Response: 1744516
Conc: 15.71 ug/ml

Instrument :
FID_G
ClientSampleId :
PB138975BL