

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG090822\
Data File : FG010536.D
Signal(s) : FID1A.ch
Acq On : 08 Sep 2022 22:08
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
RT MARKER

Integration File: Sample.e
Quant Time: Sep 09 07:57:26 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG082622.M
Quant Title :
QLast Update : Fri Aug 26 23:48:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) N-DODECANE	6.491	2356064	17.902 ug/ml
12) N-OCTACOSANE	16.958	2280389	17.244 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG090822\
Data File : FG010536.D
Signal(s) : FID1A.ch
Acq On : 08 Sep 2022 22:08
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
RT MARKER

Integration File: Sample.e
Quant Time: Sep 09 07:57:26 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG082622.M
Quant Title :
QLast Update : Fri Aug 26 23:48:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

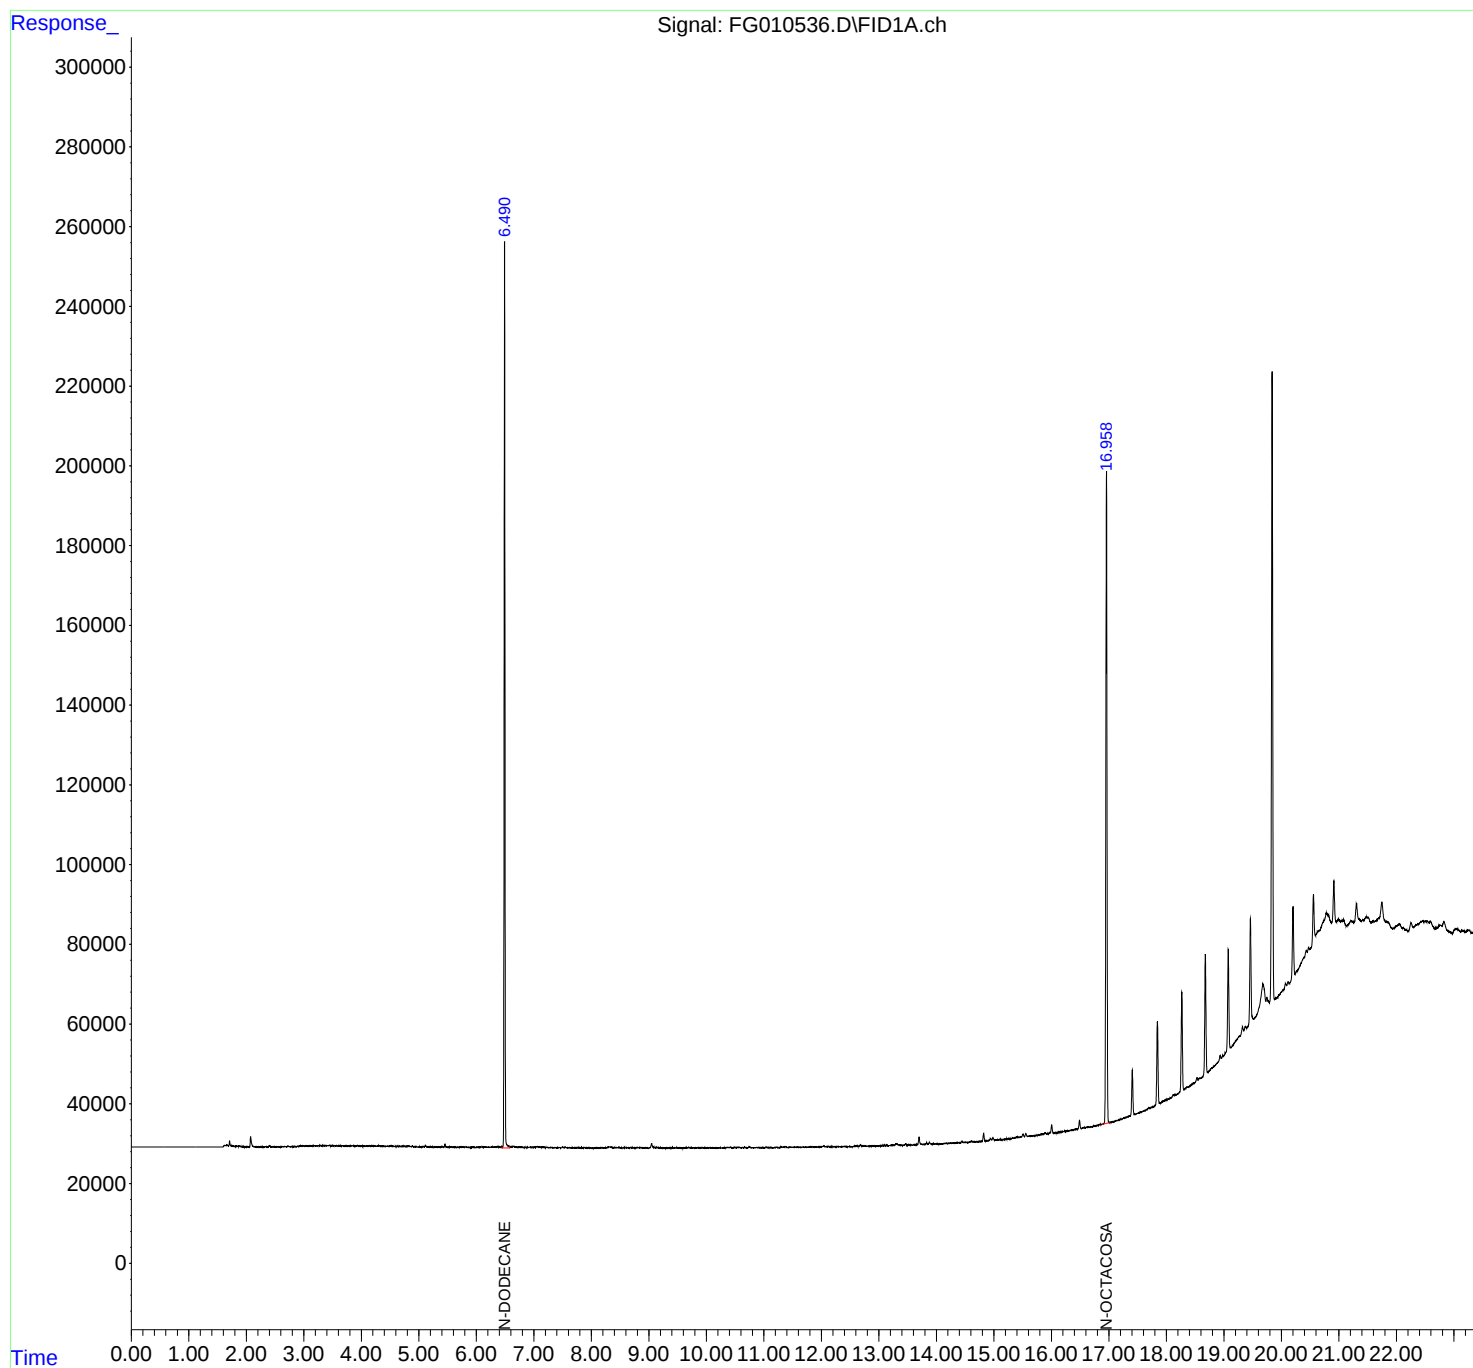


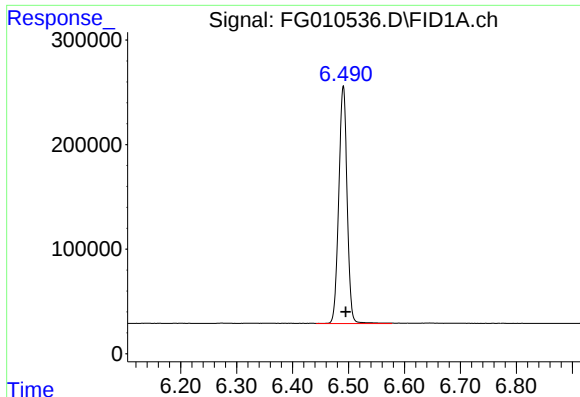

#3 N-DODECANE


R.T.: 6.491 min
Delta R.T.: -0.005 min
Response: 2356064
Conc: 17.90 ug/ml

Instrument :
FID_G
ClientSampleId :
RT MARKER

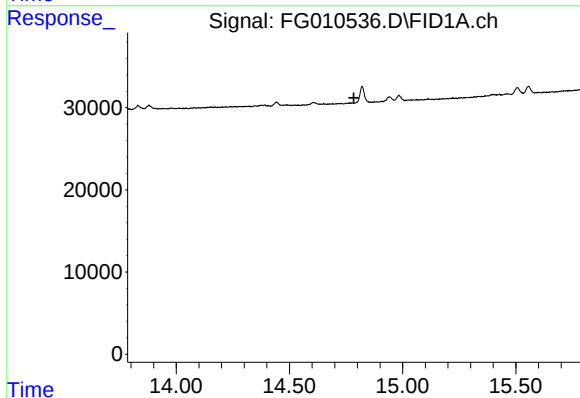

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.785 min
Response: 0
Conc: N.D.

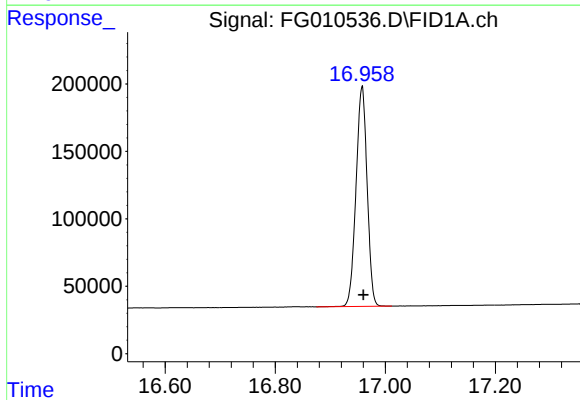

#12 N-OCTACOSANE

R.T.: 16.958 min
Delta R.T.: -0.003 min
Response: 2280389
Conc: 17.24 ug/ml