

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG090919\
 Data File : FG005881.D
 Signal(s) : FID1A.ch
 Acq On : 09 Sep 2019 12:30
 Operator : DD\AJ
 Sample : K4636-06
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Sep 10 02:06:28 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG090719.M
 Quant Title :
 QLast Update : Mon Sep 09 05:03:58 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.734	1992348	17.734 ug/ml
Target Compounds			
4) N-TETRADECANE	8.329f	693850	4.921 ug/ml
5) N-HEXADECANE	9.890	236207	1.681 ug/ml
7) N-EICOSANE	12.628	561951	4.139 ug/ml
8) N-DOCOSANE	13.784	517503	3.934 ug/ml
10) N-TETRACOSANE	14.949	7981309	62.584 ug/ml
11) N-HEXACOSANE	15.959	1735149	14.160 ug/ml
12) N-OCTACOSANE	16.912	357754	3.034 ug/ml
13) N-TRIACONTANE	17.806	1019928	9.001 ug/ml
14) N-DOTRIACONTANE	18.634	2149329	20.082 ug/ml
15) N-TETRATRIACONTANE	19.424	220999	2.137 ug/ml
16) N-HEXATRIACONTANE	20.154	650392	6.528 ug/ml
18) N-TETRACONTANE	21.851	853704	8.693 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG090919\
Data File : FG005881.D
Signal(s) : FID1A.ch
Acq On : 09 Sep 2019 12:30
Operator : DD\AJ
Sample : K4636-06
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 10 02:06:28 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG090719.M
Quant Title :
QLast Update : Mon Sep 09 05:03:58 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

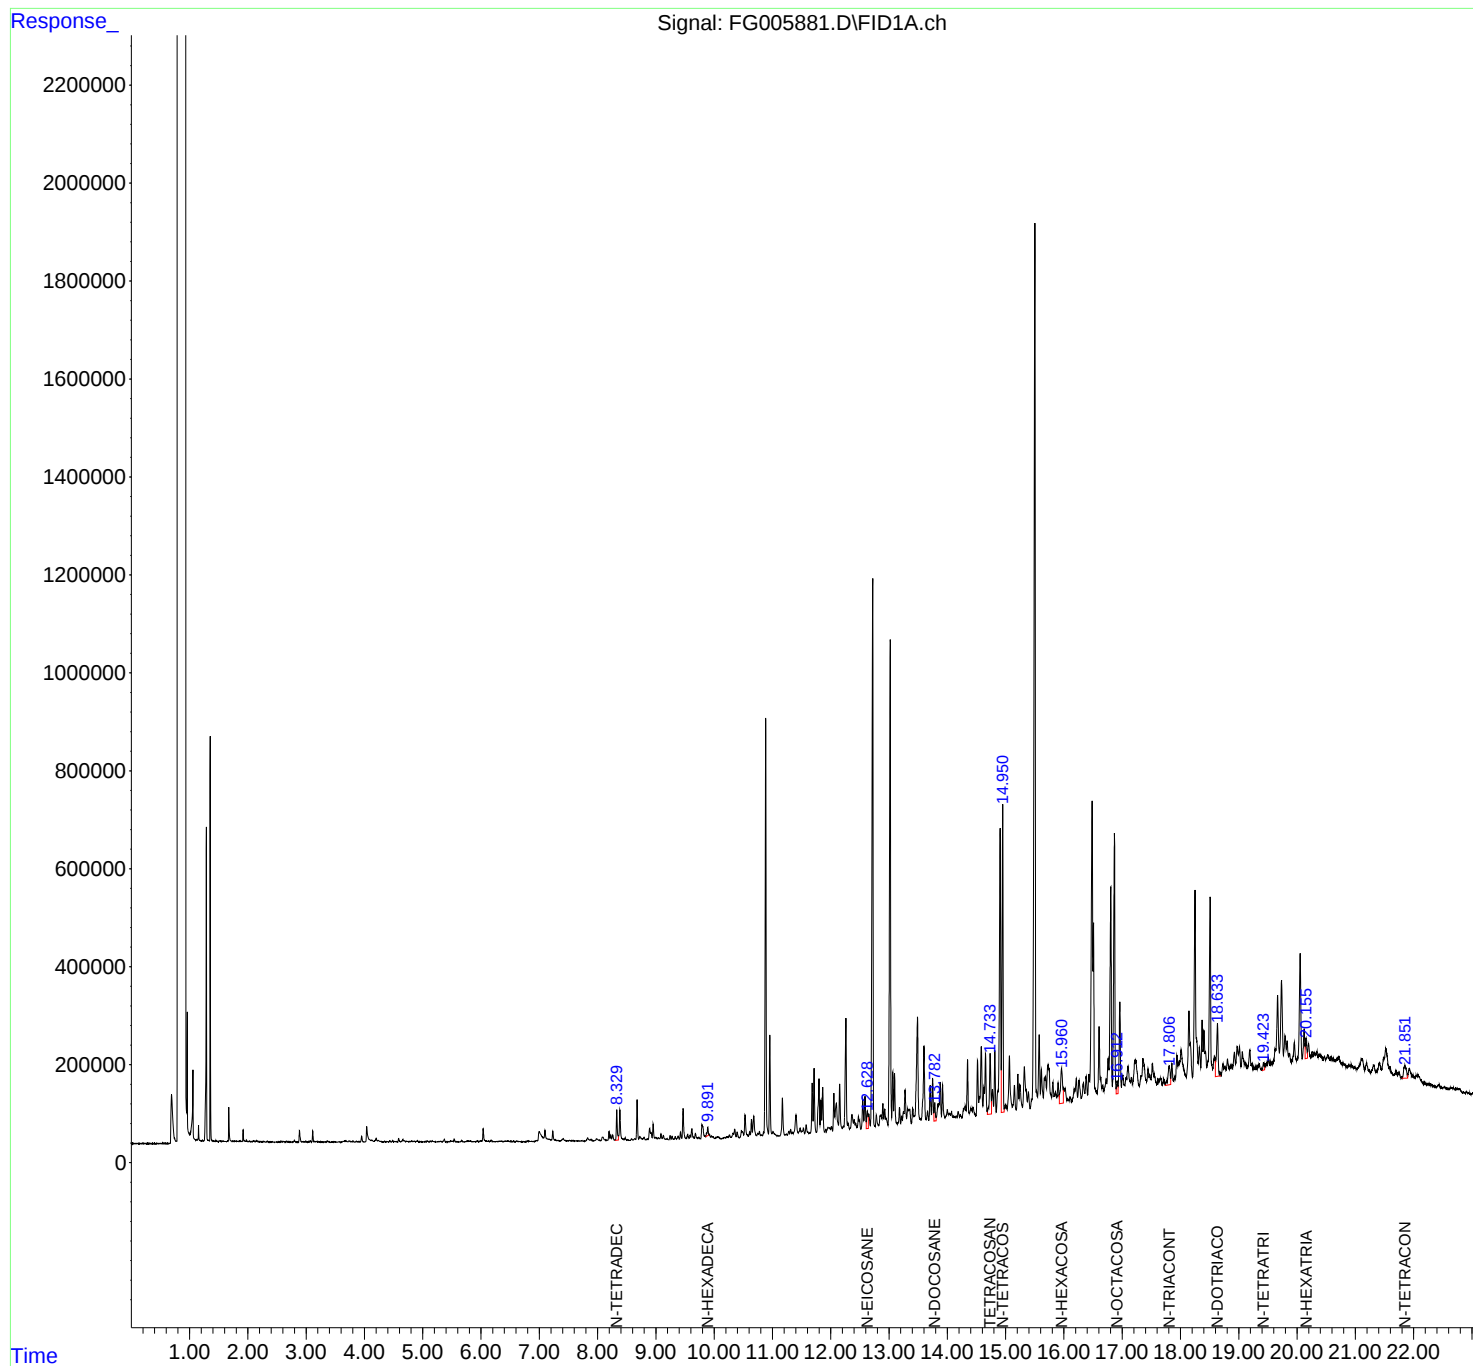


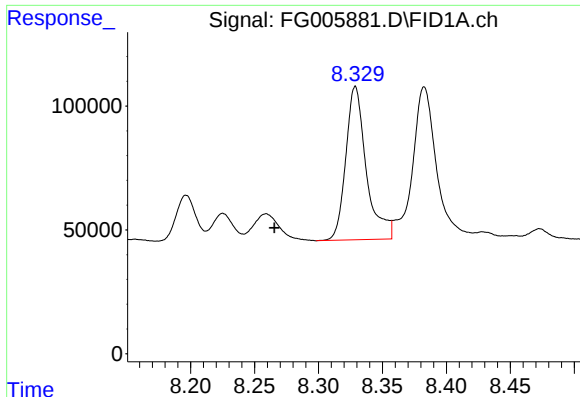

#4 N-TETRADECANE


R.T.: 8.329 min
Delta R.T.: 0.063 min
Response: 693850
Conc: 4.92 ug/ml

Instrument :
FID_G
ClientSampleId :

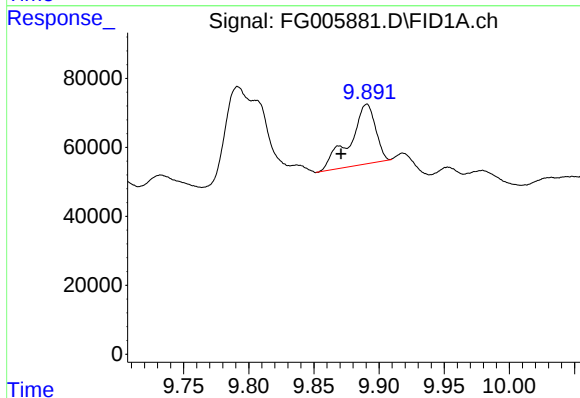


#5 N-HEXADECANE

R.T.: 9.890 min
Delta R.T.: 0.020 min
Response: 236207
Conc: 1.68 ug/ml

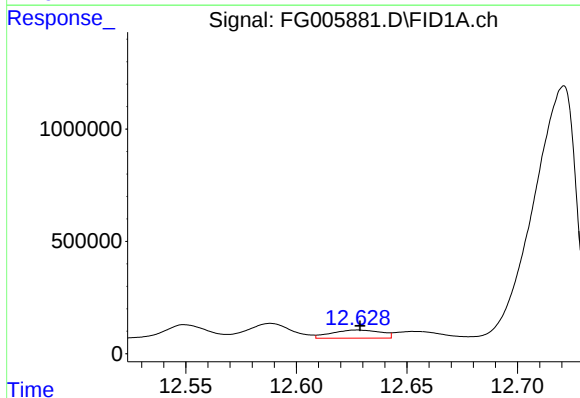


#7 N-EICOSANE

R.T.: 12.628 min
Delta R.T.: 0.000 min
Response: 561951
Conc: 4.14 ug/ml

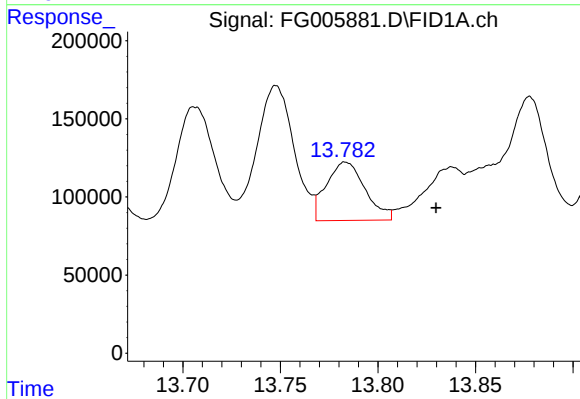

#8 N-DOCOSANE


R.T.: 13.784 min
Delta R.T.: -0.046 min
Response: 517503
Conc: 3.93 ug/ml

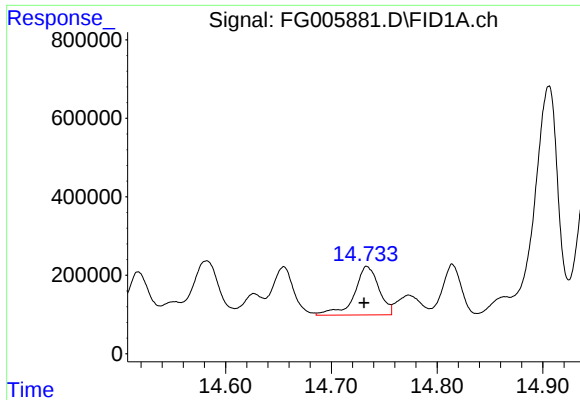

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.734 min
Delta R.T.: 0.003 min
Response: 1992348
Conc: 17.73 ug/ml

Instrument :
FID_G
ClientSampleId :

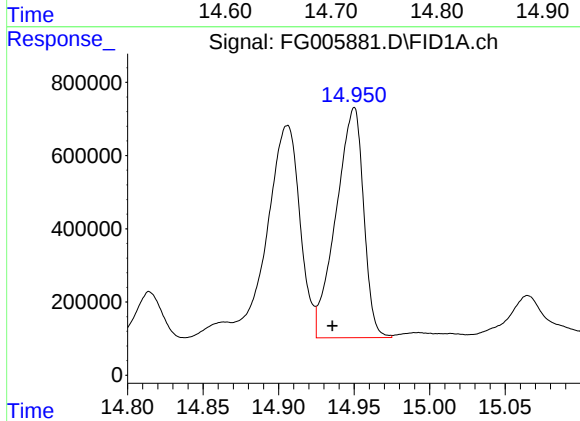


#10 N-TETRACOSANE

R.T.: 14.949 min
Delta R.T.: 0.014 min
Response: 7981309
Conc: 62.58 ug/ml

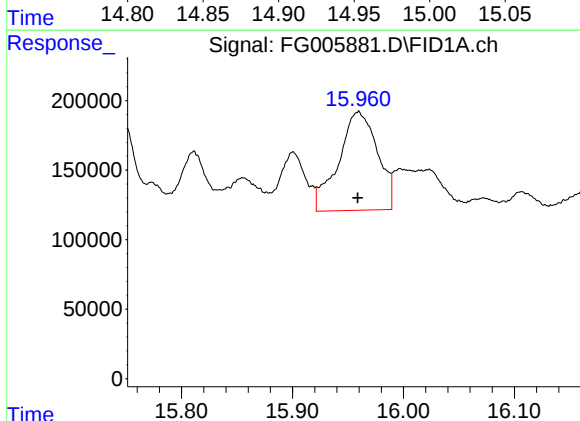


#11 N-HEXACOSANE

R.T.: 15.959 min
Delta R.T.: 0.000 min
Response: 1735149
Conc: 14.16 ug/ml

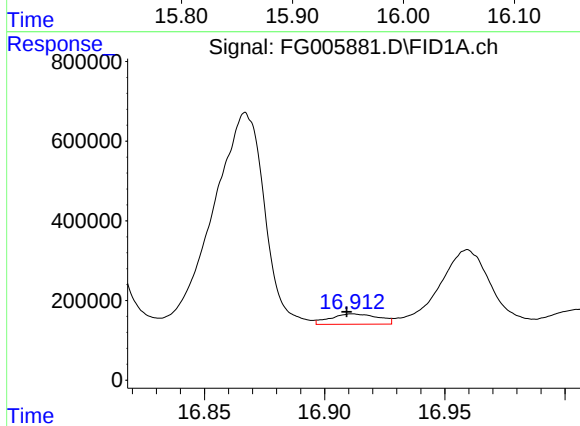

#12 N-OCTACOSANE


R.T.: 16.912 min
Delta R.T.: 0.003 min
Response: 357754
Conc: 3.03 ug/ml

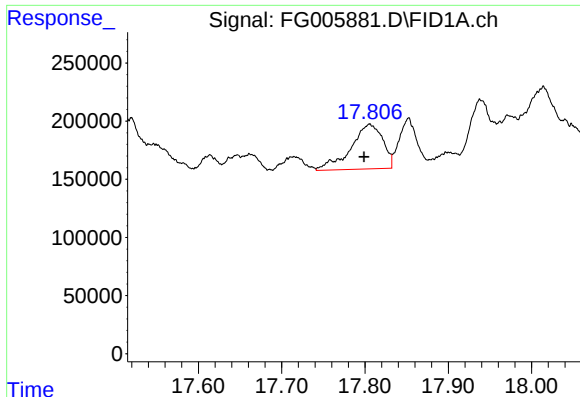

#13 N-TRIACONTANE


R.T.: 17.806 min
Delta R.T.: 0.007 min
Response: 1019928
Conc: 9.00 ug/ml

Instrument :
FID_G
ClientSampleId :

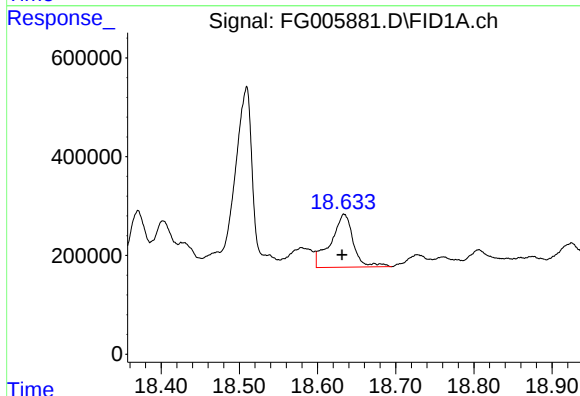


#14 N-DOTRIACONTANE

R.T.: 18.634 min
Delta R.T.: 0.003 min
Response: 2149329
Conc: 20.08 ug/ml

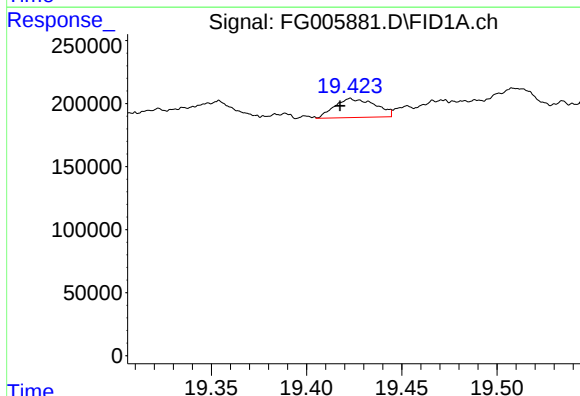


#15 N-TETRATRIACONTANE

R.T.: 19.424 min
Delta R.T.: 0.007 min
Response: 220999
Conc: 2.14 ug/ml

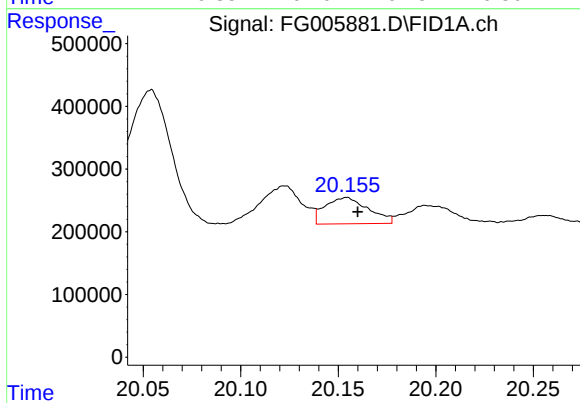

#16 N-HEXATRIACONTANE

R.T.: 20.154 min
Delta R.T.: -0.006 min
Response: 650392
Conc: 6.53 ug/ml

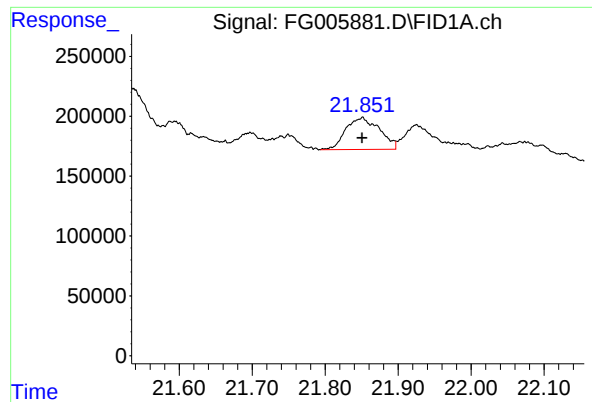

#18 N-TETRACONTANE

R.T.: 21.851 min
Delta R.T.: 0.000 min
Response: 853704
Conc: 8.69 ug/ml

Instrument :
FID_G
ClientSampleId :