

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG090919\
Data File : FG005886.D
Signal(s) : FID1A.ch
Acq On : 09 Sep 2019 15:03
Operator : DD\AJ
Sample : K4658-01 10X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 10 02:08:13 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG090719.M
Quant Title :
QLast Update : Mon Sep 09 05:03:58 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
13)	N-TRIACONTANE	17.803	76925	0.679 ug/ml
15)	N-TETRATRIACONTANE	19.434	424336	4.102 ug/ml
16)	N-HEXATRIACONTANE	20.197	1117935	11.221 ug/ml
18)	N-TETRACONTANE	21.878	581748	5.924 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG090919\
Data File : FG005886.D
Signal(s) : FID1A.ch
Acq On : 09 Sep 2019 15:03
Operator : DD\AJ
Sample : K4658-01 10X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 10 02:08:13 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG090719.M
Quant Title :
QLast Update : Mon Sep 09 05:03:58 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

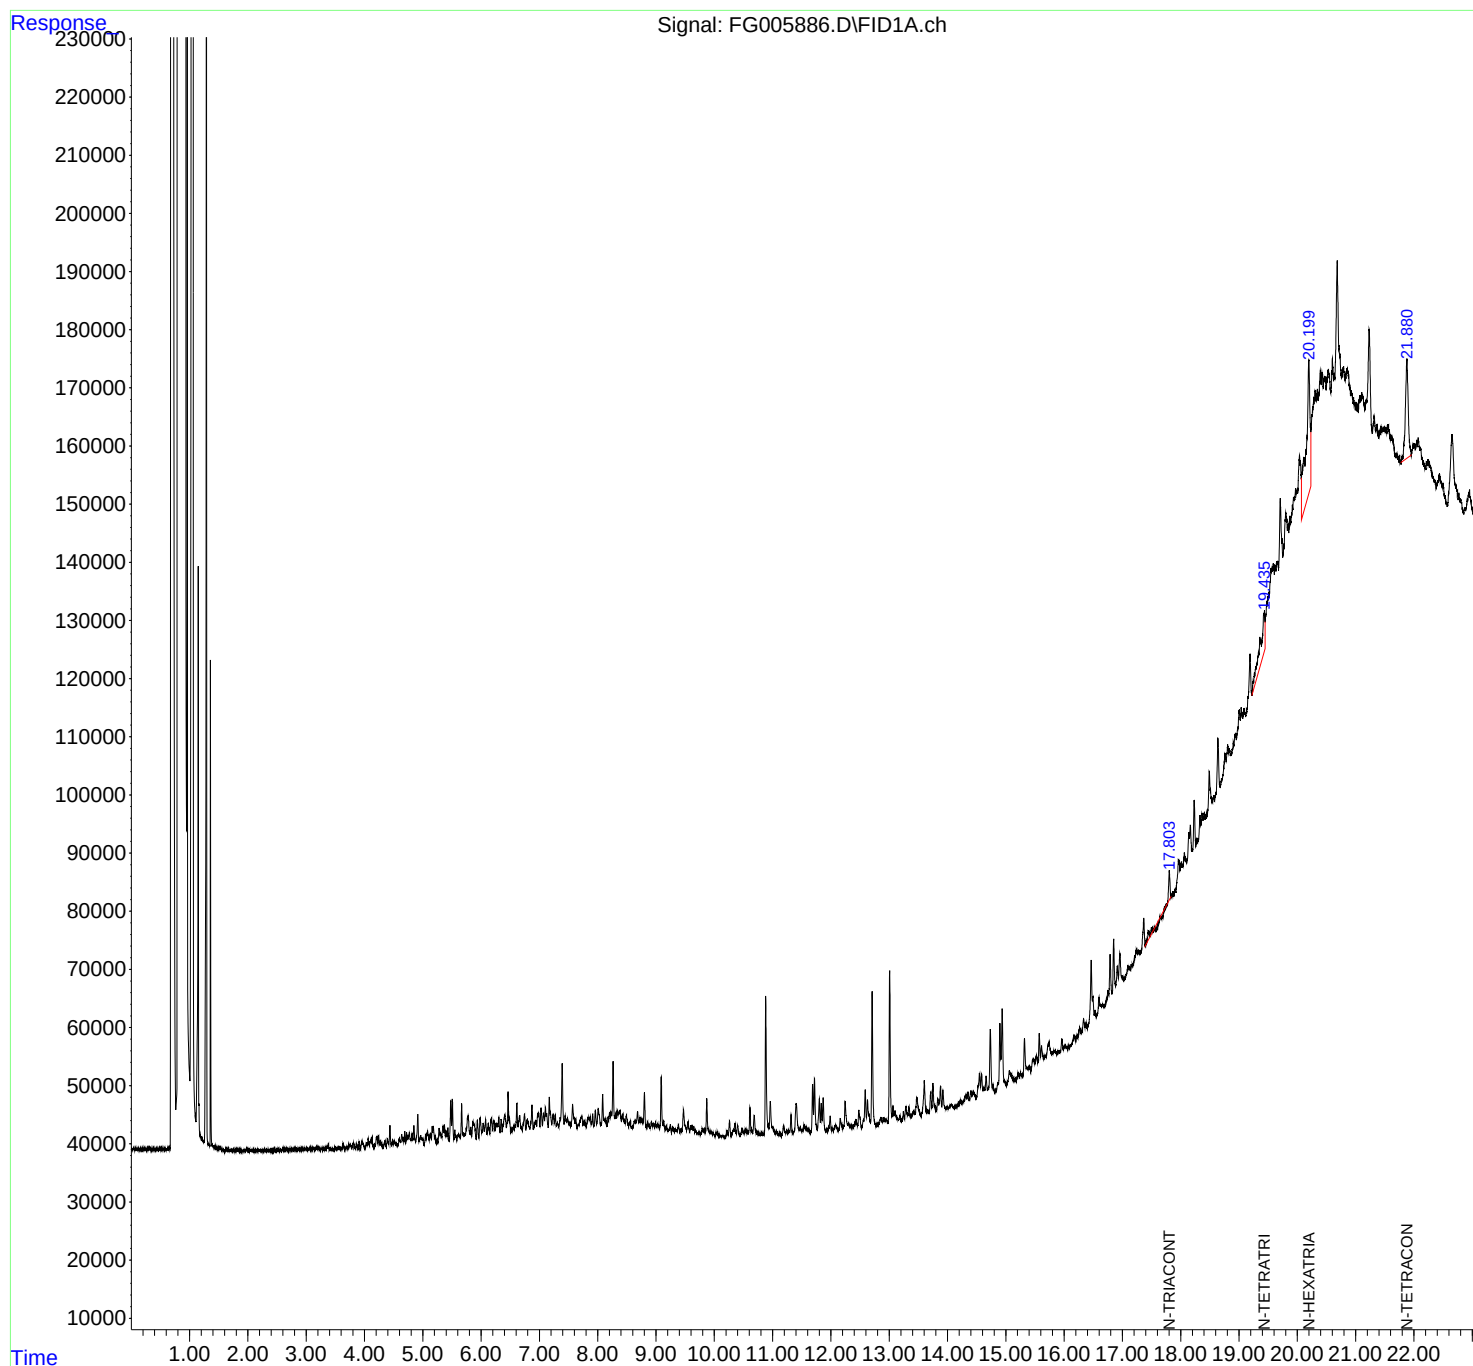


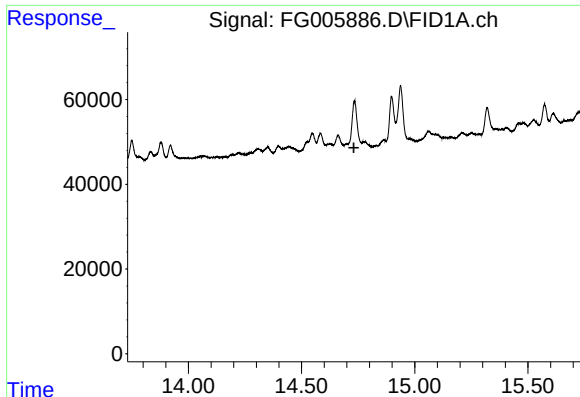

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.731 min
Response: 0
Conc: N.D.

Instrument :
FID_G
ClientSampleId :

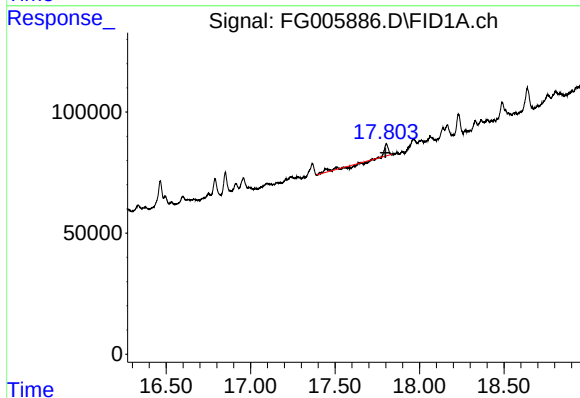


#13 N-TRIACONTANE

R.T.: 17.803 min
Delta R.T.: 0.005 min
Response: 76925
Conc: 0.68 ug/ml

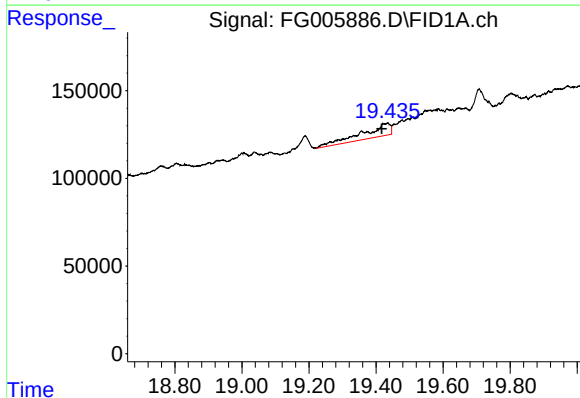


#15 N-TETRATRIACONTANE

R.T.: 19.434 min
Delta R.T.: 0.017 min
Response: 424336
Conc: 4.10 ug/ml

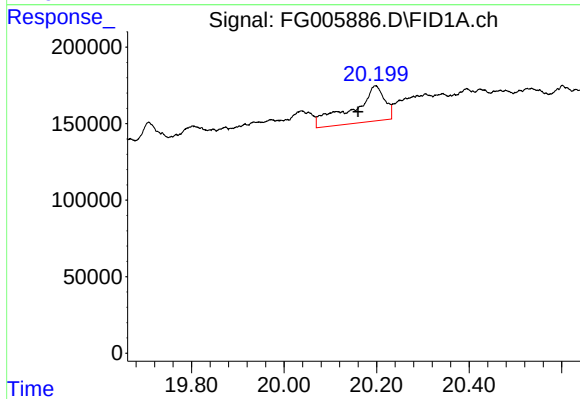

#16 N-HEXATRIACONTANE

R.T.: 20.197 min
Delta R.T.: 0.037 min
Response: 1117935
Conc: 11.22 ug/ml

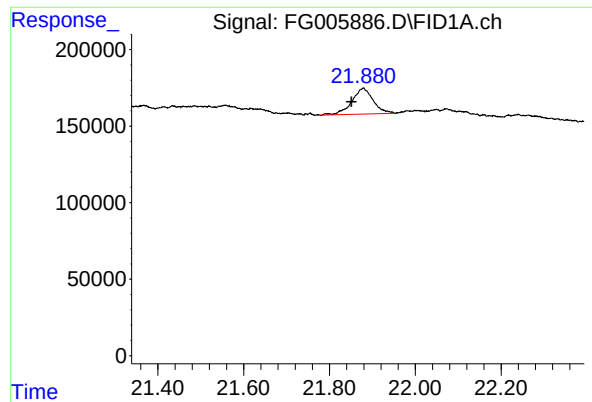

#18 N-TETRACONTANE

R.T.: 21.878 min
Delta R.T.: 0.027 min
Response: 581748
Conc: 5.92 ug/ml

Instrument :
FID_G
ClientSampleId :