

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG090919\
 Data File : FG005899.D
 Signal(s) : FID1A.ch
 Acq On : 09 Sep 2019 21:34
 Operator : DD\AJ
 Sample : K4658-01 5X
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Sep 10 02:12:11 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG090719.M
 Quant Title :
 QLast Update : Mon Sep 09 05:03:58 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.733	295023	2.626 ug/ml
Target Compounds			
3) N-DODECANE	6.463	230829	1.630 ug/ml
4) N-TETRADECANE	8.264	278621	1.976 ug/ml
7) N-EICOSANE	12.589	132039	0.972 ug/ml
10) N-TETRACOSANE	14.938	406770	3.190 ug/ml
12) N-OCTACOSANE	16.849f	239736	2.033 ug/ml
14) N-DOTRIACONTANE	18.635	271062	2.533 ug/ml
16) N-HEXATRIACONTANE	20.171	247188	2.481 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG090919\
Data File : FG005899.D
Signal(s) : FID1A.ch
Acq On : 09 Sep 2019 21:34
Operator : DD\AJ
Sample : K4658-01 5X
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 10 02:12:11 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG090719.M
Quant Title :
QLast Update : Mon Sep 09 05:03:58 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

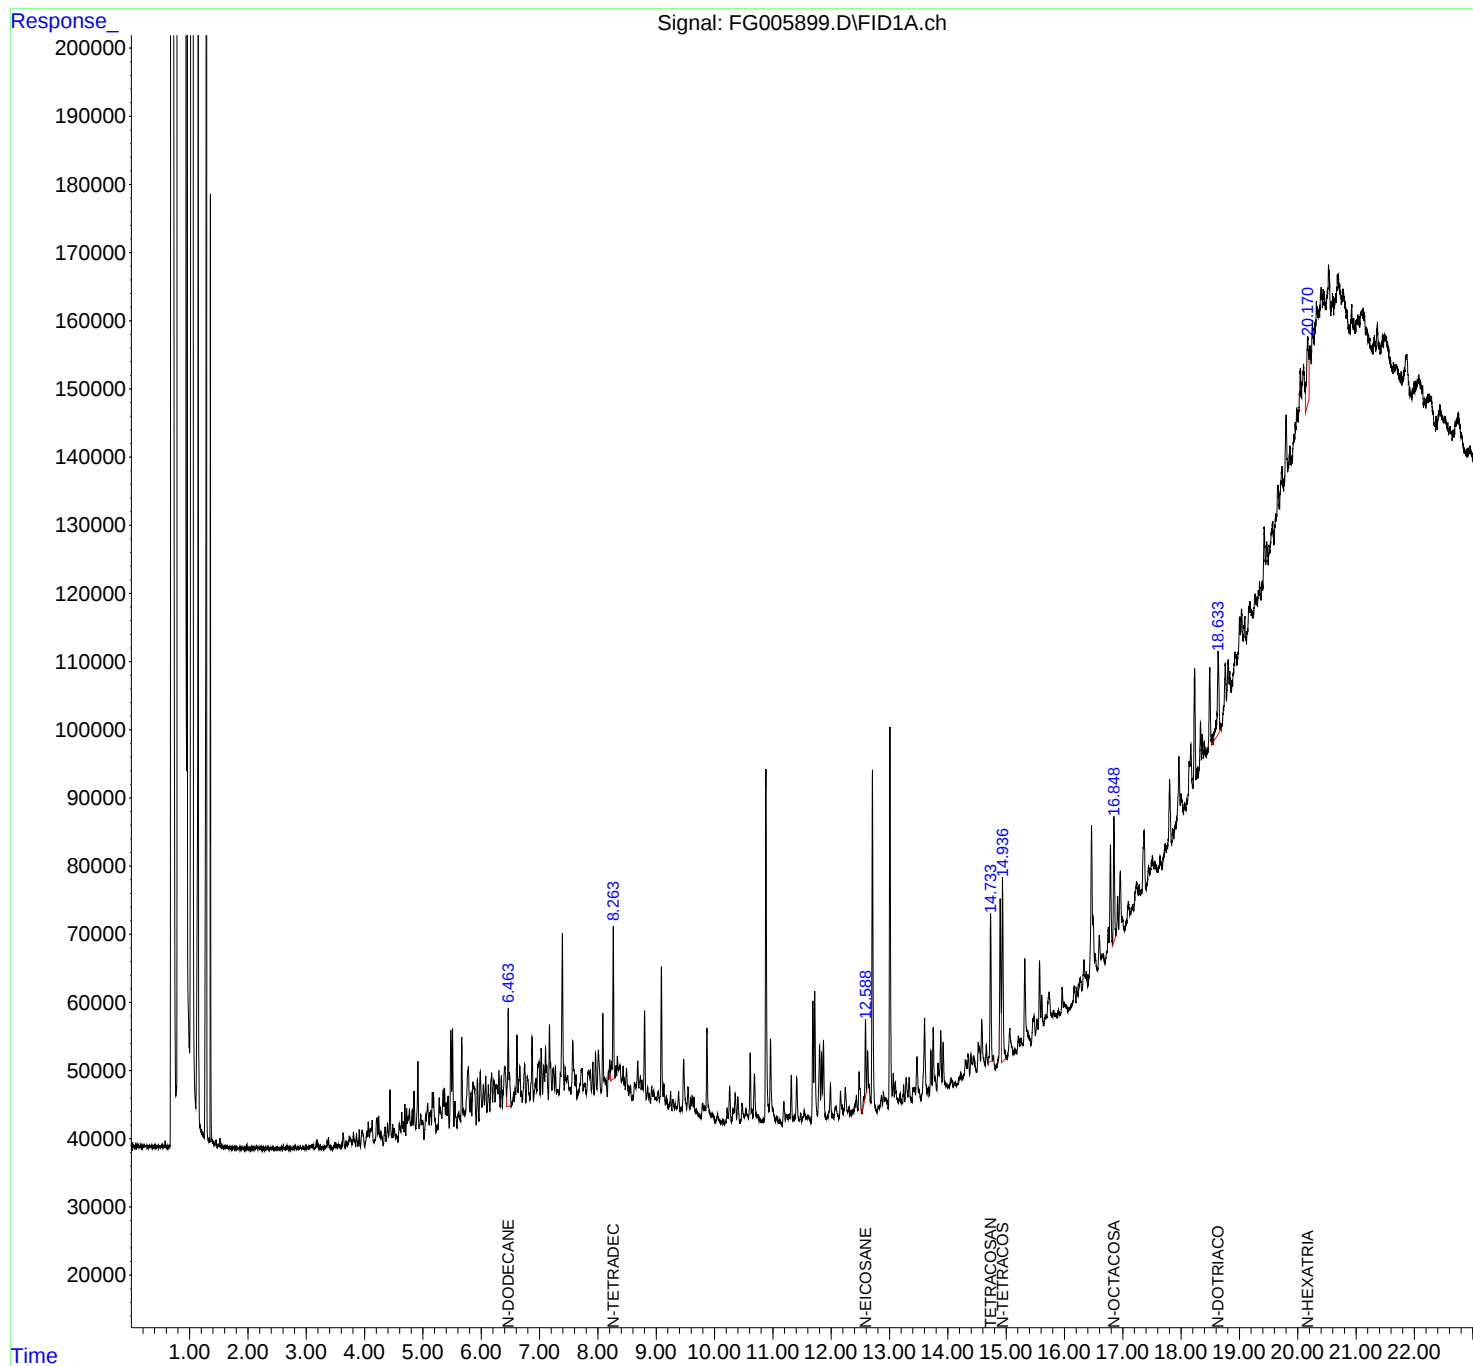


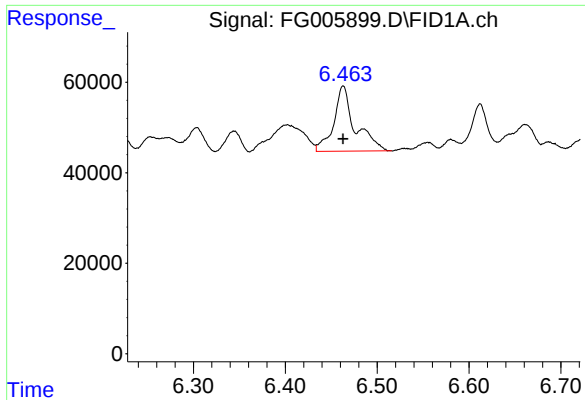

#3 N-DODECANE


R.T.: 6.463 min
Delta R.T.: 0.000 min
Response: 230829
Conc: 1.63 ug/ml

Instrument :
FID_G
ClientSampleId :

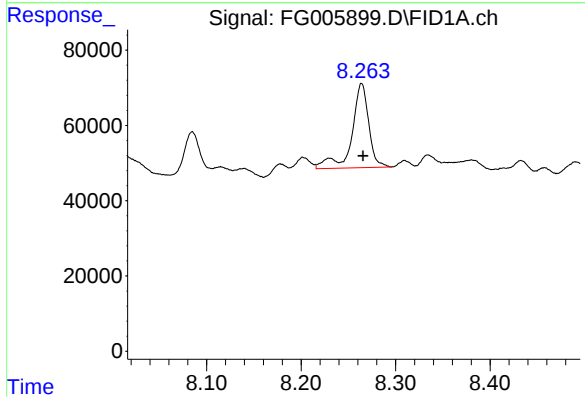


#4 N-TETRADECANE

R.T.: 8.264 min
Delta R.T.: -0.001 min
Response: 278621
Conc: 1.98 ug/ml

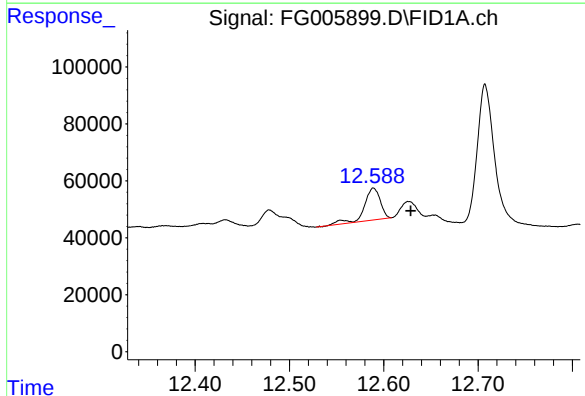


#7 N-EICOSANE

R.T.: 12.589 min
Delta R.T.: -0.040 min
Response: 132039
Conc: 0.97 ug/ml

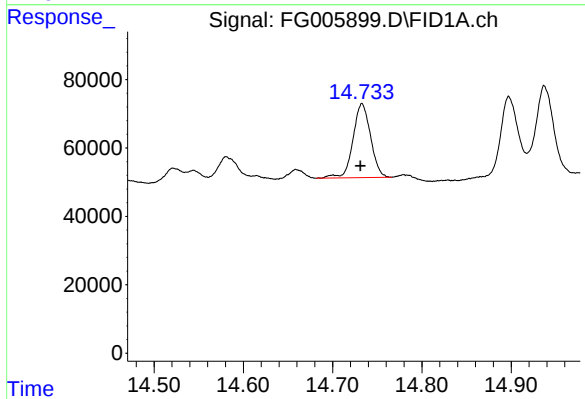

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.733 min
Delta R.T.: 0.002 min
Response: 295023
Conc: 2.63 ug/ml

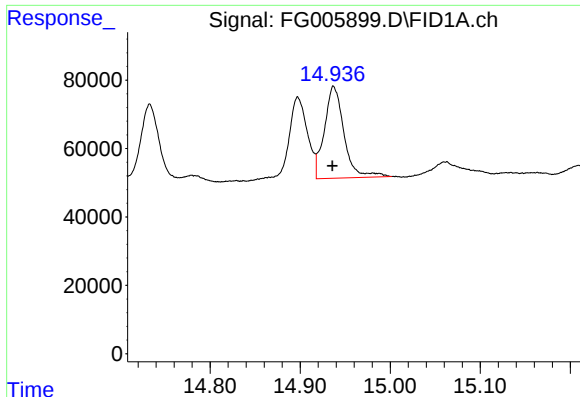

#10 N-TETRACOSANE


R.T.: 14.938 min
Delta R.T.: 0.002 min
Response: 406770
Conc: 3.19 ug/ml

Instrument :
FID_G
ClientSampleId :

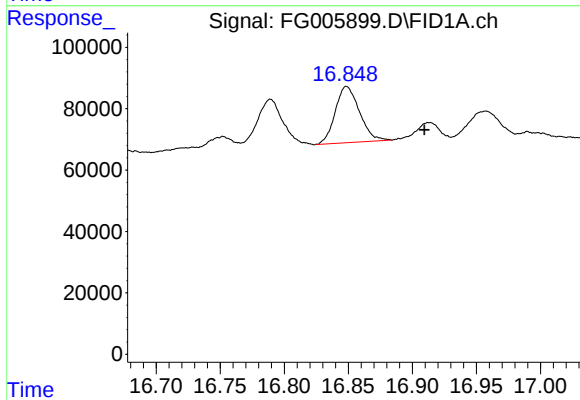


#12 N-OCTACOSANE

R.T.: 16.849 min
Delta R.T.: -0.000 min
Response: 239736
Conc: 2.03 ug/ml

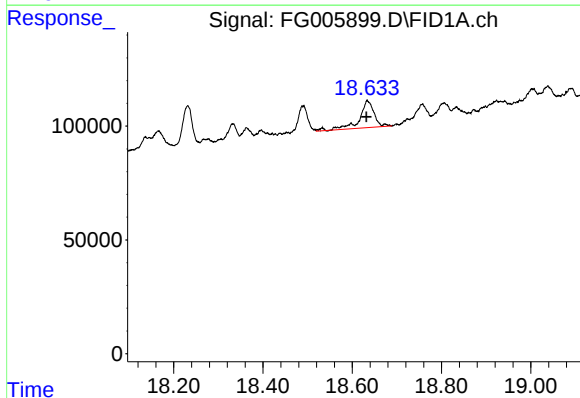

#14 N-DOTRIACONTANE

R.T.: 18.635 min
Delta R.T.: 0.003 min
Response: 271062
Conc: 2.53 ug/ml

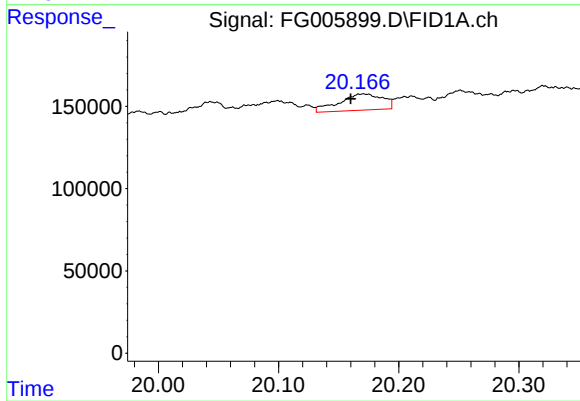

#16 N-HEXATRIACONTANE

R.T.: 20.171 min
Delta R.T.: 0.011 min
Response: 247188
Conc: 2.48 ug/ml