

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG090922\
Data File : FG010546.D
Signal(s) : FID1A.ch
Acq On : 09 Sep 2022 13:30
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 12 00:28:34 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG082622.M
Quant Title :
QLast Update : Fri Aug 26 23:48:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.486	2408530	18.301 ug/ml
12)	N-OCTACOSANE	16.958	2375180	17.961 ug/ml
13)	N-TRIACONTANE	17.845	354487	2.736 ug/ml
14)	N-DOTRIACONTANE	18.677	500579	3.915 ug/ml
15)	N-TETRATRIACONTANE	19.462	446499	3.609 ug/ml
16)	N-HEXATRIACONTANE	20.204	301513	2.598 ug/ml
17)	N-OCTATRIACONTANE	20.916	193495	1.685 ug/ml
18)	N-TETRACONTANE	21.751	122547	1.039 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG090922\
Data File : FG010546.D
Signal(s) : FID1A.ch
Acq On : 09 Sep 2022 13:30
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 12 00:28:34 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG082622.M
Quant Title :
QLast Update : Fri Aug 26 23:48:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

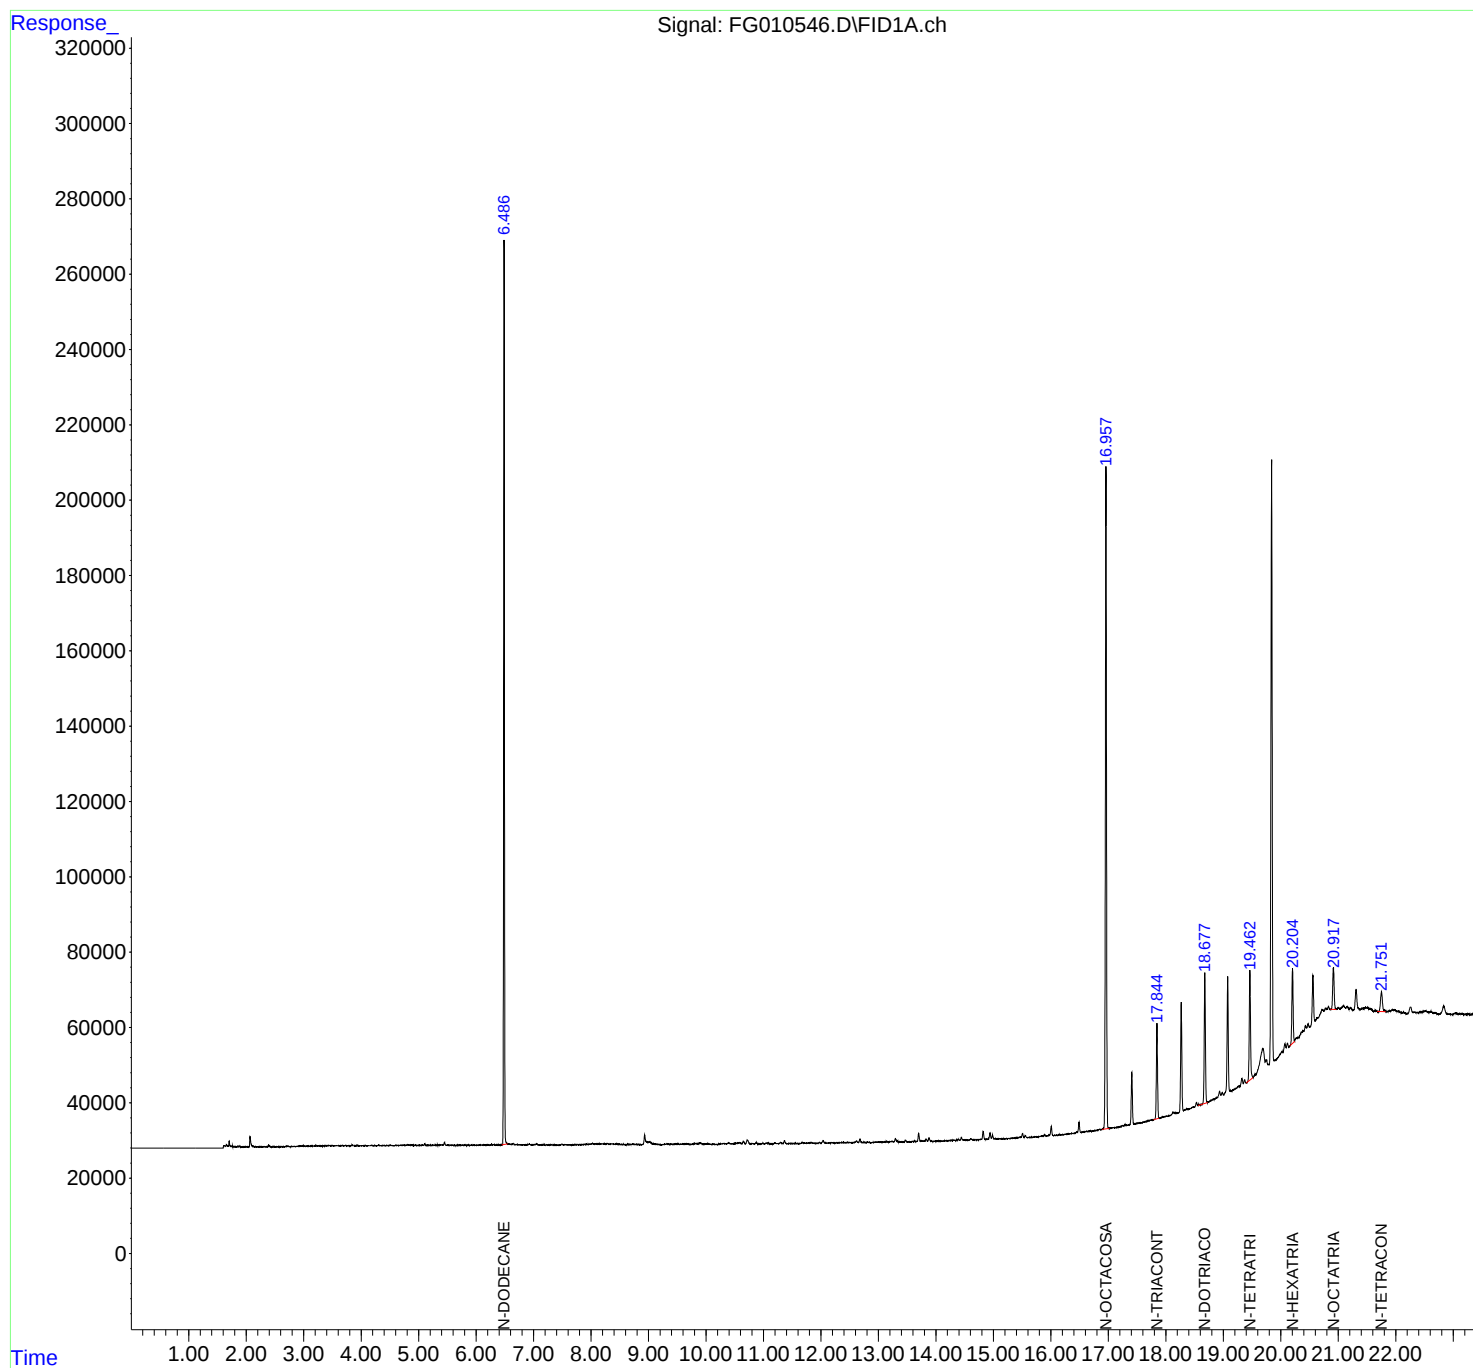


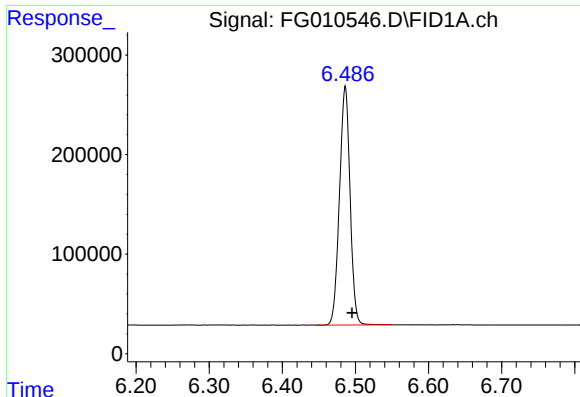

#3 N-DODECANE


R.T.: 6.486 min
Delta R.T.: -0.009 min
Response: 2408530
Conc: 18.30 ug/ml

Instrument :
FID_G
ClientSampleId :

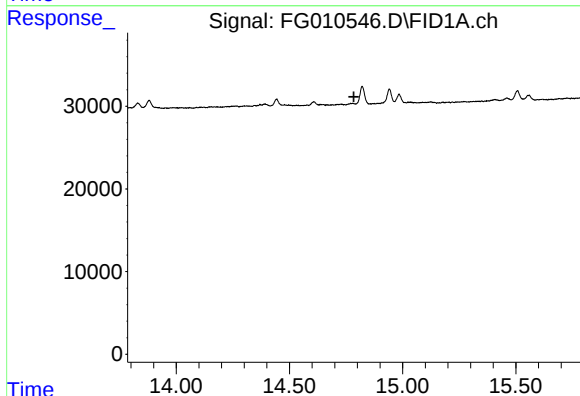


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.785 min
Response: 0
Conc: N.D.

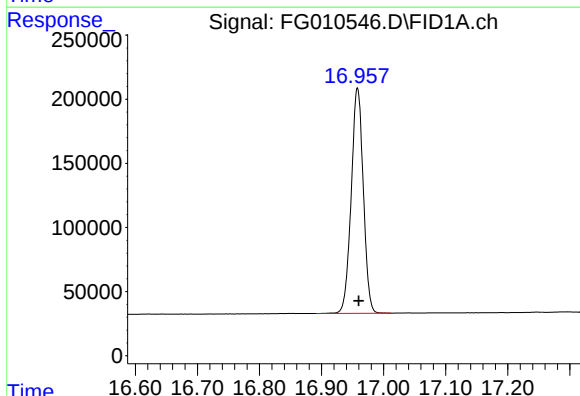


#12 N-OCTACOSANE

R.T.: 16.958 min
Delta R.T.: -0.002 min
Response: 2375180
Conc: 17.96 ug/ml

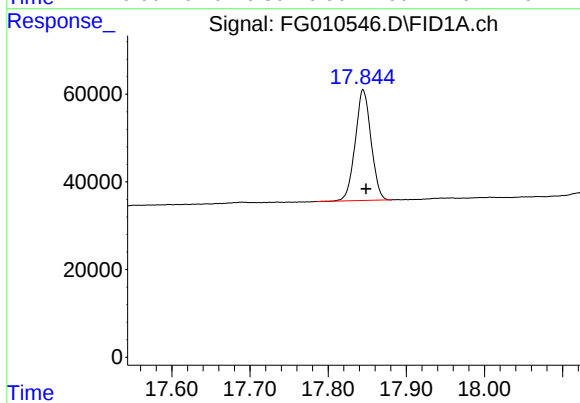

#13 N-TRIACONTANE


R.T.: 17.845 min
Delta R.T.: -0.004 min
Response: 354487
Conc: 2.74 ug/ml

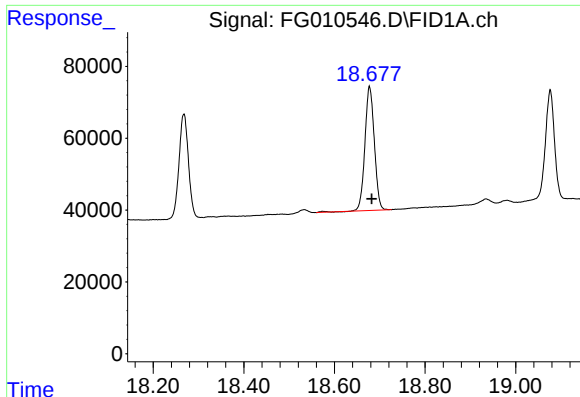

#14 N-DOTRIACONTANE


R.T.: 18.677 min
Delta R.T.: -0.005 min
Response: 500579
Conc: 3.92 ug/ml

Instrument :
FID_G
ClientSampleId :

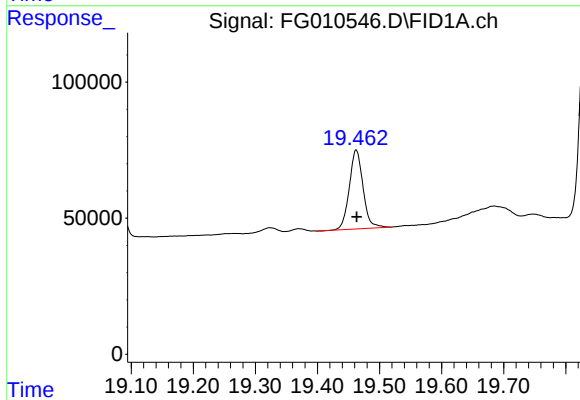


#15 N-TETRATRIACONTANE

R.T.: 19.462 min
Delta R.T.: 0.000 min
Response: 446499
Conc: 3.61 ug/ml

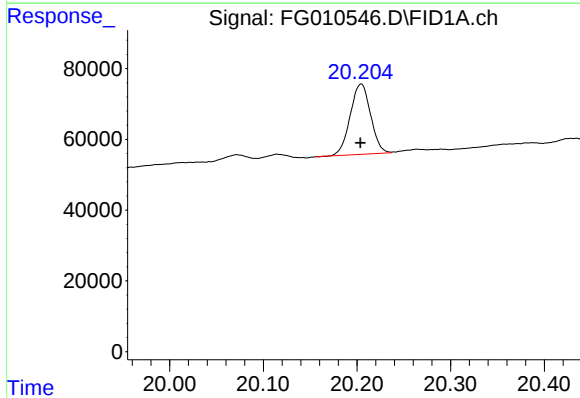


#16 N-HEXATRIACONTANE

R.T.: 20.204 min
Delta R.T.: 0.000 min
Response: 301513
Conc: 2.60 ug/ml

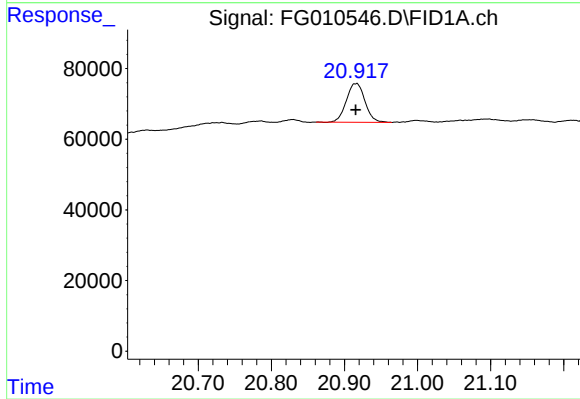

#17 N-OCTATRIACONTANE

R.T.: 20.916 min
Delta R.T.: 0.000 min
Response: 193495
Conc: 1.68 ug/ml

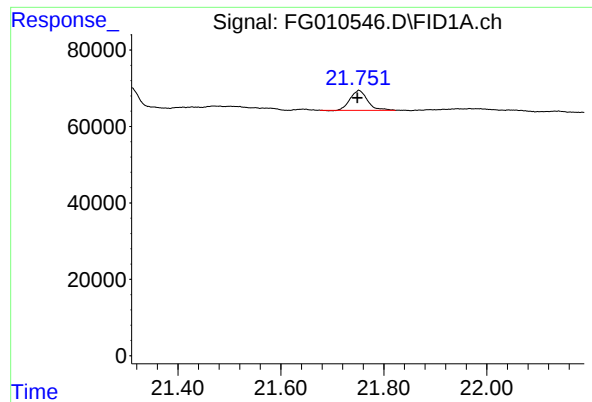

#18 N-TETRACONTANE

R.T.: 21.751 min
Delta R.T.: 0.003 min
Response: 122547
Conc: 1.04 ug/ml

Instrument :

FID_G

ClientSampleId :