

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG090924\
 Data File : FG014179.D
 Signal(s) : FID1A.ch
 Acq On : 09 Sep 2024 14:45
 Operator : YP\AJ
 Sample : P3880-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Sep 10 02:46:03 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG081624.M
 Quant Title :
 QLast Update : Fri Aug 16 10:59:42 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.933	1297882	12.282 ug/ml
Target Compounds			
7) N-EICOSANE	12.879	489234	4.111 ug/ml
10) N-TETRACOSANE	15.107	426382	3.608 ug/ml
11) N-HEXACOSANE	16.162	99800	0.843 ug/ml
12) N-OCTACOSANE	17.113	140227	1.189 ug/ml
13) N-TRIACONTANE	18.005	99053	0.827 ug/ml
14) N-DOTRIACONTANE	18.832	110532	0.925 ug/ml
15) N-TETRATRIACONTANE	19.634	60691	0.521 ug/ml
16) N-HEXATRIACONTANE	20.325	66347	0.575 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG090924\
Data File : FG014179.D
Signal(s) : FID1A.ch
Acq On : 09 Sep 2024 14:45
Operator : YP\AJ
Sample : P3880-01
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 10 02:46:03 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG081624.M
Quant Title :
QLast Update : Fri Aug 16 10:59:42 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

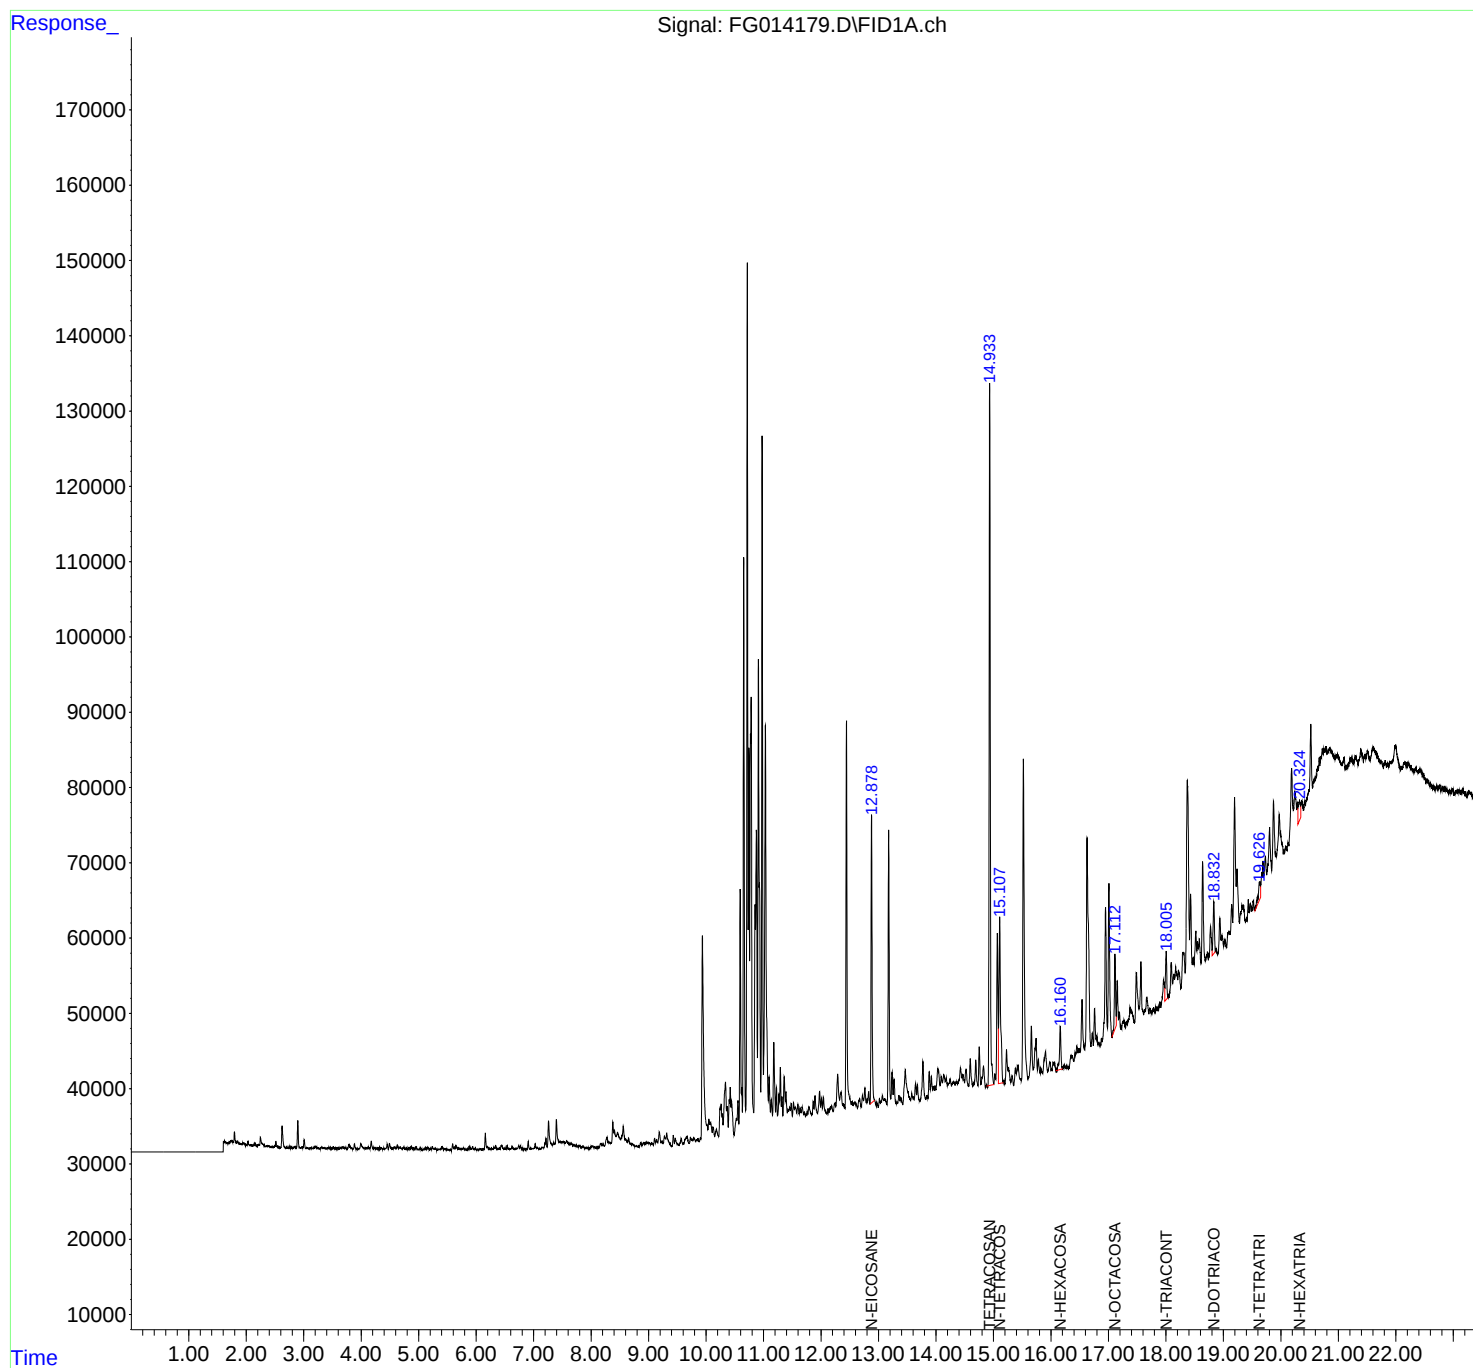


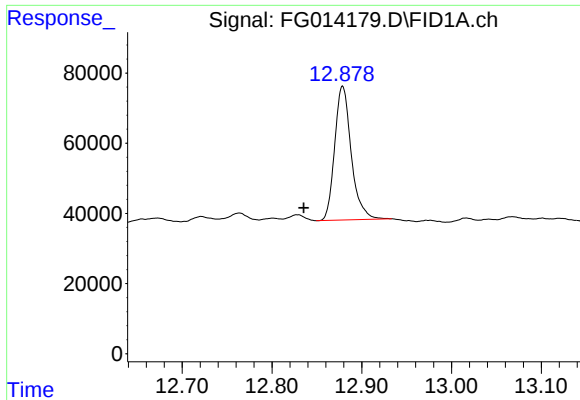

#7 N-EICOSANE


R.T.: 12.879 min
Delta R.T.: 0.043 min
Response: 489234
Conc: 4.11 ug/ml

Instrument :
FID_G
ClientSampleId :

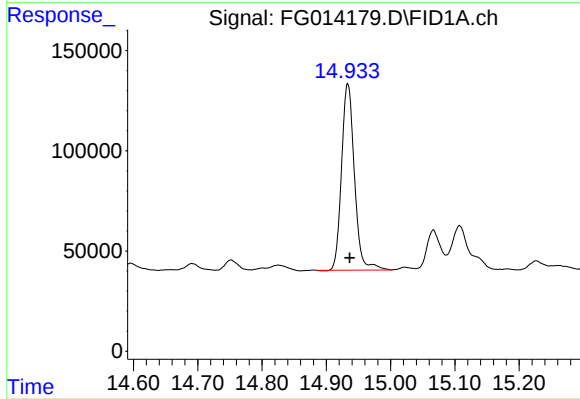


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.933 min
Delta R.T.: -0.003 min
Response: 1297882
Conc: 12.28 ug/ml

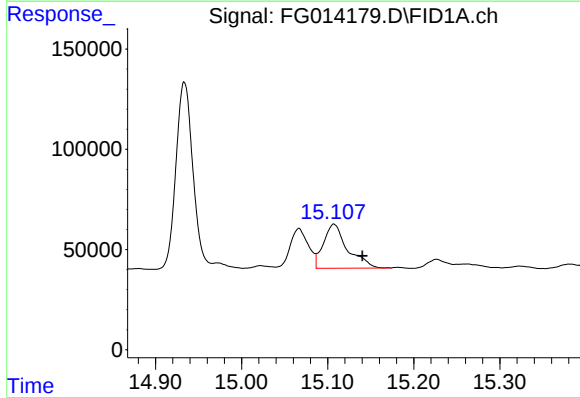


#10 N-TETRACOSANE

R.T.: 15.107 min
Delta R.T.: -0.033 min
Response: 426382
Conc: 3.61 ug/ml

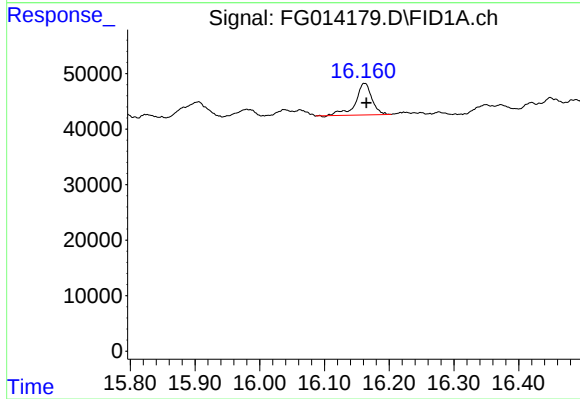

#11 N-HEXACOSANE


R.T.: 16.162 min
Delta R.T.: -0.003 min
Response: 99800
Conc: 0.84 ug/ml

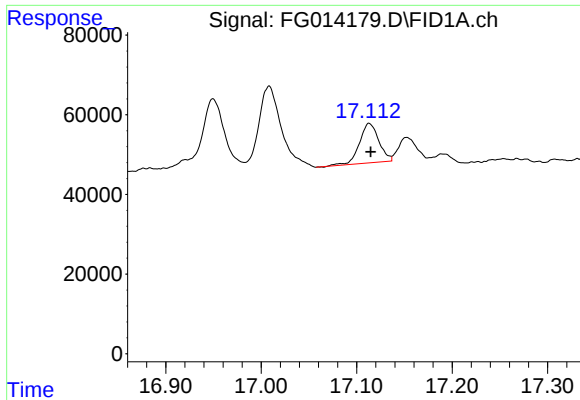

#12 N-OCTACOSANE


R.T.: 17.113 min
Delta R.T.: -0.002 min
Response: 140227
Conc: 1.19 ug/ml

Instrument :
FID_G
ClientSampleId :

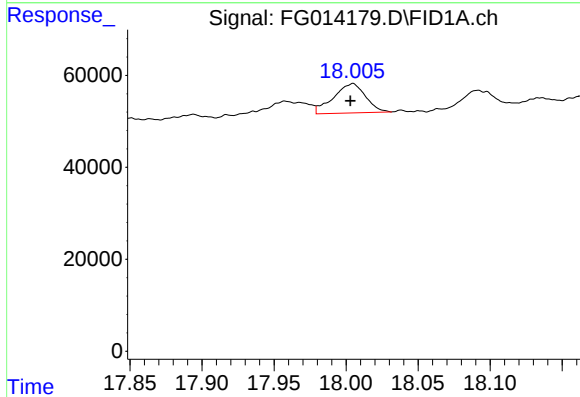


#13 N-TRIACONTANE

R.T.: 18.005 min
Delta R.T.: 0.002 min
Response: 99053
Conc: 0.83 ug/ml

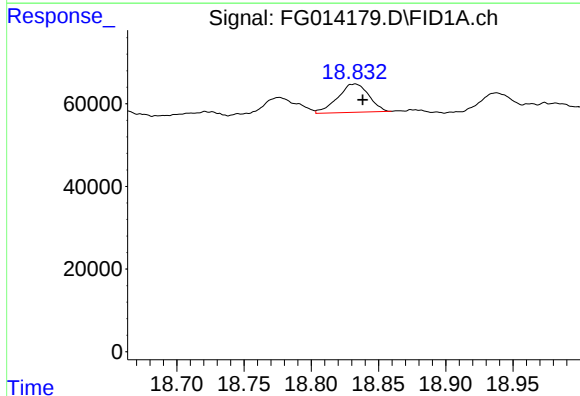


#14 N-DOTRIACONTANE

R.T.: 18.832 min
Delta R.T.: -0.006 min
Response: 110532
Conc: 0.92 ug/ml

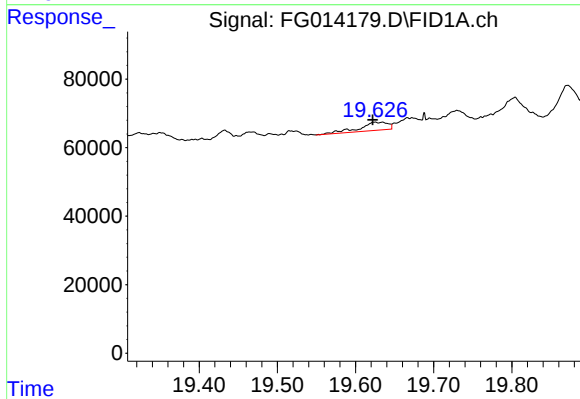

#15 N-TETRATRIACONTANE

R.T.: 19.634 min
Delta R.T.: 0.012 min
Response: 60691
Conc: 0.52 ug/ml

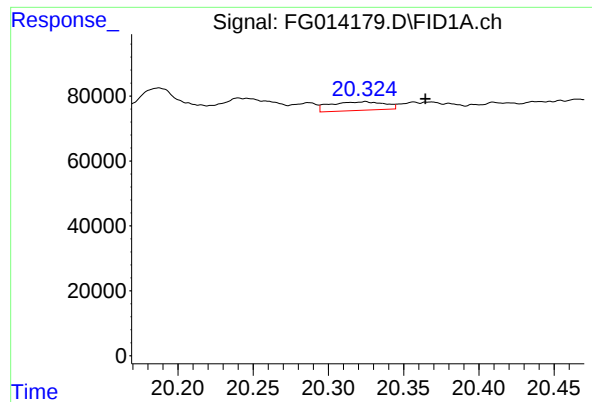

#16 N-HEXATRIACONTANE

R.T.: 20.325 min
Delta R.T.: -0.040 min
Response: 66347
Conc: 0.57 ug/ml

Instrument :

FID_G

ClientSampleId :