

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG091018\
Data File : FG002268.D
Signal(s) : FID1A.ch
Acq On : 10 Sep 2018 14:09
Operator : AJ\SJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 11 04:15:36 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG083018.M
Quant Title :
QLast Update : Thu Aug 30 14:49:31 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.197	4175577	33.180 ug/ml
12)	N-OCTACOSANE	16.597	4026059	27.517 ug/ml
13)	N-TRIACONTANE	17.481	138991	0.916 ug/ml
14)	N-DOTRIACONTANE	18.313	182024	1.234 ug/ml
15)	N-TETRATRIACONTANE	19.098	124771	0.904 ug/ml
18)	N-TETRACONTANE	21.366	70385	0.649 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG091018\
Data File : FG002268.D
Signal(s) : FID1A.ch
Acq On : 10 Sep 2018 14:09
Operator : AJ\SJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 11 04:15:36 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG083018.M
Quant Title :
QLast Update : Thu Aug 30 14:49:31 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

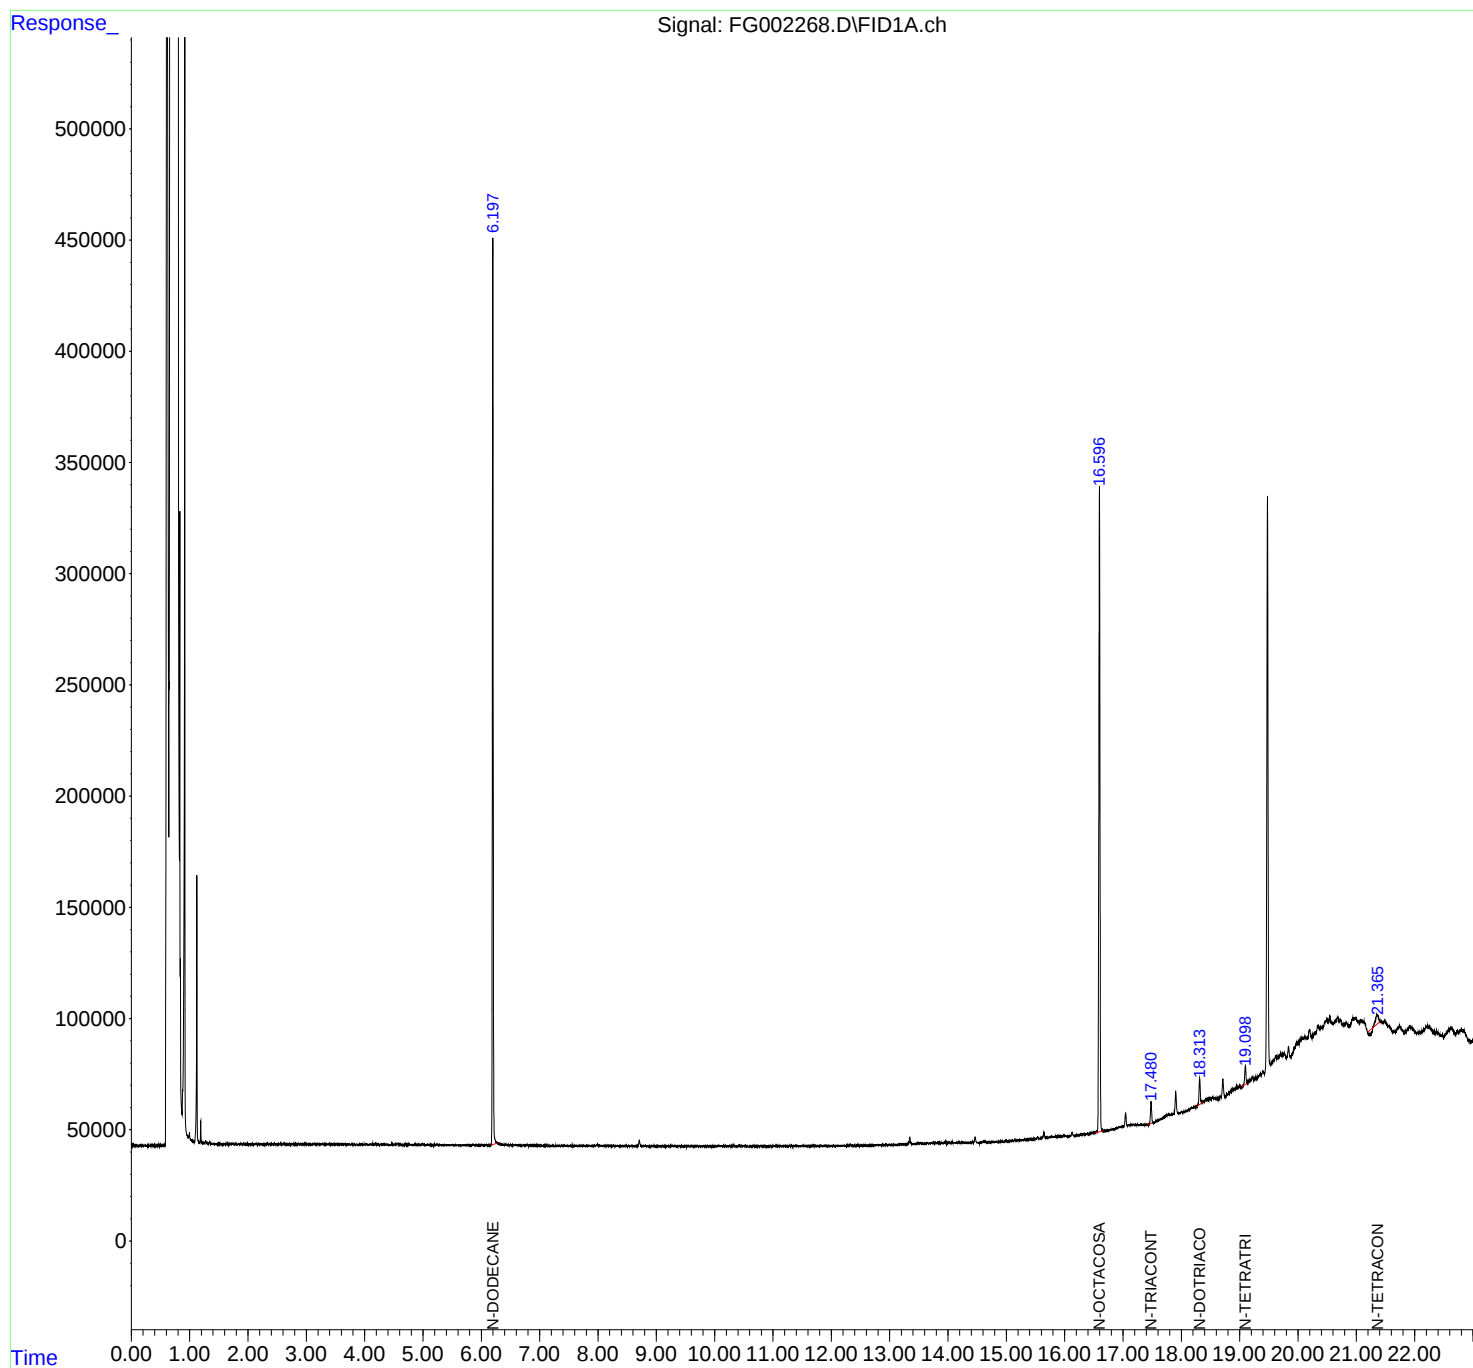


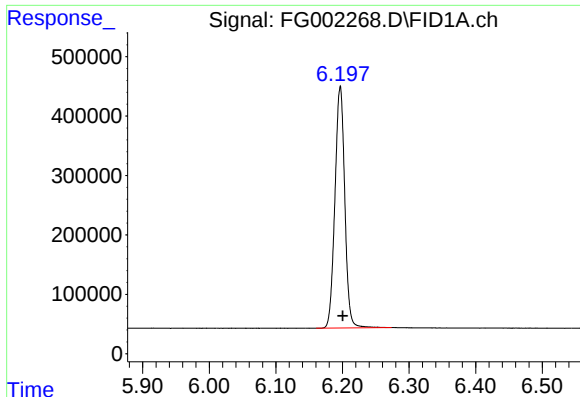

#3 N-DODECANE


R.T.: 6.197 min
Delta R.T.: -0.004 min
Response: 4175577
Conc: 33.18 ug/ml

Instrument :
FID_G
ClientSampleId :

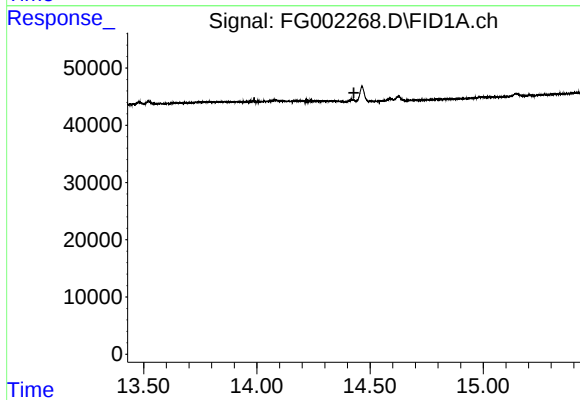


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.429 min
Response: 0
Conc: N.D.

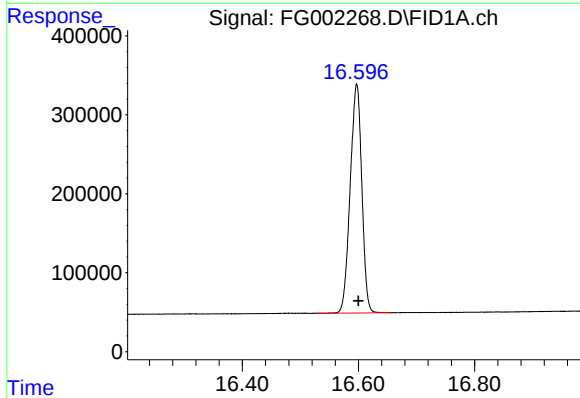


#12 N-OCTACOSANE

R.T.: 16.597 min
Delta R.T.: -0.003 min
Response: 4026059
Conc: 27.52 ug/ml

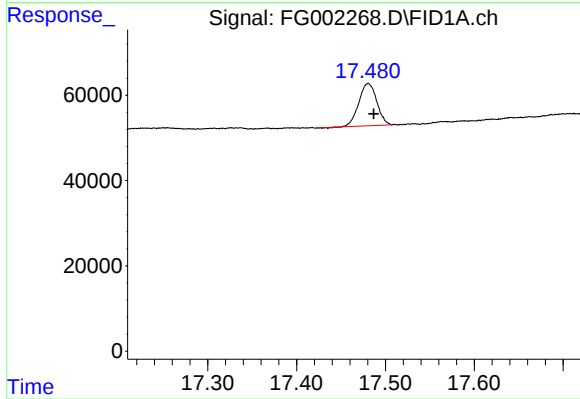

#13 N-TRIACONTANE


R.T.: 17.481 min
Delta R.T.: -0.006 min
Response: 138991
Conc: 0.92 ug/ml

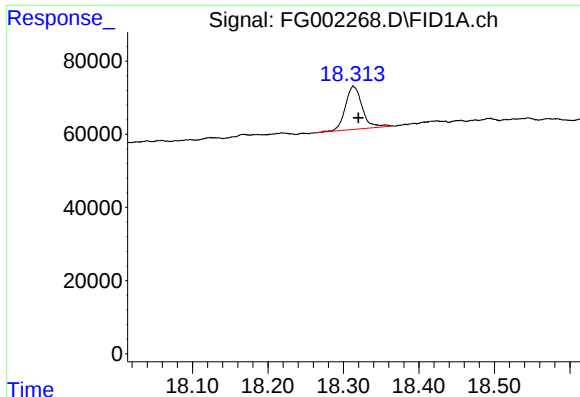

#14 N-DOTRIACONTANE


R.T.: 18.313 min
Delta R.T.: -0.007 min
Response: 182024
Conc: 1.23 ug/ml

Instrument :
FID_G
ClientSampleId :

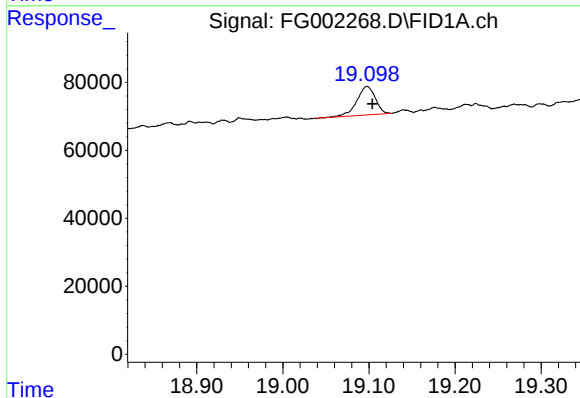

#15 N-TETRATRIACONTANE

R.T.: 19.098 min
Delta R.T.: -0.006 min
Response: 124771
Conc: 0.90 ug/ml

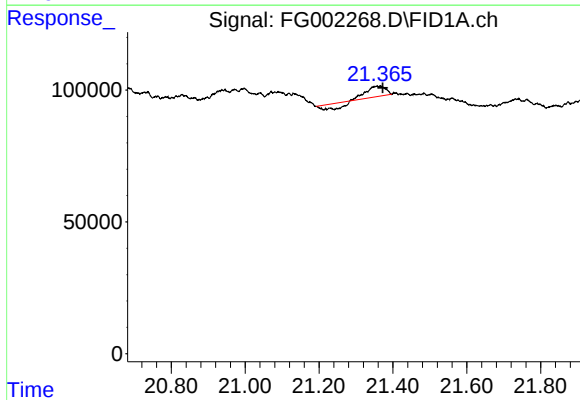

#18 N-TETRACONTANE

R.T.: 21.366 min
Delta R.T.: -0.006 min
Response: 70385
Conc: 0.65 ug/ml