

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG091018\
 Data File : FG002271.D
 Signal(s) : FID1A.ch
 Acq On : 10 Sep 2018 15:39
 Operator : AJ\SJ
 Sample : J4774-01 10X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Sep 11 04:15:55 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG083018.M
 Quant Title :
 QLast Update : Thu Aug 30 14:49:31 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.421	200377	1.588 ug/ml
Target Compounds			
7) N-EICOSANE	12.377	1268320	8.928 ug/ml
8) N-DOCOSANE	13.544	176328	1.235 ug/ml
10) N-TETRACOSANE	14.601	884631	6.188 ug/ml
11) N-HEXACOSANE	15.646	178509	1.243 ug/ml
12) N-OCTACOSANE	16.601	309218	2.113 ug/ml
13) N-TRIACONTANE	17.482	328250	2.164 ug/ml
14) N-DOTRIACONTANE	18.313	472775	3.206 ug/ml
15) N-TETRATRIACONTANE	19.101	211572	1.534 ug/ml
16) N-HEXATRIACONTANE	19.845	259899	2.027 ug/ml
17) N-OCTATRIACONTANE	20.553	158091	1.406 ug/ml
18) N-TETRACONTANE	21.366	149261	1.375 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG091018\
Data File : FG002271.D
Signal(s) : FID1A.ch
Acq On : 10 Sep 2018 15:39
Operator : AJ\SJ
Sample : J4774-01 10X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 11 04:15:55 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG083018.M
Quant Title :
QLast Update : Thu Aug 30 14:49:31 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

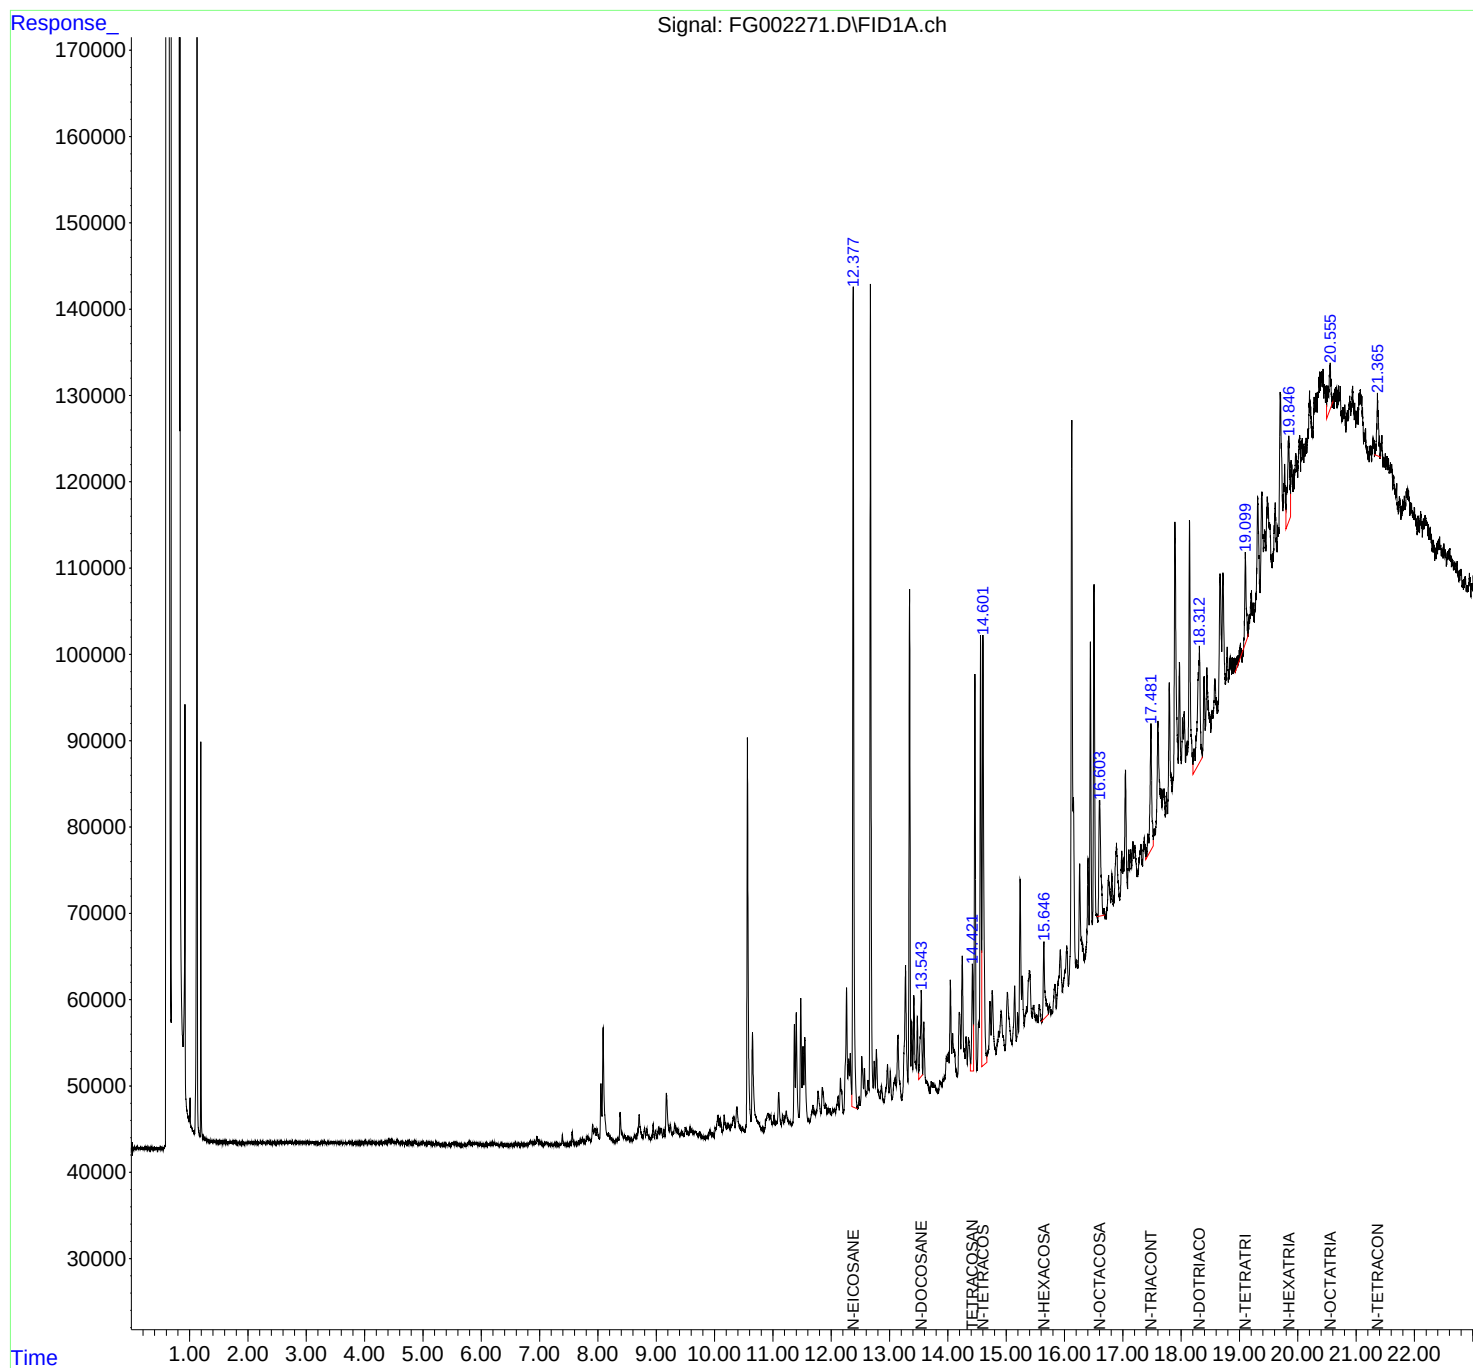


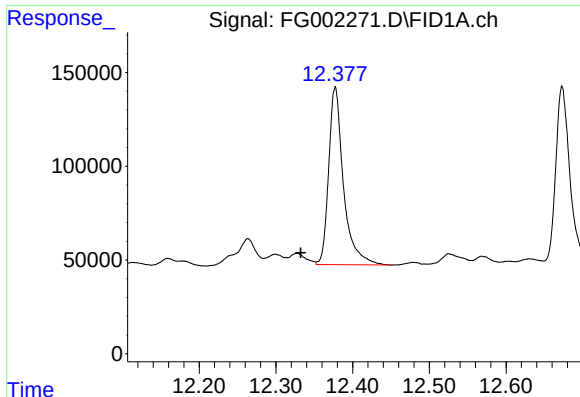

#7 N-EICOSANE


R.T.: 12.377 min
Delta R.T.: 0.045 min
Response: 1268320
Conc: 8.93 ug/ml

Instrument :
FID_G
ClientSampleId :

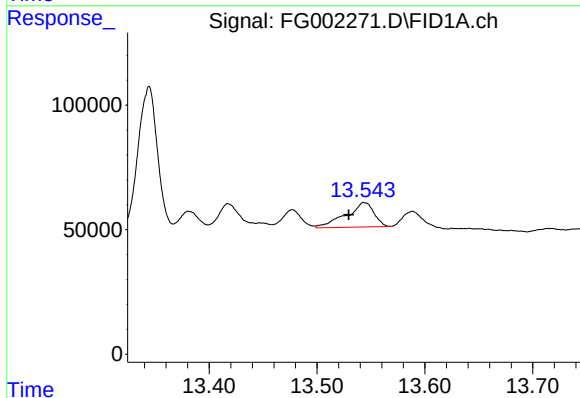


#8 N-DOCOSANE

R.T.: 13.544 min
Delta R.T.: 0.015 min
Response: 176328
Conc: 1.24 ug/ml

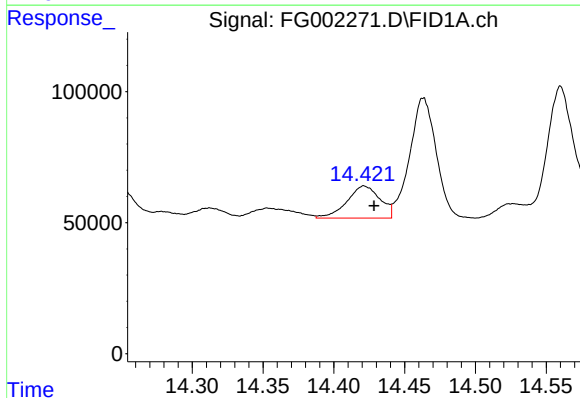


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.421 min
Delta R.T.: -0.007 min
Response: 200377
Conc: 1.59 ug/ml

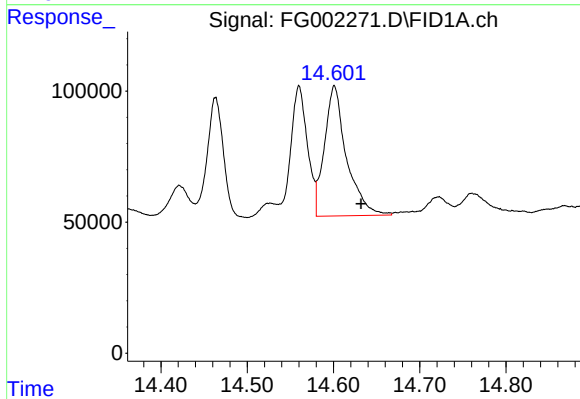

#10 N-TETRACOSANE


R.T.: 14.601 min
Delta R.T.: -0.031 min
Response: 884631
Conc: 6.19 ug/ml

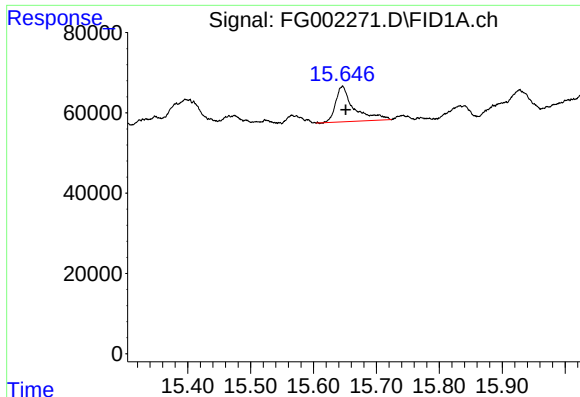

#11 N-HEXACOSANE


R.T.: 15.646 min
Delta R.T.: -0.005 min
Response: 178509
Conc: 1.24 ug/ml

Instrument :
FID_G
ClientSampleId :

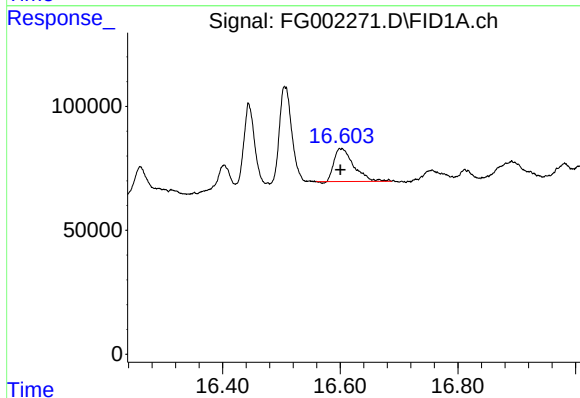


#12 N-OCTACOSANE

R.T.: 16.601 min
Delta R.T.: 0.001 min
Response: 309218
Conc: 2.11 ug/ml

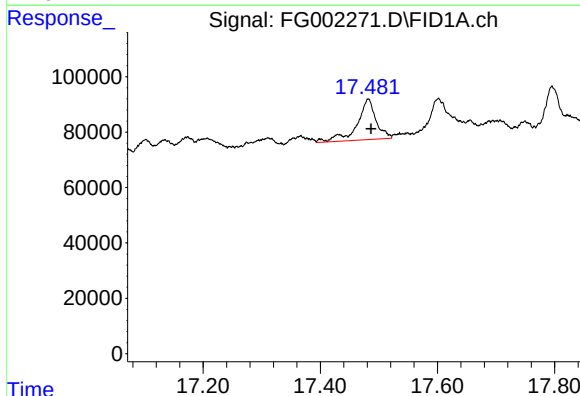


#13 N-TRIACONTANE

R.T.: 17.482 min
Delta R.T.: -0.005 min
Response: 328250
Conc: 2.16 ug/ml

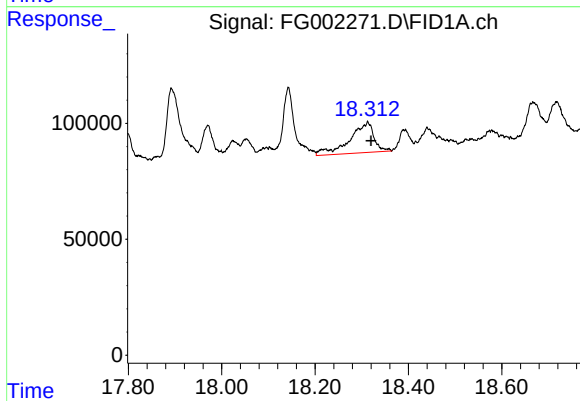

#14 N-DOTRIACONTANE


R.T.: 18.313 min
Delta R.T.: -0.007 min
Response: 472775
Conc: 3.21 ug/ml

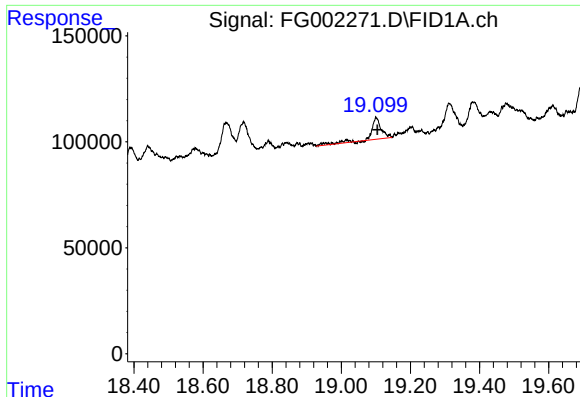

#15 N-TETRATRIACONTANE


R.T.: 19.101 min
Delta R.T.: -0.003 min
Response: 211572
Conc: 1.53 ug/ml

Instrument :
FID_G
ClientSampleId :

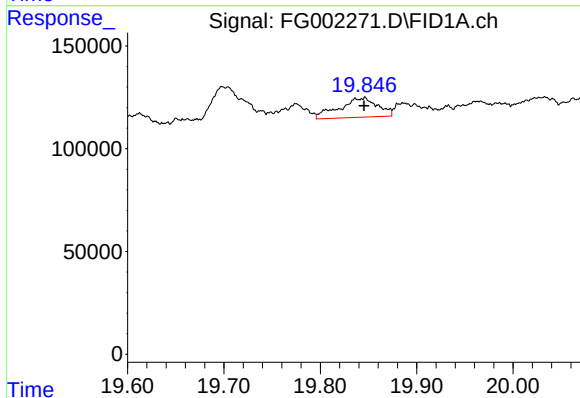


#16 N-HEXATRIACONTANE

R.T.: 19.845 min
Delta R.T.: 0.000 min
Response: 259899
Conc: 2.03 ug/ml

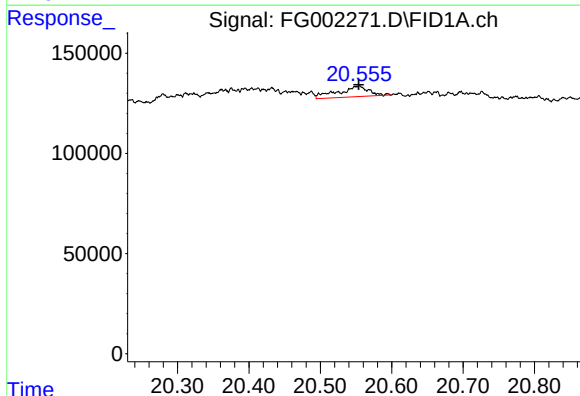

#17 N-OCTATRIACONTANE

R.T.: 20.553 min
Delta R.T.: 0.000 min
Response: 158091
Conc: 1.41 ug/ml

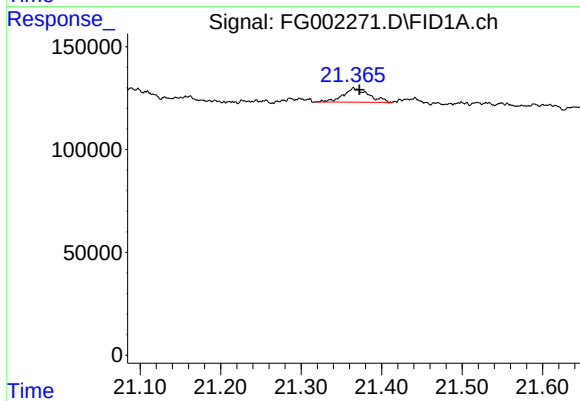

#18 N-TETRACONTANE

R.T.: 21.366 min
Delta R.T.: -0.006 min
Response: 149261
Conc: 1.38 ug/ml