

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG091018\
 Data File : FG002272.D
 Signal(s) : FID1A.ch
 Acq On : 10 Sep 2018 16:09
 Operator : AJ\SJ
 Sample : J4775-01 10X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Sep 11 04:16:02 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG083018.M
 Quant Title :
 QLast Update : Thu Aug 30 14:49:31 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.421	103153	0.818 ug/ml
Target Compounds			
7) N-EICOSANE	12.383f	337983	2.379 ug/ml
10) N-TETRACOSANE	14.611	226251	1.583 ug/ml
12) N-OCTACOSANE	16.597	73720	0.504 ug/ml
13) N-TRIACONTANE	17.482	167450	1.104 ug/ml
14) N-DOTRIACONTANE	18.313	223198	1.513 ug/ml
15) N-TETRATRIACONTANE	19.096	138673	1.005 ug/ml
16) N-HEXATRIACONTANE	19.843	88290	0.688 ug/ml
18) N-TETRACONTANE	21.335	35355	0.326 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG091018\
Data File : FG002272.D
Signal(s) : FID1A.ch
Acq On : 10 Sep 2018 16:09
Operator : AJ\SJ
Sample : J4775-01 10X
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_G
ClientSampled :

Integration File: autoint1.e
Quant Time: Sep 11 04:16:02 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG083018.M
Quant Title :
QLast Update : Thu Aug 30 14:49:31 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

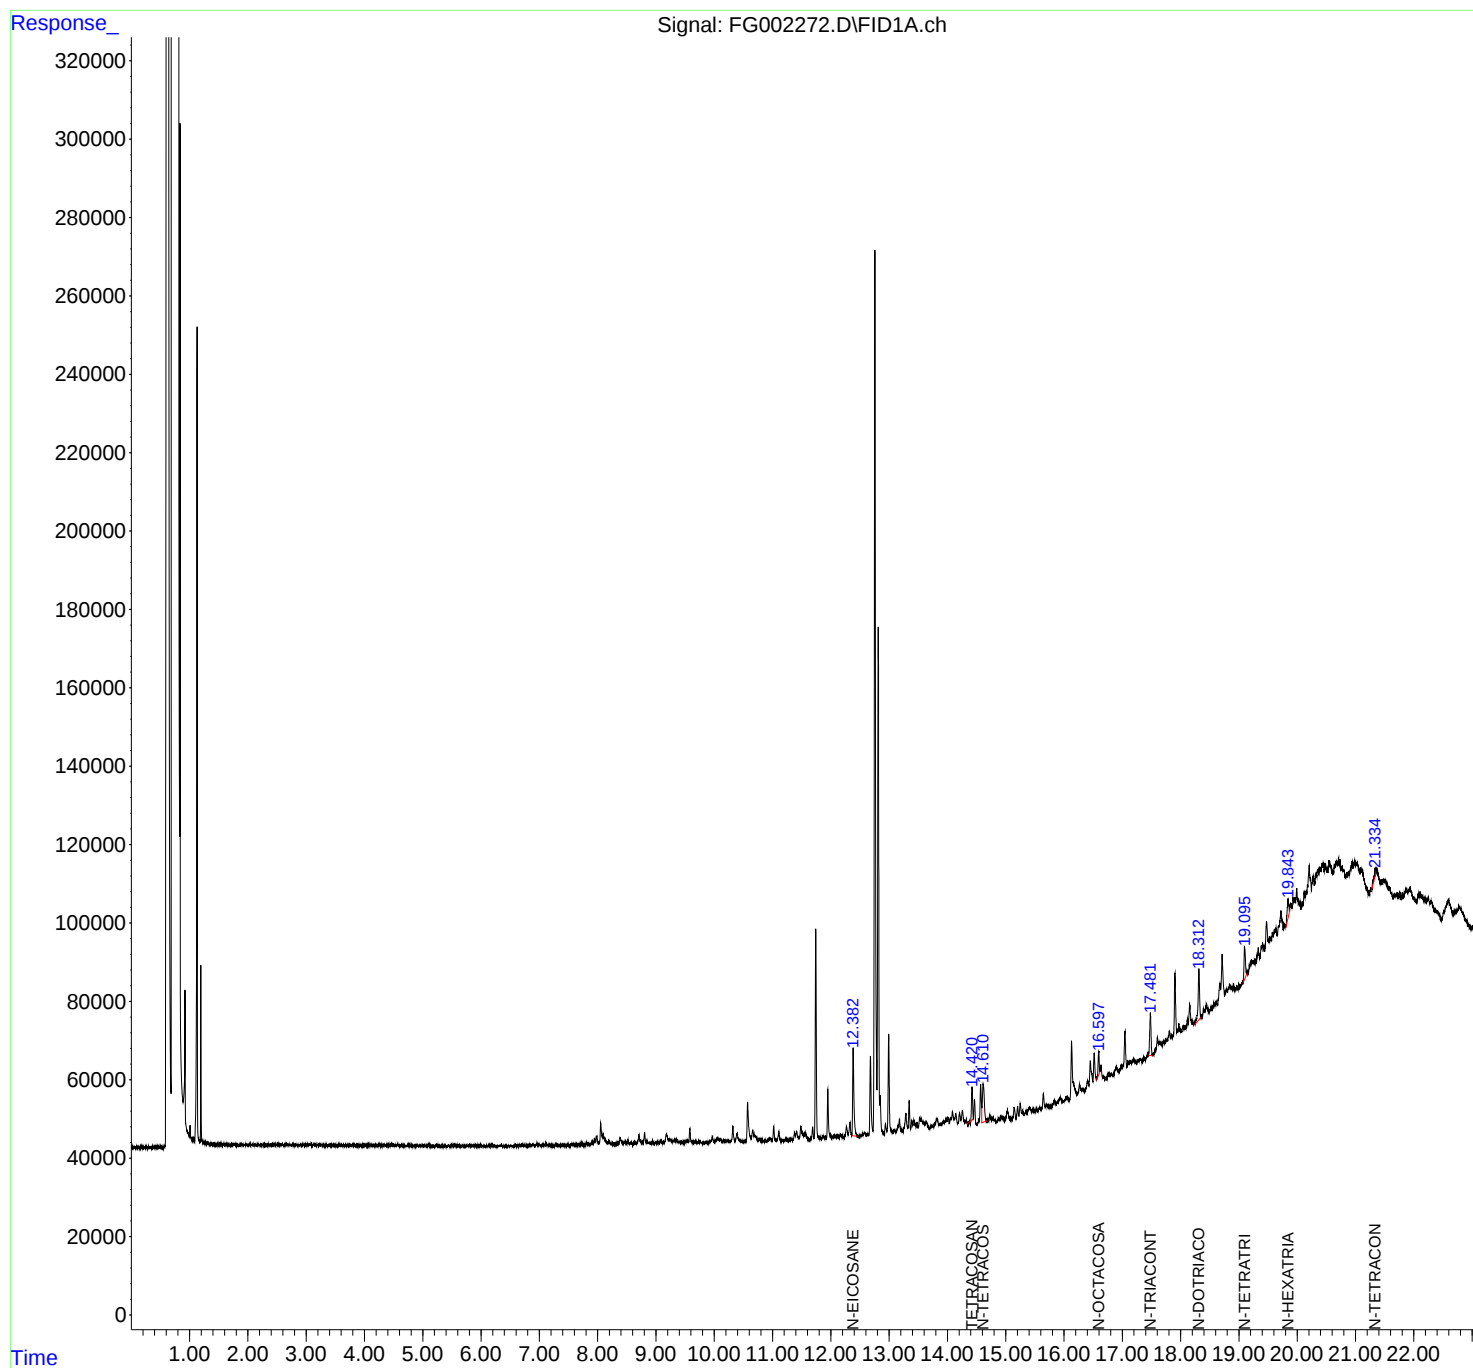


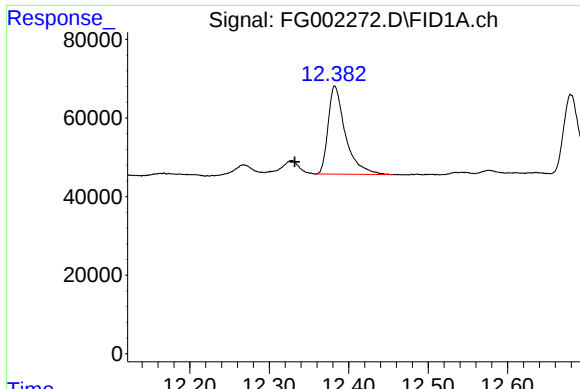

#7 N-EICOSANE


R.T.: 12.383 min
Delta R.T.: 0.050 min
Response: 337983
Conc: 2.38 ug/ml

Instrument :
FID_G
ClientSampleId :

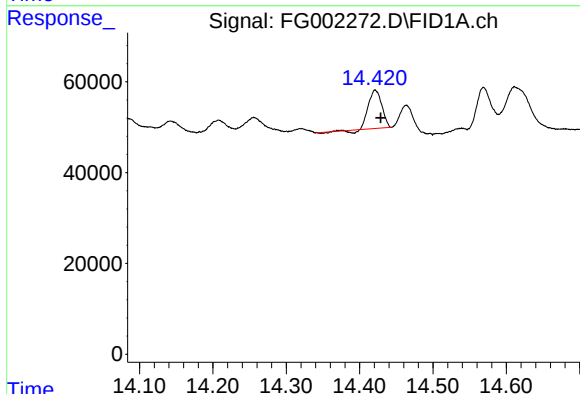


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.421 min
Delta R.T.: -0.007 min
Response: 103153
Conc: 0.82 ug/ml

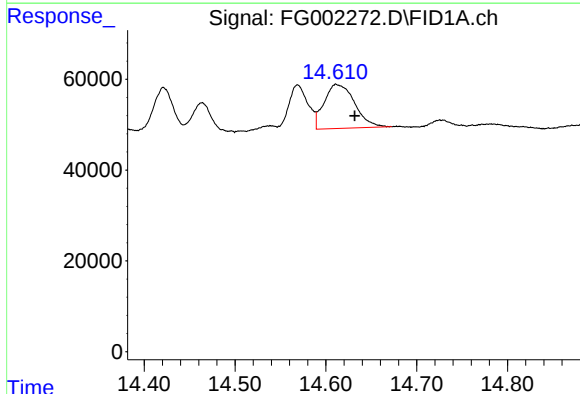


#10 N-TETRACOSANE

R.T.: 14.611 min
Delta R.T.: -0.021 min
Response: 226251
Conc: 1.58 ug/ml

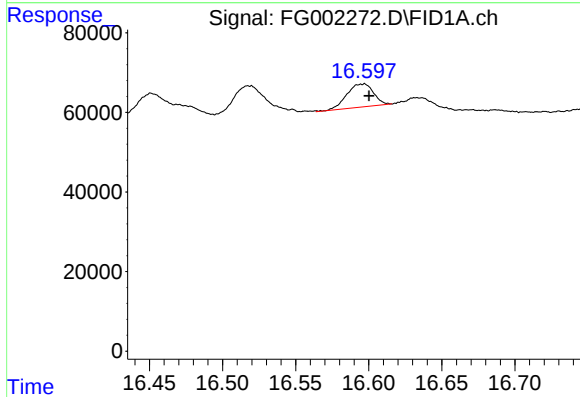

#12 N-OCTACOSANE


R.T.: 16.597 min
Delta R.T.: -0.003 min
Response: 73720
Conc: 0.50 ug/ml

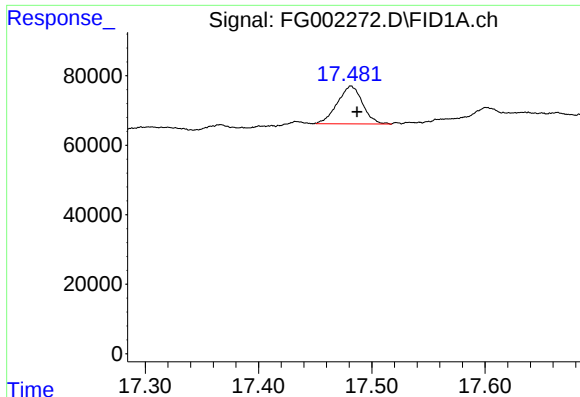

#13 N-TRIACONTANE


R.T.: 17.482 min
Delta R.T.: -0.005 min
Response: 167450
Conc: 1.10 ug/ml

Instrument :
FID_G
ClientSampleId :

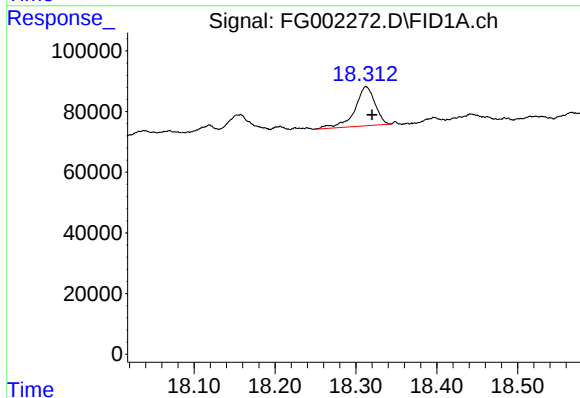


#14 N-DOTRIACONTANE

R.T.: 18.313 min
Delta R.T.: -0.007 min
Response: 223198
Conc: 1.51 ug/ml

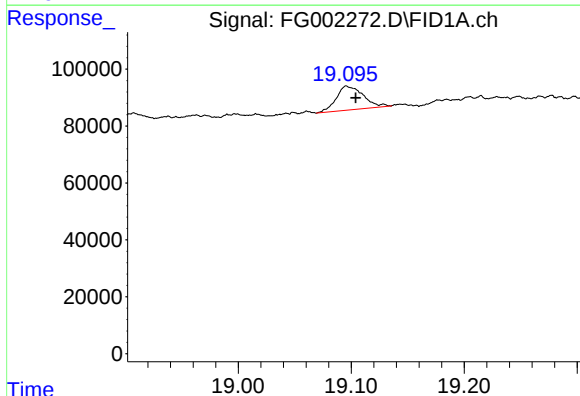


#15 N-TETRATRIACONTANE

R.T.: 19.096 min
Delta R.T.: -0.008 min
Response: 138673
Conc: 1.01 ug/ml

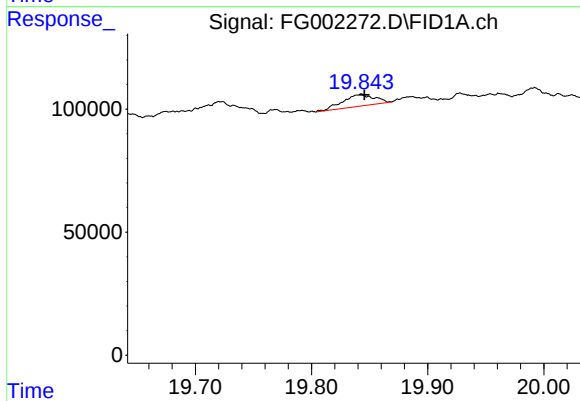

#16 N-HEXATRIACONTANE

R.T.: 19.843 min
Delta R.T.: -0.003 min
Response: 88290
Conc: 0.69 ug/ml

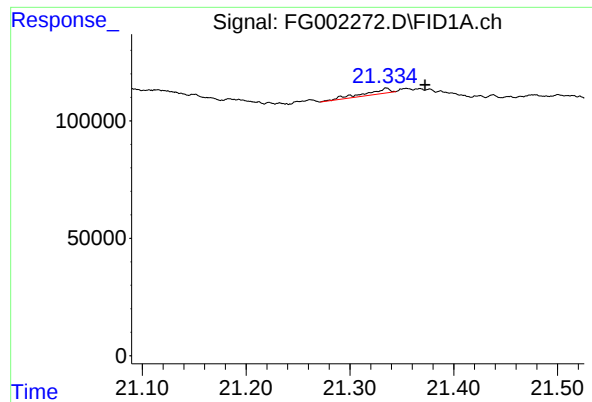

#18 N-TETRACONTANE

R.T.: 21.335 min
Delta R.T.: -0.037 min
Response: 35355
Conc: 0.33 ug/ml

Instrument :
FID_G
ClientSampleId :