

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG091018\
 Data File : FG002274.D
 Signal(s) : FID1A.ch
 Acq On : 10 Sep 2018 17:09
 Operator : AJ\SJ
 Sample : J4779-01 10X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Sep 11 04:16:15 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG083018.M
 Quant Title :
 QLast Update : Thu Aug 30 14:49:31 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.423	153276	1.215 ug/ml
Target Compounds			
7) N-EICOSANE	12.380	704167	4.957 ug/ml
8) N-DOCOSANE	13.478f	105544	0.740 ug/ml
10) N-TETRACOSANE	14.605	509085	3.561 ug/ml
11) N-HEXACOSANE	15.646	102370	0.713 ug/ml
12) N-OCTACOSANE	16.597	257100	1.757 ug/ml
13) N-TRIACONTANE	17.484	219925	1.450 ug/ml
14) N-DOTRIACONTANE	18.316	316705	2.147 ug/ml
15) N-TETRATRIACONTANE	19.103	199362	1.445 ug/ml
16) N-HEXATRIACONTANE	19.846	83158	0.648 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG091018\
Data File : FG002274.D
Signal(s) : FID1A.ch
Acq On : 10 Sep 2018 17:09
Operator : AJ\SJ
Sample : J4779-01 10X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 11 04:16:15 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG083018.M
Quant Title :
QLast Update : Thu Aug 30 14:49:31 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

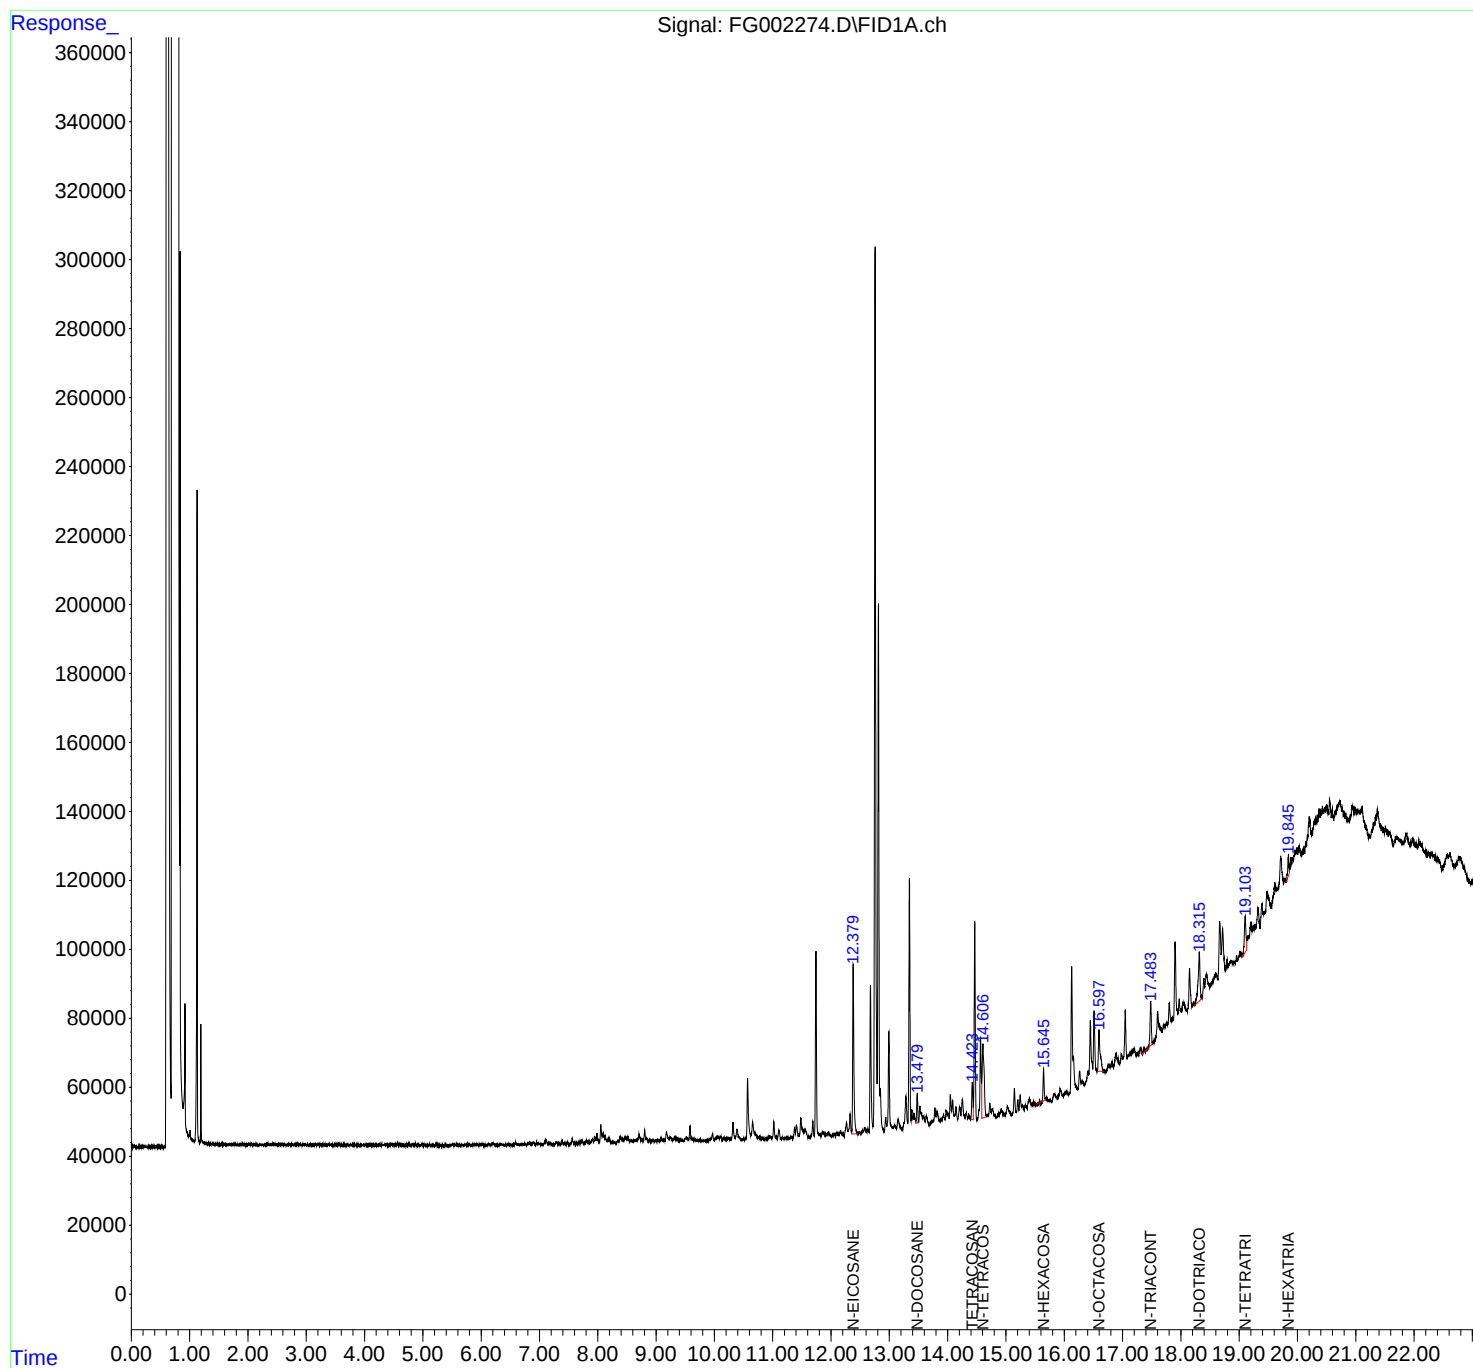


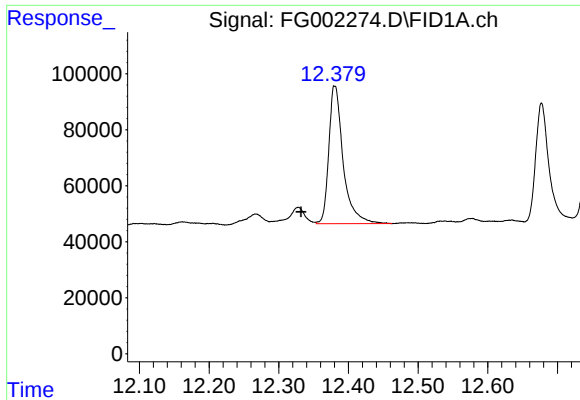

#7 N-EICOSANE


R.T.: 12.380 min
Delta R.T.: 0.048 min
Response: 704167
Conc: 4.96 ug/ml

Instrument :
FID_G
ClientSampleId :

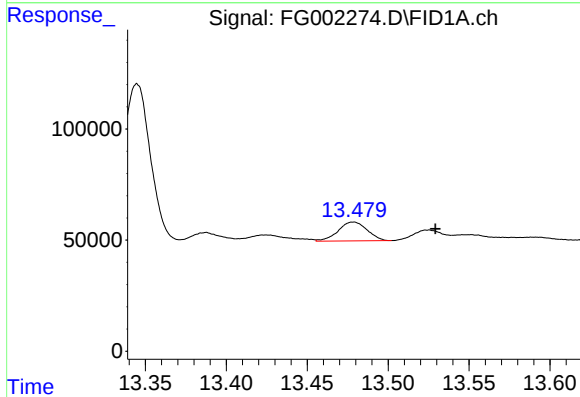


#8 N-DOCOSANE

R.T.: 13.478 min
Delta R.T.: -0.051 min
Response: 105544
Conc: 0.74 ug/ml

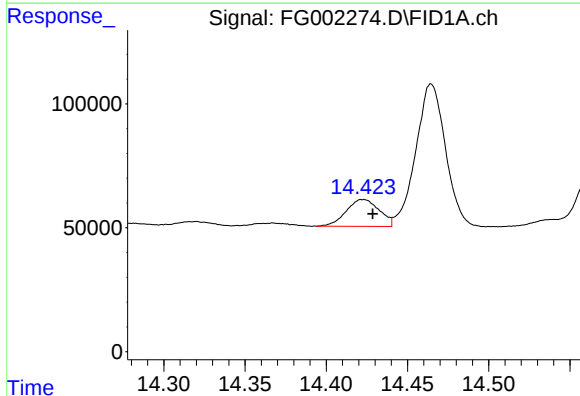


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.423 min
Delta R.T.: -0.006 min
Response: 153276
Conc: 1.21 ug/ml

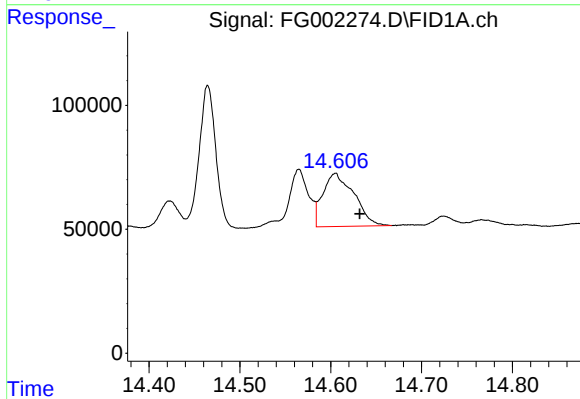

#10 N-TETRACOSANE


R.T.: 14.605 min
Delta R.T.: -0.027 min
Response: 509085
Conc: 3.56 ug/ml

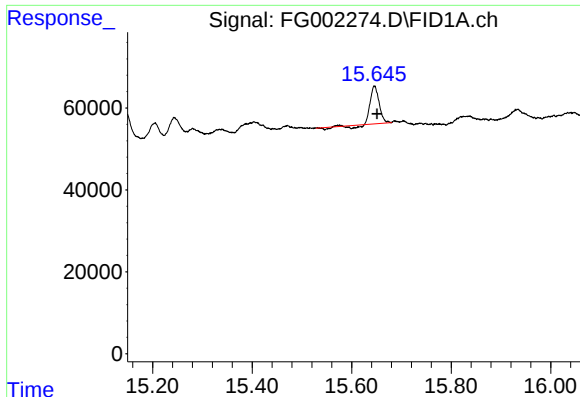

#11 N-HEXACOSANE


R.T.: 15.646 min
Delta R.T.: -0.005 min
Response: 102370
Conc: 0.71 ug/ml

Instrument :
FID_G
ClientSampleId :

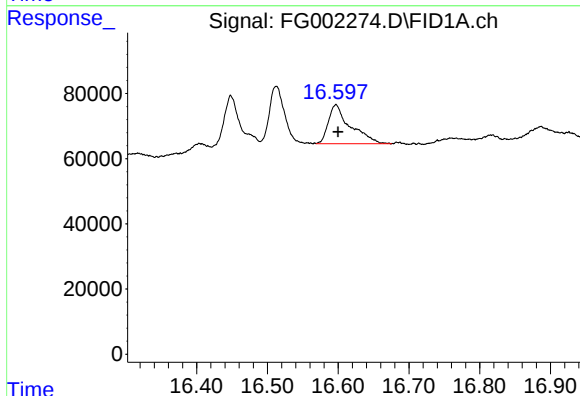


#12 N-OCTACOSANE

R.T.: 16.597 min
Delta R.T.: -0.003 min
Response: 257100
Conc: 1.76 ug/ml

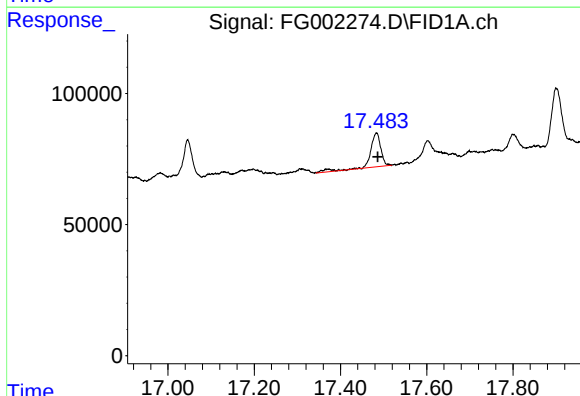


#13 N-TRIACONTANE

R.T.: 17.484 min
Delta R.T.: -0.003 min
Response: 219925
Conc: 1.45 ug/ml

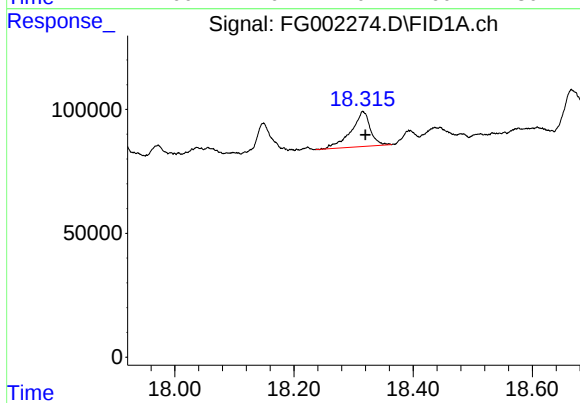

#14 N-DOTRIACONTANE


R.T.: 18.316 min
Delta R.T.: -0.004 min
Response: 316705
Conc: 2.15 ug/ml

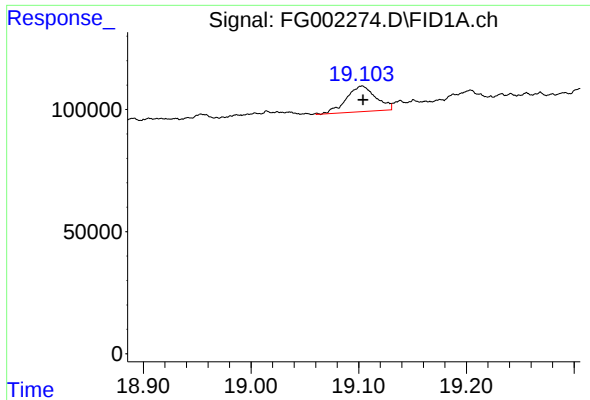

#15 N-TETRATRIACONTANE

R.T.: 19.103 min
Delta R.T.: 0.000 min
Response: 199362
Conc: 1.45 ug/ml

Instrument :
FID_G
ClientSampleId :

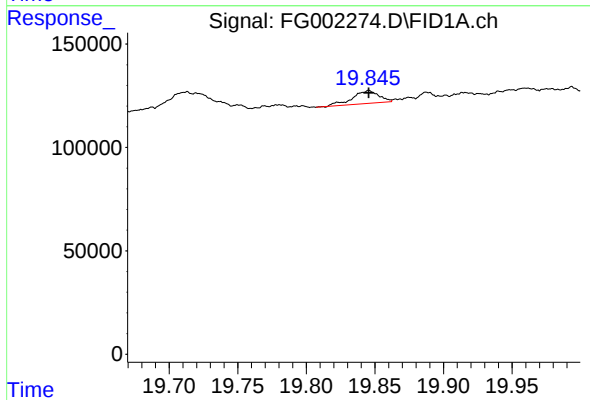

#16 N-HEXATRIACONTANE

R.T.: 19.846 min
Delta R.T.: 0.000 min
Response: 83158
Conc: 0.65 ug/ml