

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG091018\
Data File : FG002278.D
Signal(s) : FID1A.ch
Acq On : 10 Sep 2018 19:08
Operator : AJ\SJ
Sample : PB112714BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 11 04:16:54 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG083018.M
Quant Title :
QLast Update : Thu Aug 30 14:49:31 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.425	1696580	13.448 ug/ml
Target Compounds			
14) N-DOTRIACONTANE	18.317	69101	0.469 ug/ml
16) N-HEXATRIACONTANE	19.875	245862	1.917 ug/ml
18) N-TETRACONTANE	21.351	118928	1.096 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG091018\
Data File : FG002278.D
Signal(s) : FID1A.ch
Acq On : 10 Sep 2018 19:08
Operator : AJ\SJ
Sample : PB112714BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
FID_G
ClientSampled :

Integration File: autoint1.e
Quant Time: Sep 11 04:16:54 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG083018.M
Quant Title :
QLast Update : Thu Aug 30 14:49:31 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

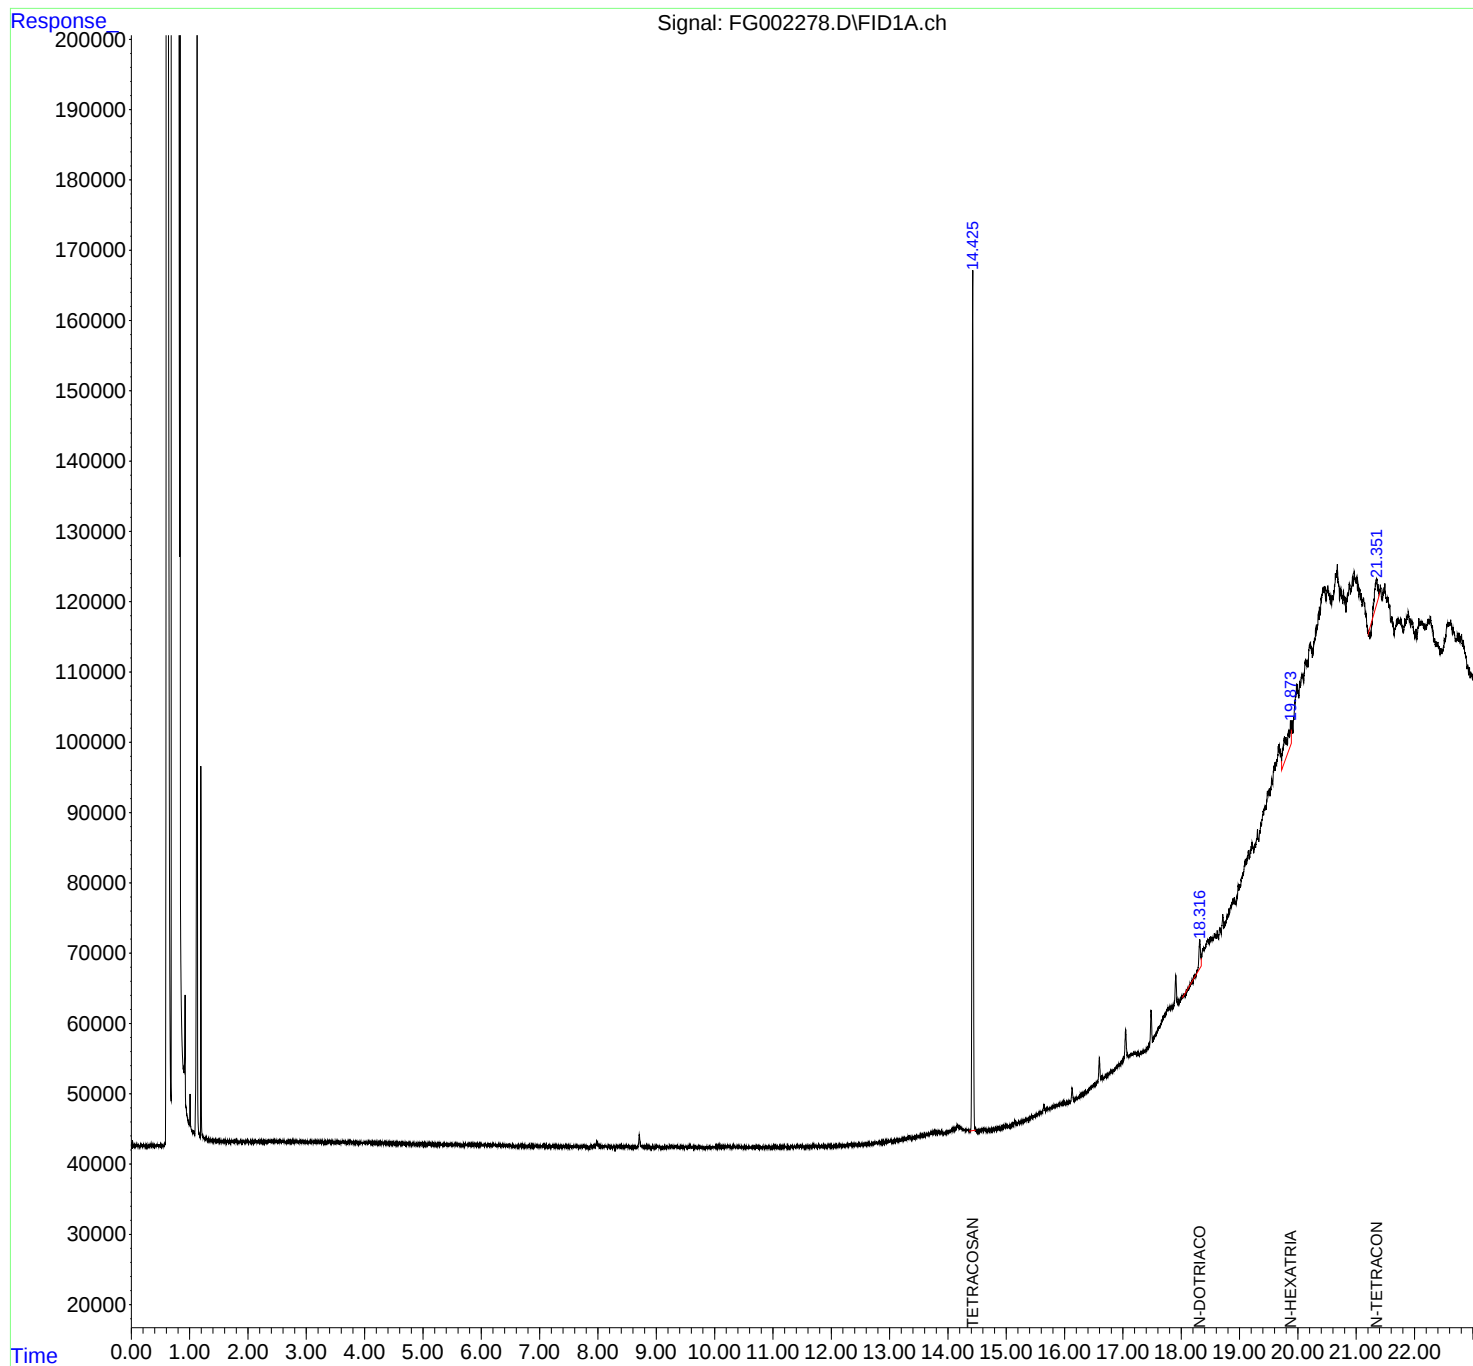


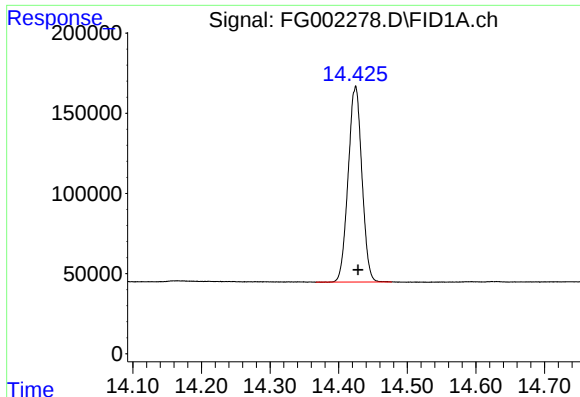

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.425 min
Delta R.T.: -0.004 min
Response: 1696580
Conc: 13.45 ug/ml

Instrument :
FID_G
ClientSampleId :

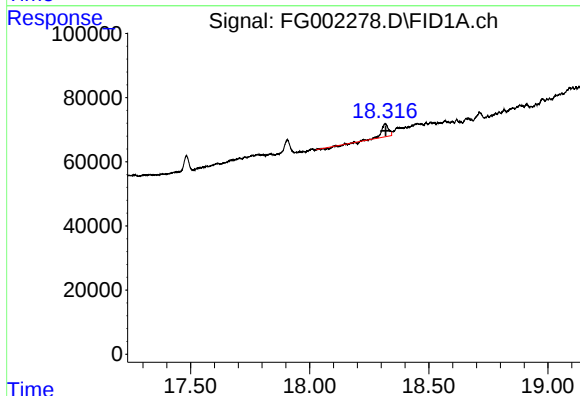


#14 N-DOTRIACONTANE

R.T.: 18.317 min
Delta R.T.: -0.003 min
Response: 69101
Conc: 0.47 ug/ml

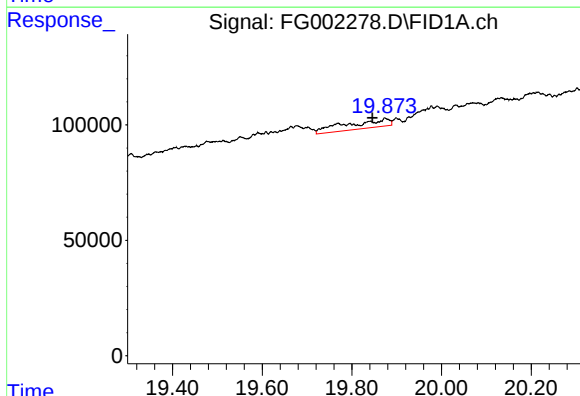

#16 N-HEXATRIACONTANE

R.T.: 19.875 min
Delta R.T.: 0.029 min
Response: 245862
Conc: 1.92 ug/ml

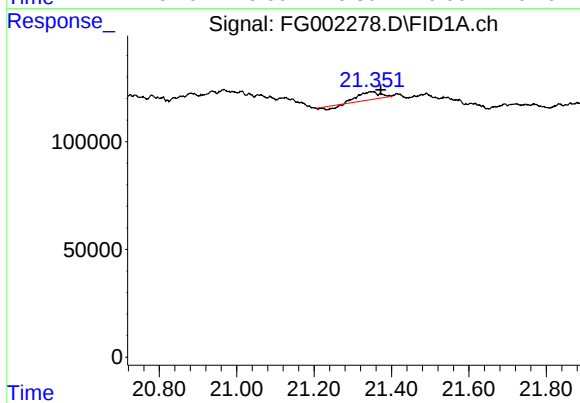

#18 N-TETRACONTANE

R.T.: 21.351 min
Delta R.T.: -0.021 min
Response: 118928
Conc: 1.10 ug/ml