

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG091018\
 Data File : FG002287.D
 Signal(s) : FID1A.ch
 Acq On : 10 Sep 2018 23:38
 Operator : AJ\SJ
 Sample : J4777-01 10X
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Sep 11 04:17:59 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG083018.M
 Quant Title :
 QLast Update : Thu Aug 30 14:49:31 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.425	105058	0.833 ug/ml
Target Compounds			
7) N-EICOSANE	12.385f	405458	2.854 ug/ml
10) N-TETRACOSANE	14.609	269359	1.884 ug/ml
13) N-TRIACONTANE	17.482	211026	1.391 ug/ml
14) N-DOTRIACONTANE	18.314	204229	1.385 ug/ml
15) N-TETRATRIACONTANE	19.110	182341	1.322 ug/ml
16) N-HEXATRIACONTANE	19.844	74836	0.584 ug/ml
18) N-TETRACONTANE	21.398	296333	2.731 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG091018\
Data File : FG002287.D
Signal(s) : FID1A.ch
Acq On : 10 Sep 2018 23:38
Operator : AJ\SJ
Sample : J4777-01 10X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 11 04:17:59 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG083018.M
Quant Title :
QLast Update : Thu Aug 30 14:49:31 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

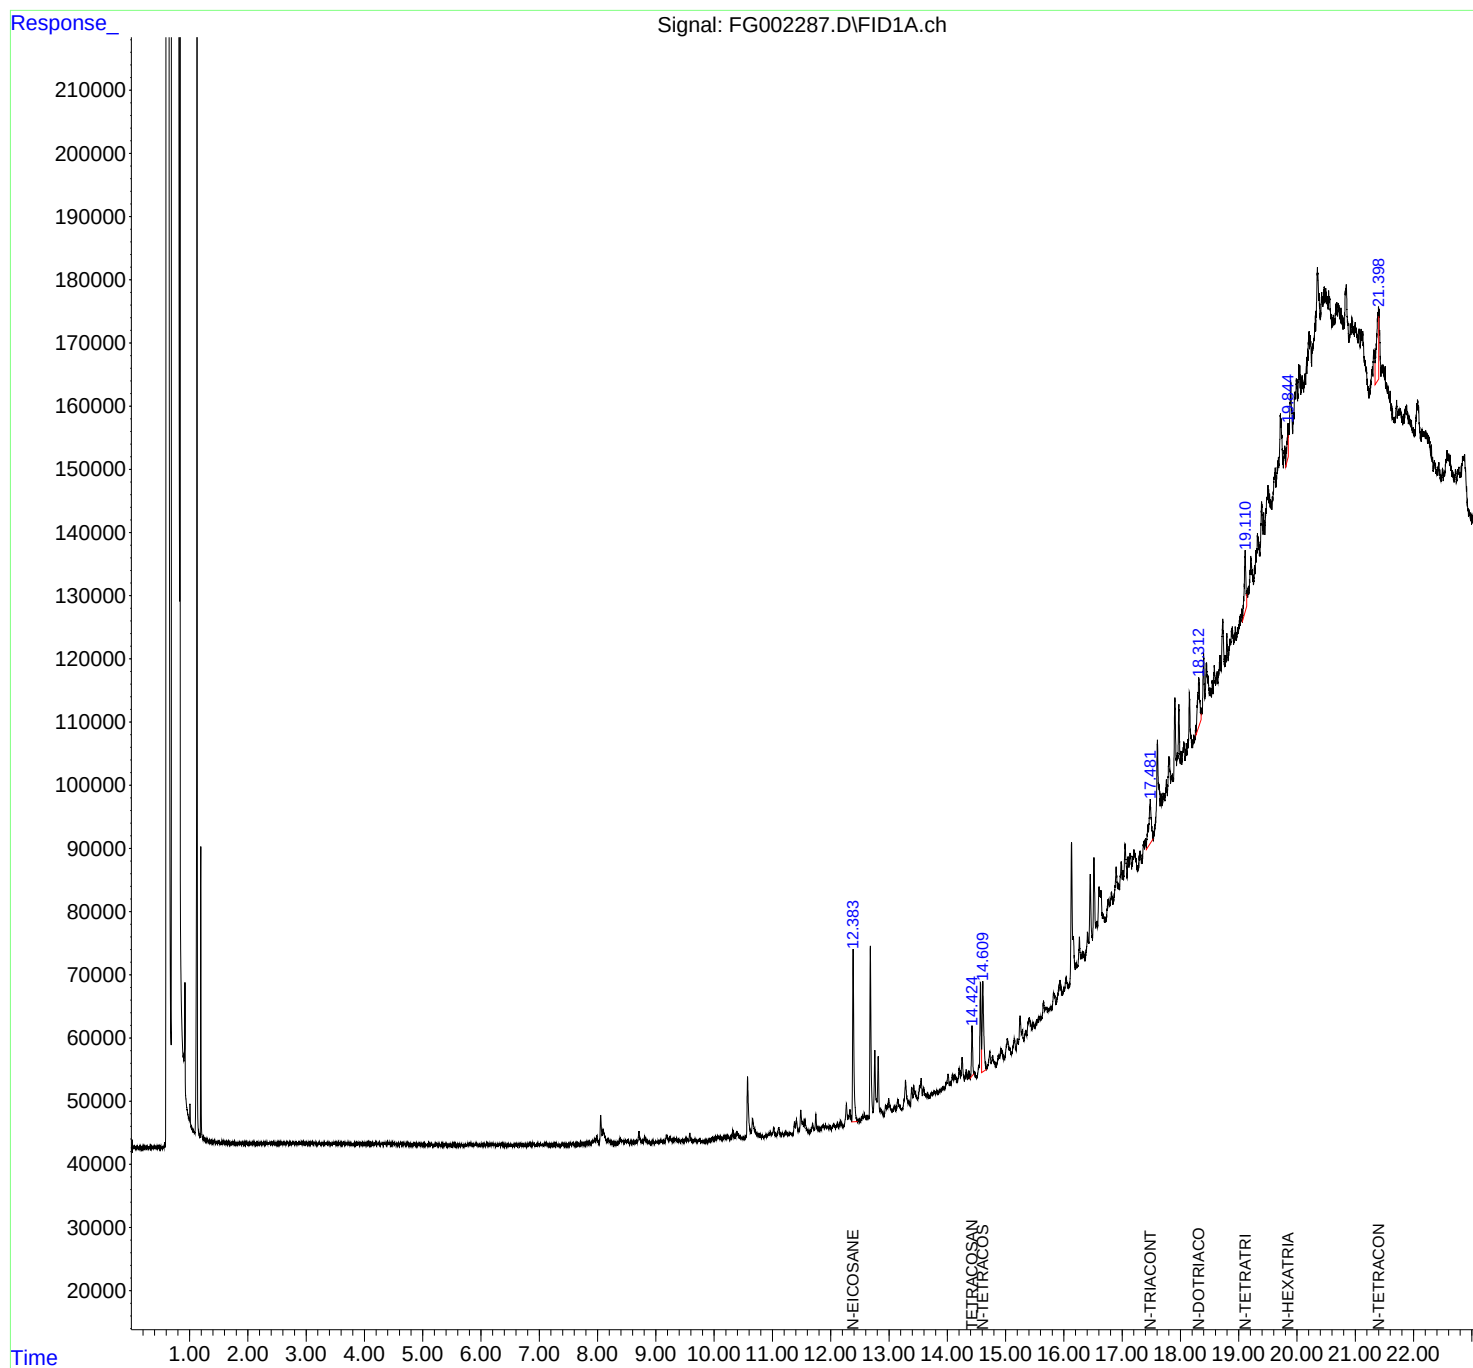


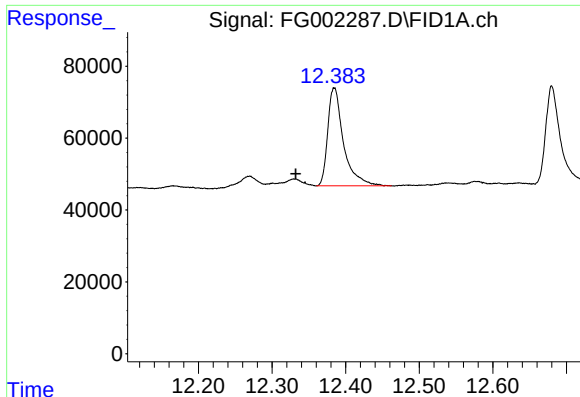

#7 N-EICOSANE


R.T.: 12.385 min
Delta R.T.: 0.052 min
Response: 405458
Conc: 2.85 ug/ml

Instrument :
FID_G
ClientSampleId :

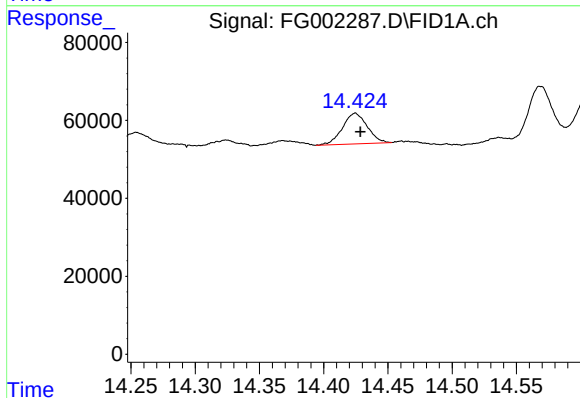


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.425 min
Delta R.T.: -0.004 min
Response: 105058
Conc: 0.83 ug/ml

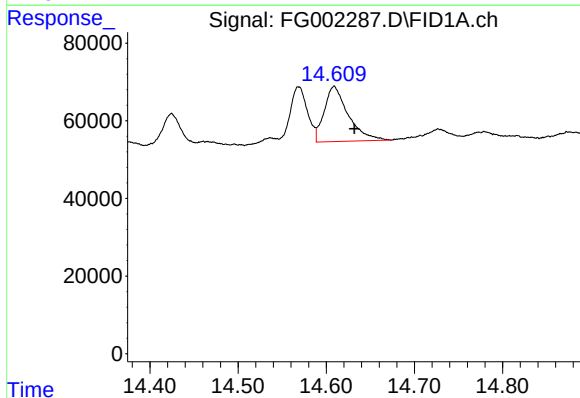


#10 N-TETRACOSANE

R.T.: 14.609 min
Delta R.T.: -0.023 min
Response: 269359
Conc: 1.88 ug/ml

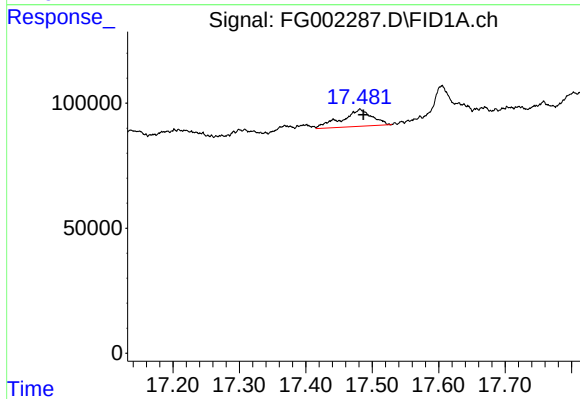

#13 N-TRIACONTANE


R.T.: 17.482 min
Delta R.T.: -0.005 min
Response: 211026
Conc: 1.39 ug/ml

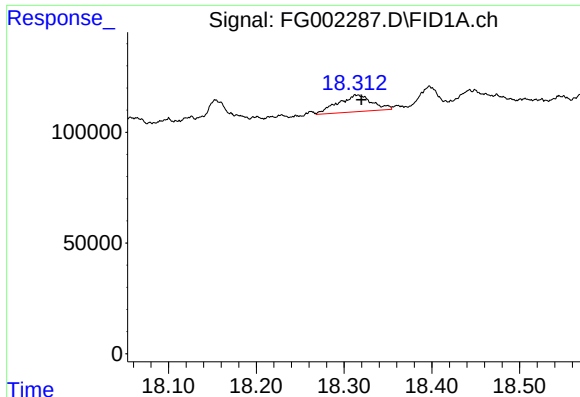

#14 N-DOTRIACONTANE


R.T.: 18.314 min
Delta R.T.: -0.006 min
Response: 204229
Conc: 1.38 ug/ml

Instrument :
FID_G
ClientSampleId :

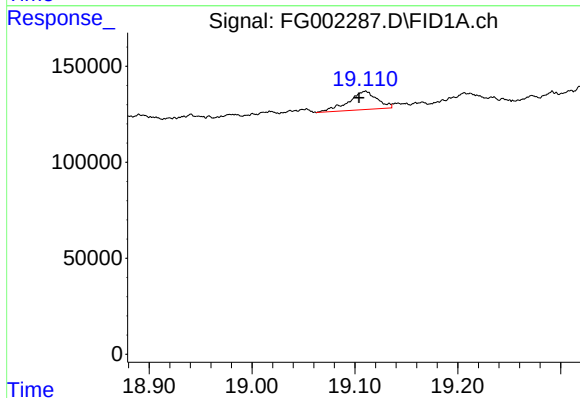


#15 N-TETRATRIACONTANE

R.T.: 19.110 min
Delta R.T.: 0.006 min
Response: 182341
Conc: 1.32 ug/ml

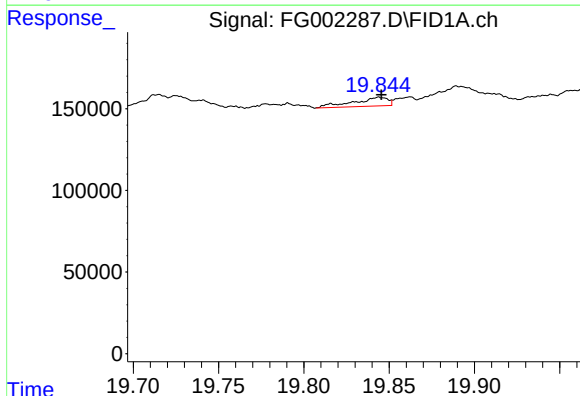

#16 N-HEXATRIACONTANE

R.T.: 19.844 min
Delta R.T.: -0.001 min
Response: 74836
Conc: 0.58 ug/ml

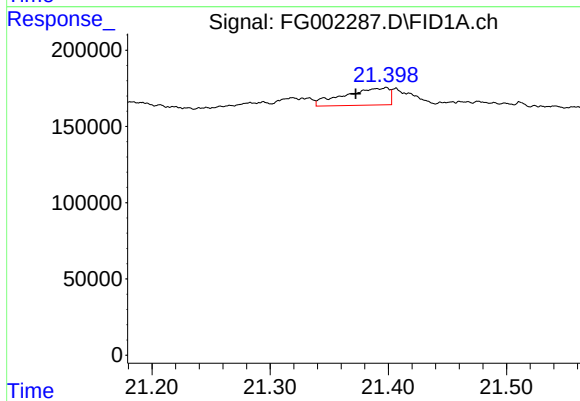

#18 N-TETRACONTANE

R.T.: 21.398 min
Delta R.T.: 0.026 min
Response: 296333
Conc: 2.73 ug/ml