

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG091018\
 Data File : FG002290.D
 Signal(s) : FID1A.ch
 Acq On : 11 Sep 2018 01:08
 Operator : AJ\SJ
 Sample : J4777-03 10X
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Sep 11 04:18:31 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG083018.M
 Quant Title :
 QLast Update : Thu Aug 30 14:49:31 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.425	170496	1.351 ug/ml
Target Compounds			
4) N-TETRADECANE	8.052f	72669	0.554 ug/ml
7) N-EICOSANE	12.385f	361214	2.543 ug/ml
10) N-TETRACOSANE	14.611	236129	1.652 ug/ml
12) N-OCTACOSANE	16.604	102525	0.701 ug/ml
13) N-TRIACONTANE	17.482	229056	1.510 ug/ml
14) N-DOTRIACONTANE	18.321	320772	2.175 ug/ml
15) N-TETRATRIACONTANE	19.109	137295	0.995 ug/ml
16) N-HEXATRIACONTANE	19.847	98594	0.769 ug/ml
18) N-TETRACONTANE	21.356	27005	0.249 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG091018\
Data File : FG002290.D
Signal(s) : FID1A.ch
Acq On : 11 Sep 2018 01:08
Operator : AJ\SJ
Sample : J4777-03 10X
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
FID_G
ClientSampled :

Integration File: autoint1.e
Quant Time: Sep 11 04:18:31 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG083018.M
Quant Title :
QLast Update : Thu Aug 30 14:49:31 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

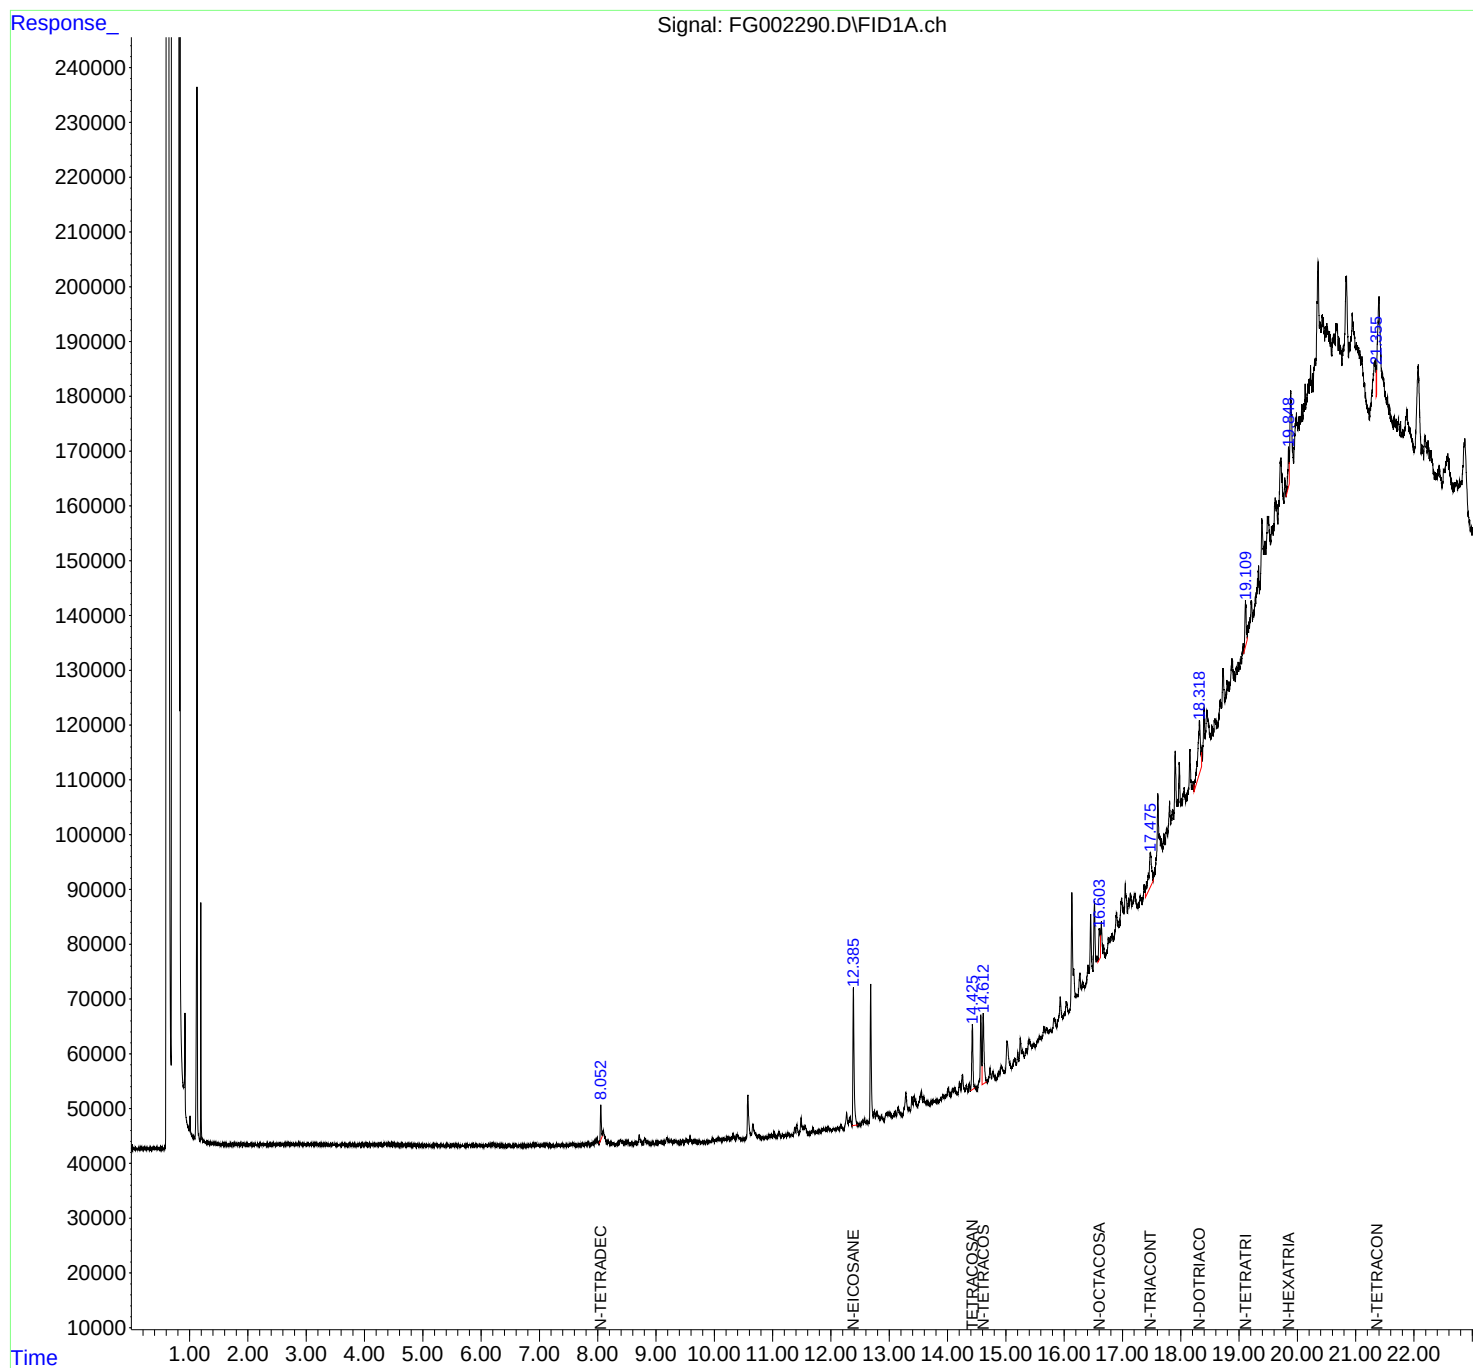


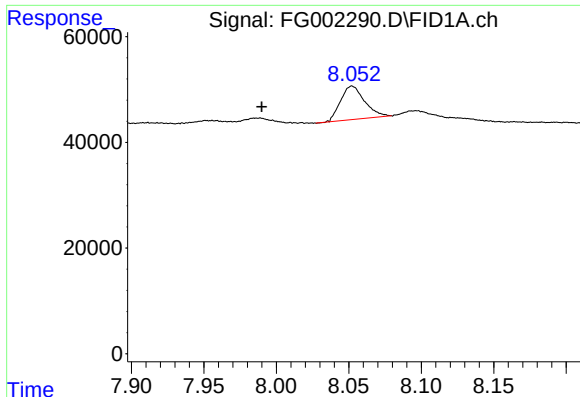

#4 N-TETRADECANE


R.T.: 8.052 min
Delta R.T.: 0.062 min
Response: 72669
Conc: 0.55 ug/ml

Instrument :
FID_G
ClientSampleId :

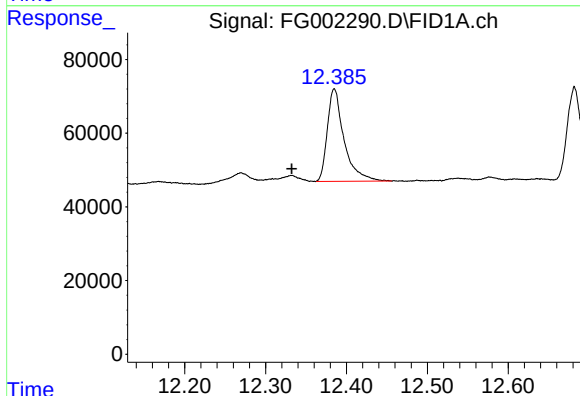


#7 N-EICOSANE

R.T.: 12.385 min
Delta R.T.: 0.053 min
Response: 361214
Conc: 2.54 ug/ml

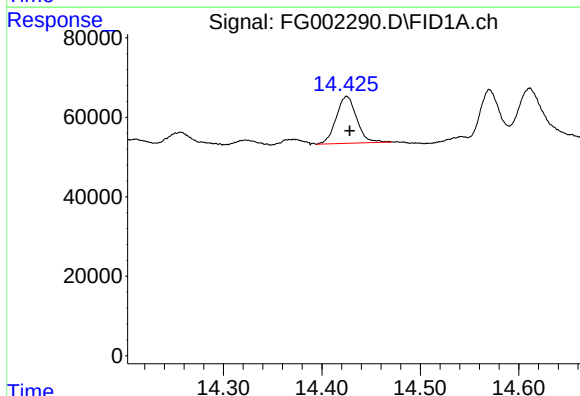


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.425 min
Delta R.T.: -0.003 min
Response: 170496
Conc: 1.35 ug/ml

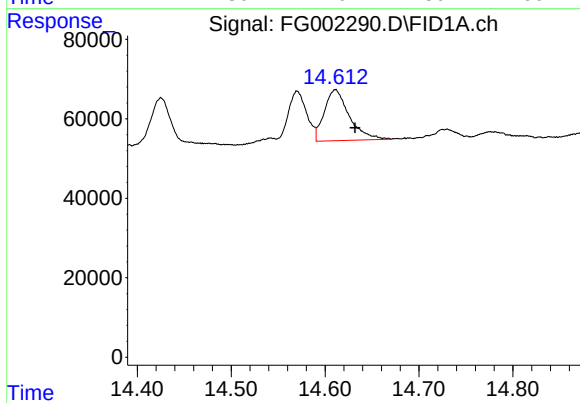

#10 N-TETRACOSANE


R.T.: 14.611 min
Delta R.T.: -0.021 min
Response: 236129
Conc: 1.65 ug/ml

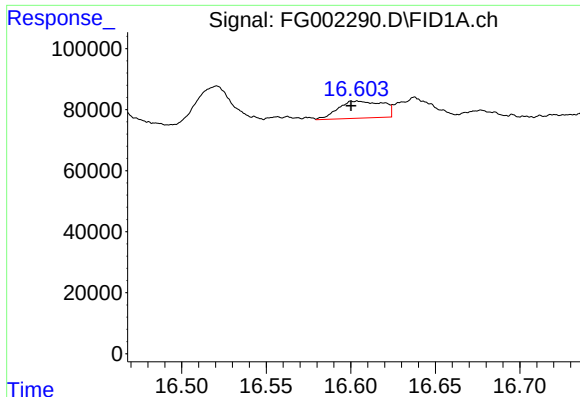

#12 N-OCTACOSANE


R.T.: 16.604 min
Delta R.T.: 0.004 min
Response: 102525
Conc: 0.70 ug/ml

Instrument :
FID_G
ClientSampleId :

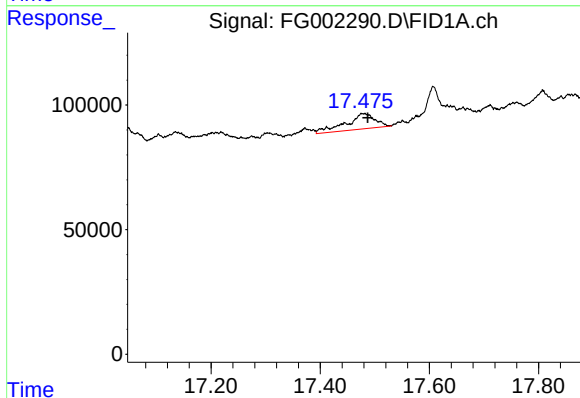


#13 N-TRIACONTANE

R.T.: 17.482 min
Delta R.T.: -0.005 min
Response: 229056
Conc: 1.51 ug/ml

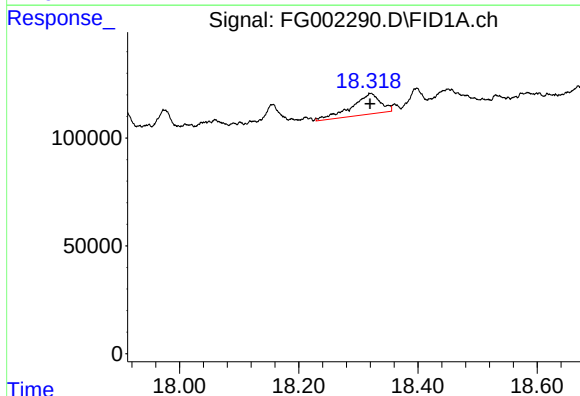


#14 N-DOTRIACONTANE

R.T.: 18.321 min
Delta R.T.: 0.000 min
Response: 320772
Conc: 2.17 ug/ml

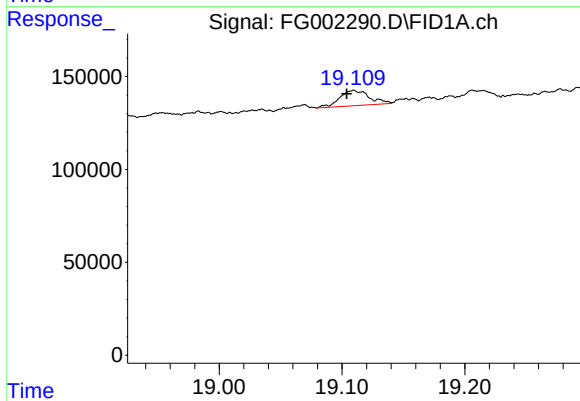

#15 N-TETRATRIACONTANE


R.T.: 19.109 min
Delta R.T.: 0.005 min
Response: 137295
Conc: 1.00 ug/ml

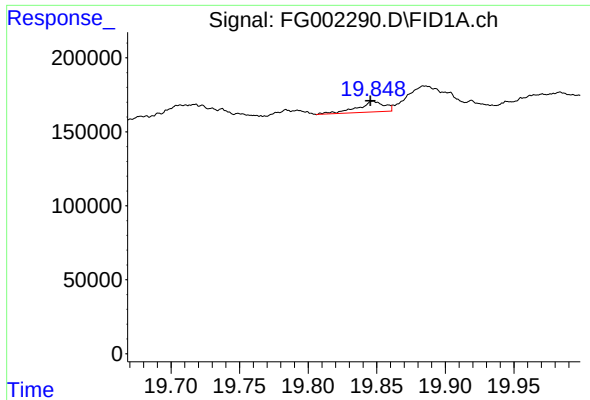

#16 N-HEXATRIACONTANE

R.T.: 19.847 min
Delta R.T.: 0.002 min
Response: 98594
Conc: 0.77 ug/ml

Instrument :
FID_G
ClientSampleId :

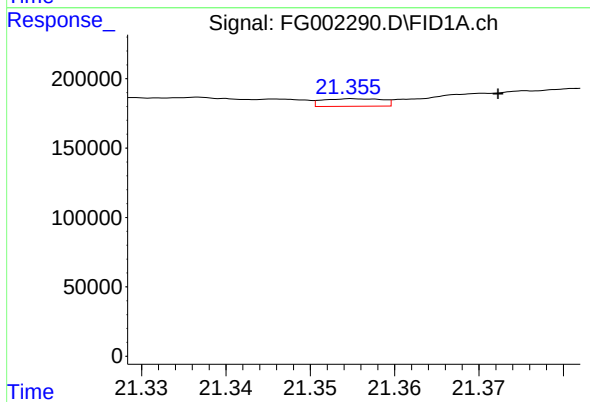

#18 N-TETRACONTANE

R.T.: 21.356 min
Delta R.T.: -0.017 min
Response: 27005
Conc: 0.25 ug/ml