

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG091018\
 Data File : FG002291.D
 Signal(s) : FID1A.ch
 Acq On : 11 Sep 2018 01:38
 Operator : AJ\SJ
 Sample : J4777-05 10X
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Sep 11 04:18:42 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG083018.M
 Quant Title :
 QLast Update : Thu Aug 30 14:49:31 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.426	153229	1.215 ug/ml
Target Compounds			
4) N-TETRADECANE	8.053f	66377	0.506 ug/ml
7) N-EICOSANE	12.383f	631923	4.448 ug/ml
10) N-TETRACOSANE	14.608	359096	2.512 ug/ml
12) N-OCTACOSANE	16.609	204601	1.398 ug/ml
13) N-TRIACONTANE	17.484	197481	1.302 ug/ml
14) N-DOTRIACONTANE	18.317	282634	1.916 ug/ml
15) N-TETRATRIACONTANE	19.110	201220	1.458 ug/ml
16) N-HEXATRIACONTANE	19.851	68141	0.531 ug/ml
17) N-OCTATRIACONTANE	20.494f	156780	1.395 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG091018\
Data File : FG002291.D
Signal(s) : FID1A.ch
Acq On : 11 Sep 2018 01:38
Operator : AJ\SJ
Sample : J4777-05 10X
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 11 04:18:42 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG083018.M
Quant Title :
QLast Update : Thu Aug 30 14:49:31 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

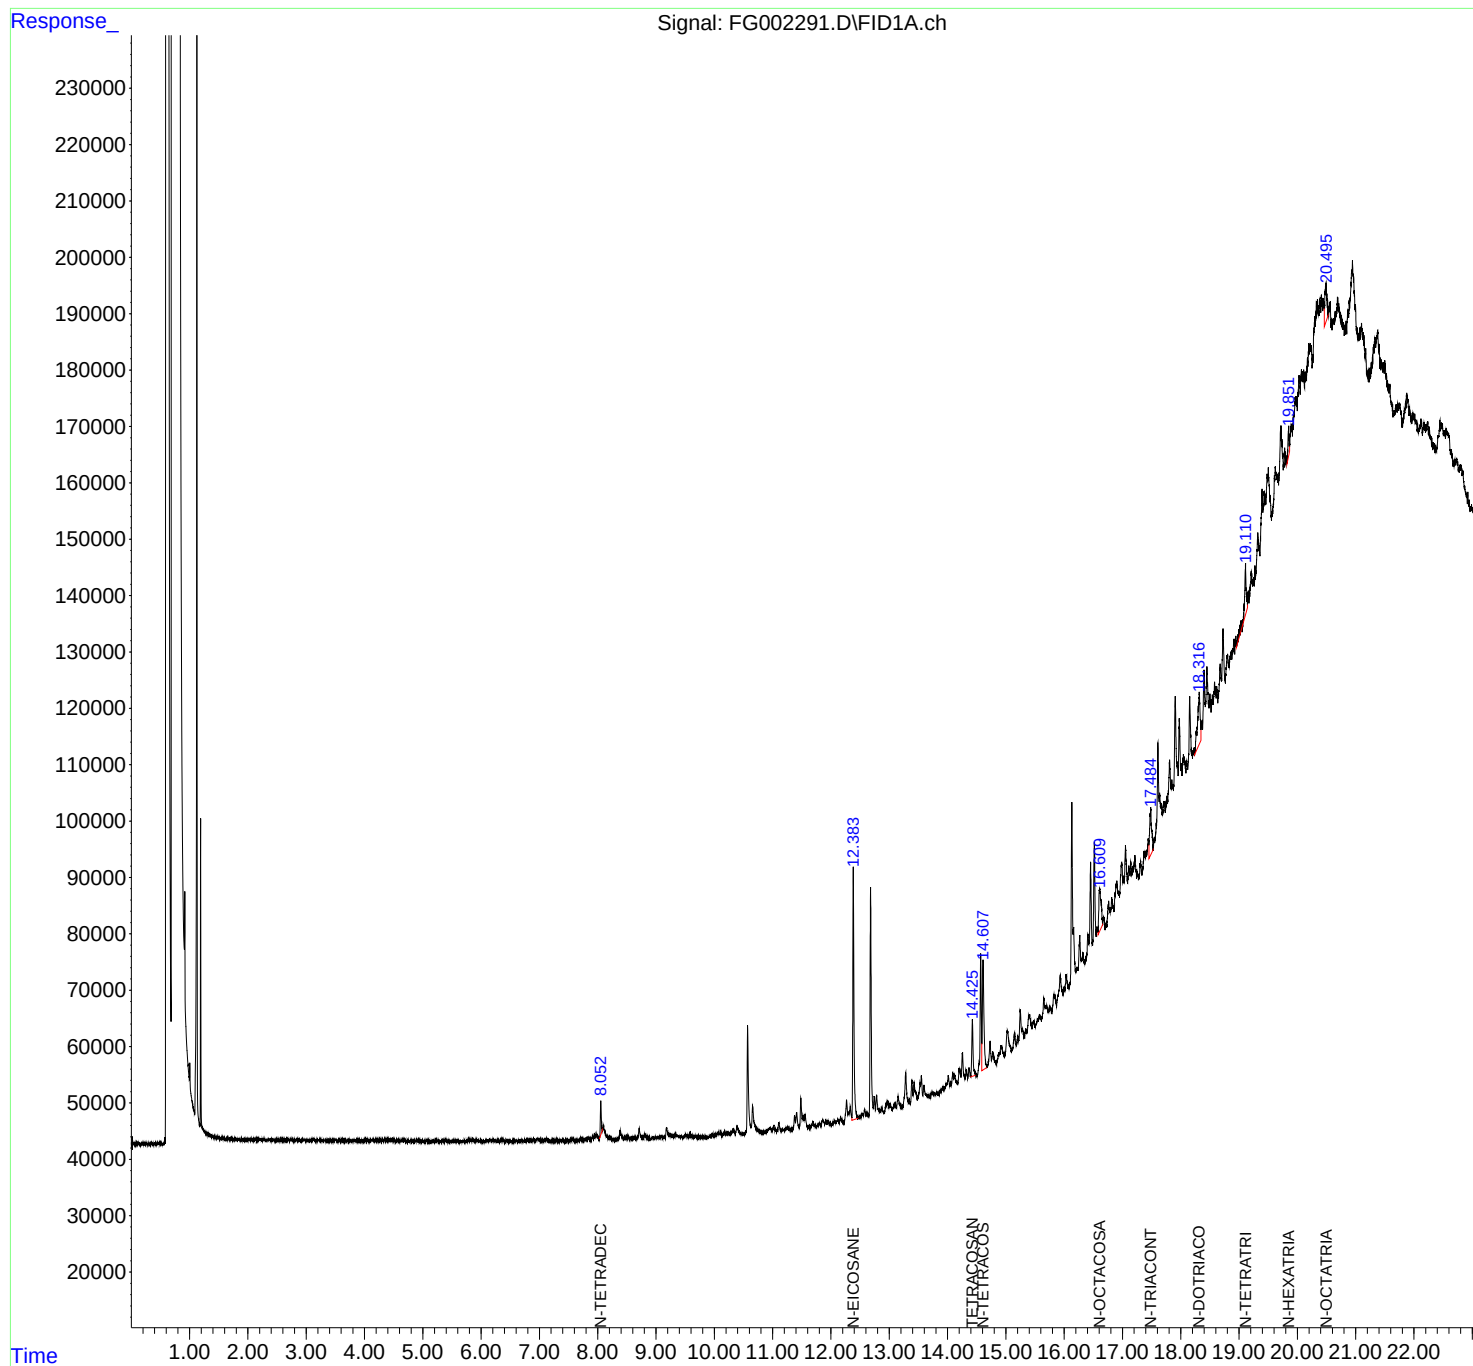


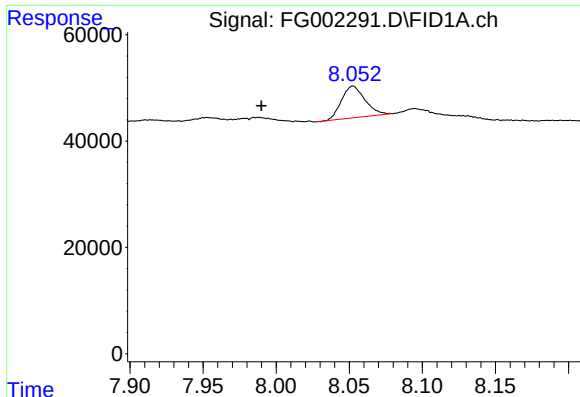

#4 N-TETRADECANE


R.T.: 8.053 min
Delta R.T.: 0.063 min
Response: 66377
Conc: 0.51 ug/ml

Instrument :
FID_G
ClientSampleId :

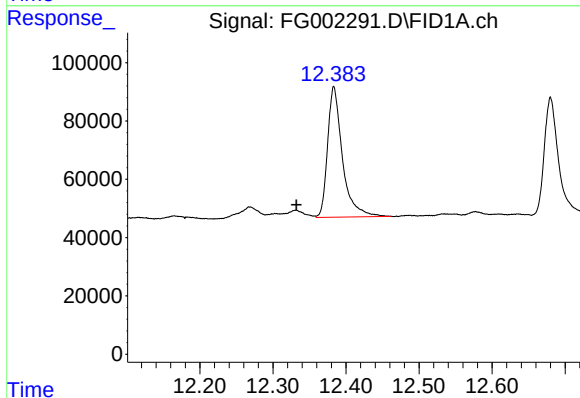


#7 N-EICOSANE

R.T.: 12.383 min
Delta R.T.: 0.051 min
Response: 631923
Conc: 4.45 ug/ml

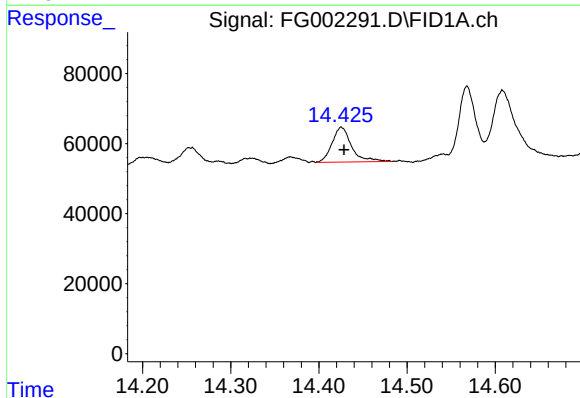


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.426 min
Delta R.T.: -0.003 min
Response: 153229
Conc: 1.21 ug/ml

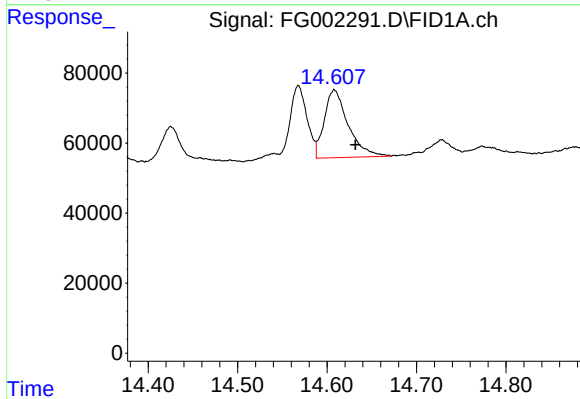

#10 N-TETRACOSANE


R.T.: 14.608 min
Delta R.T.: -0.024 min
Response: 359096
Conc: 2.51 ug/ml

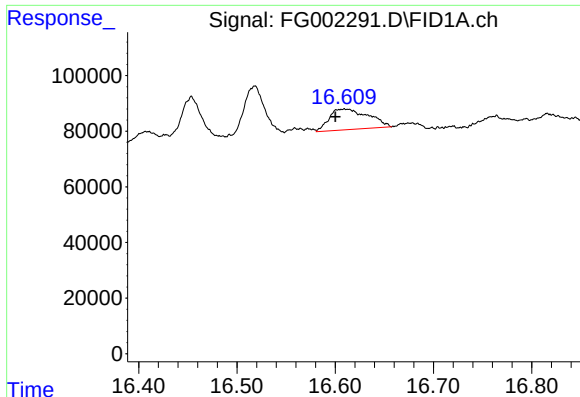

#12 N-OCTACOSANE


R.T.: 16.609 min
Delta R.T.: 0.009 min
Response: 204601
Conc: 1.40 ug/ml

Instrument :
FID_G
ClientSampleId :

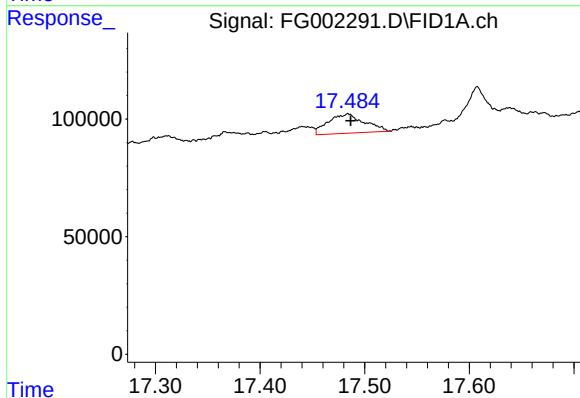


#13 N-TRIACONTANE

R.T.: 17.484 min
Delta R.T.: -0.002 min
Response: 197481
Conc: 1.30 ug/ml

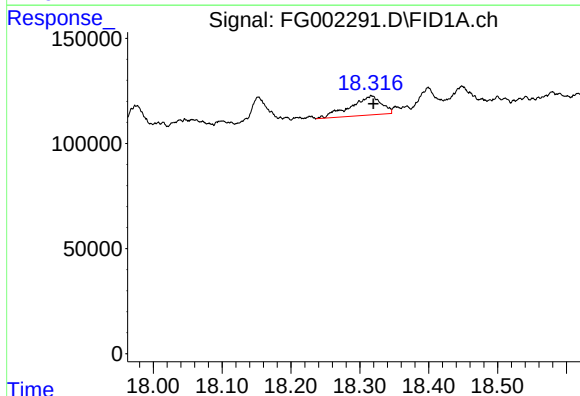


#14 N-DOTRIACONTANE

R.T.: 18.317 min
Delta R.T.: -0.003 min
Response: 282634
Conc: 1.92 ug/ml

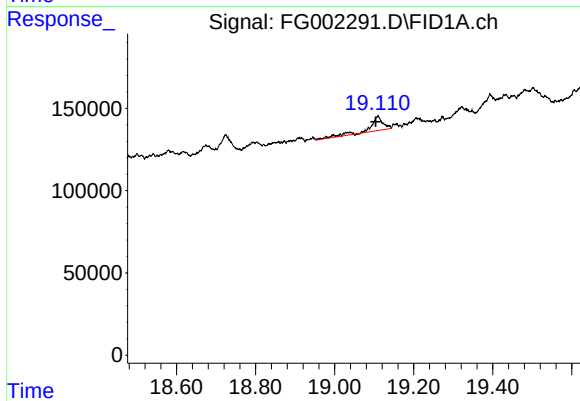

#15 N-TETRATRIACONTANE


R.T.: 19.110 min
Delta R.T.: 0.006 min
Response: 201220
Conc: 1.46 ug/ml

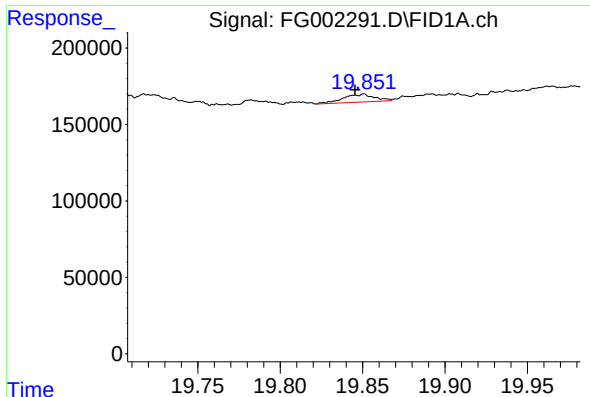

#16 N-HEXATRIACONTANE

R.T.: 19.851 min
Delta R.T.: 0.005 min
Response: 68141
Conc: 0.53 ug/ml

Instrument :
FID_G
ClientSampleId :

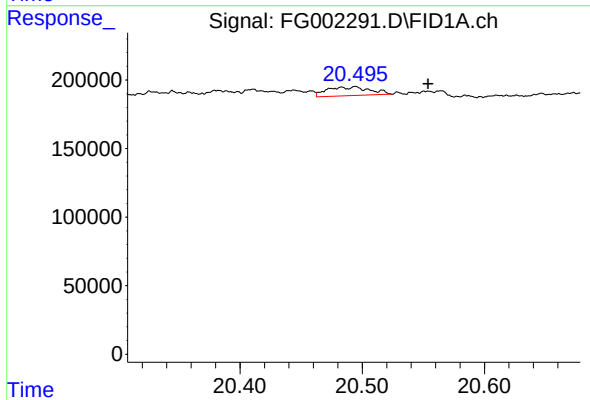

#17 N-OCTATRIACONTANE

R.T.: 20.494 min
Delta R.T.: -0.059 min
Response: 156780
Conc: 1.39 ug/ml