

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG091018\
 Data File : FG002292.D
 Signal(s) : FID1A.ch
 Acq On : 11 Sep 2018 02:08
 Operator : AJ\SJ
 Sample : J4777-07 10X
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Sep 11 04:18:54 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG083018.M
 Quant Title :
 QLast Update : Thu Aug 30 14:49:31 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.426	118028	0.936 ug/ml
Target Compounds			
7) N-EICOSANE	12.386f	395645	2.785 ug/ml
10) N-TETRACOSANE	14.609	321923	2.252 ug/ml
12) N-OCTACOSANE	16.612	428237	2.927 ug/ml
13) N-TRIACONTANE	17.477	590786	3.895 ug/ml
14) N-DOTRIACONTANE	18.312	1465805	9.938 ug/ml
15) N-TETRATRIACONTANE	19.116	1704373	12.354 ug/ml
16) N-HEXATRIACONTANE	19.858	2012331	15.691 ug/ml
17) N-OCTATRIACONTANE	20.564	1536833	13.670 ug/ml
18) N-TETRACONTANE	21.389	597035	5.501 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG091018\
Data File : FG002292.D
Signal(s) : FID1A.ch
Acq On : 11 Sep 2018 02:08
Operator : AJ\SJ
Sample : J4777-07 10X
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 11 04:18:54 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG083018.M
Quant Title :
QLast Update : Thu Aug 30 14:49:31 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

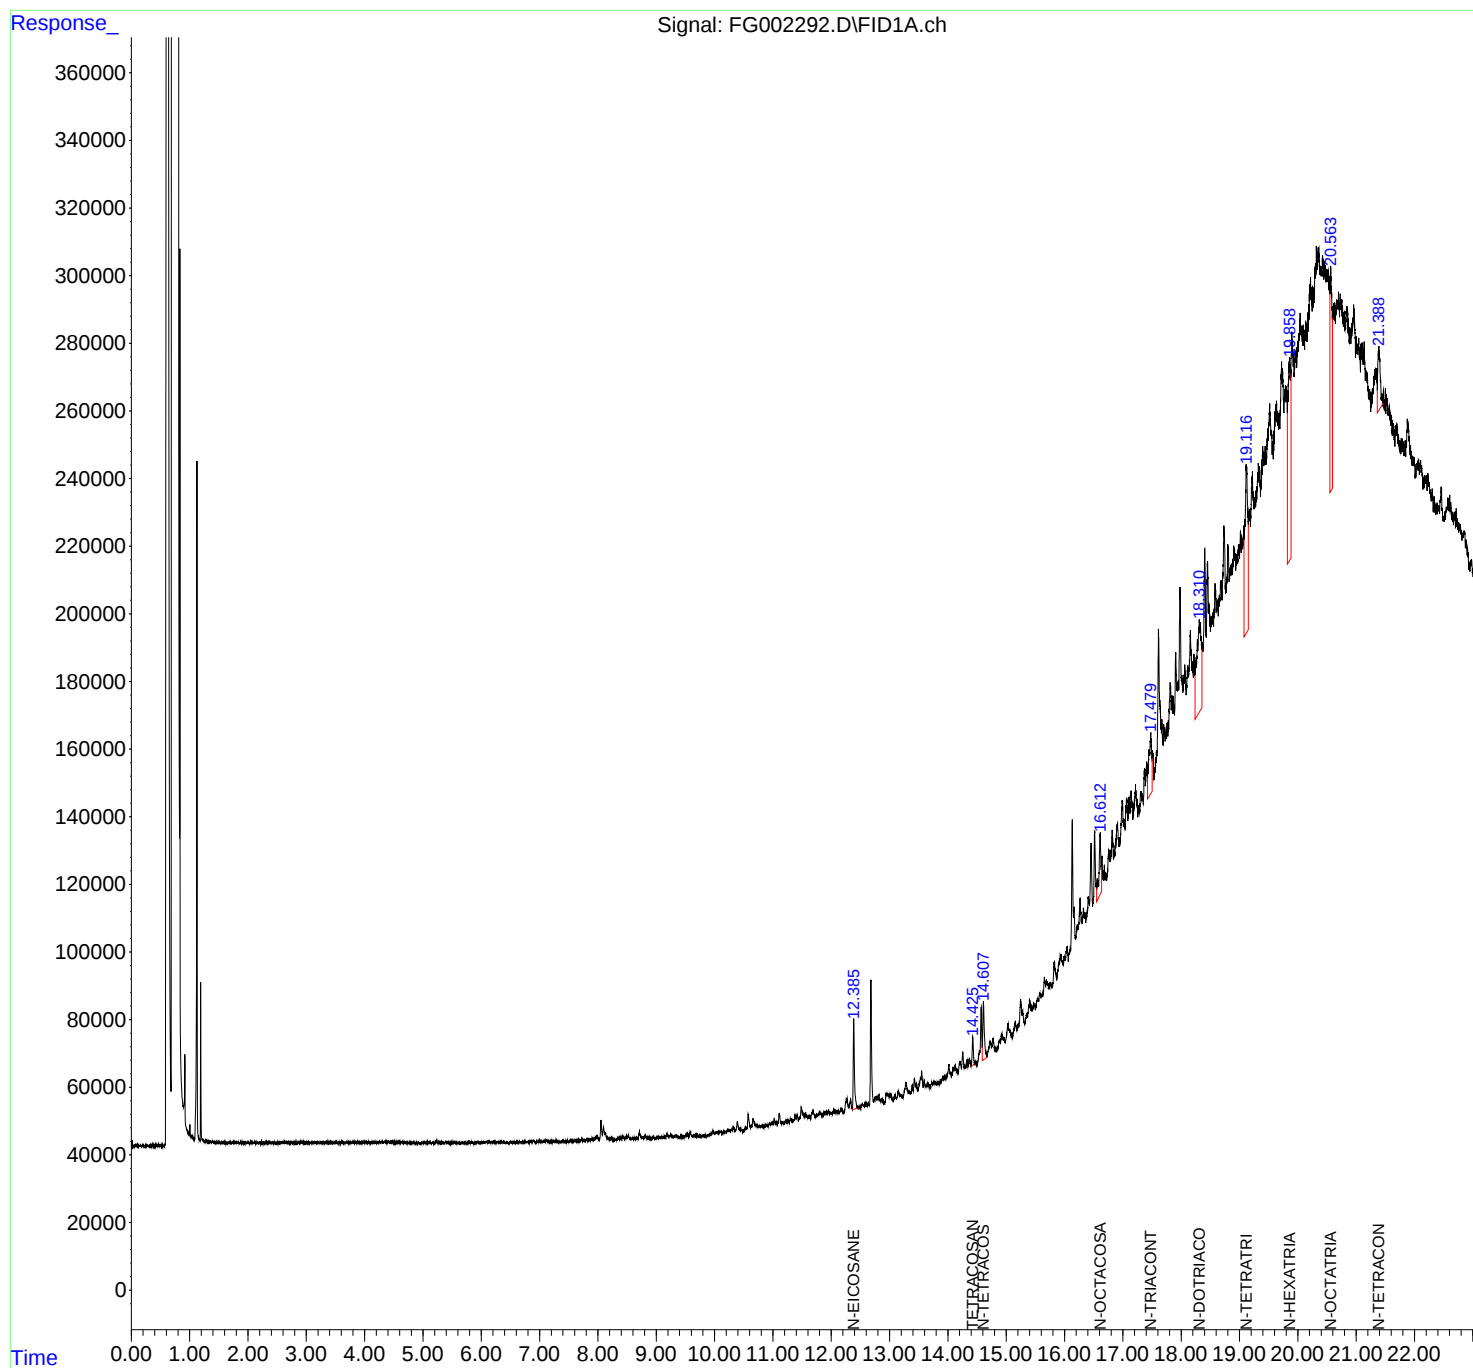


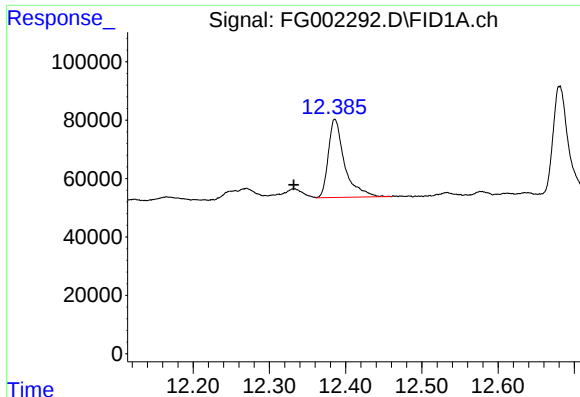

#7 N-EICOSANE


R.T.: 12.386 min
Delta R.T.: 0.054 min
Response: 395645
Conc: 2.78 ug/ml

Instrument :
FID_G
ClientSampleId :

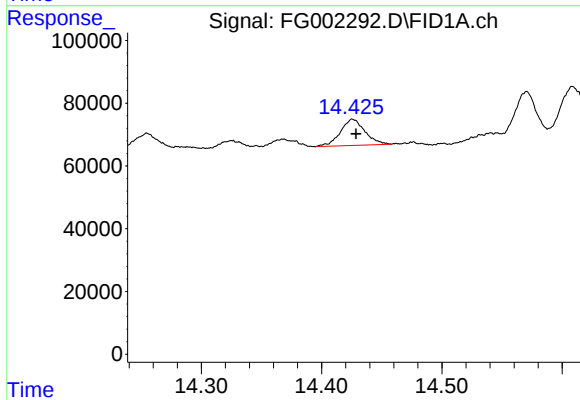


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.426 min
Delta R.T.: -0.003 min
Response: 118028
Conc: 0.94 ug/ml

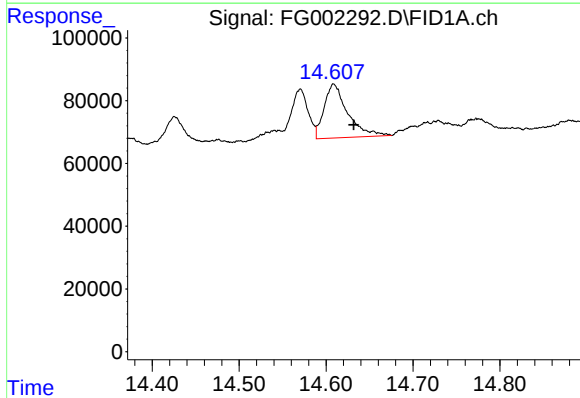


#10 N-TETRACOSANE

R.T.: 14.609 min
Delta R.T.: -0.023 min
Response: 321923
Conc: 2.25 ug/ml

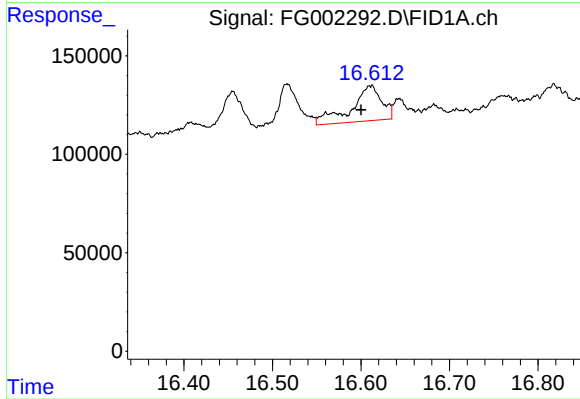

#12 N-OCTACOSANE


R.T.: 16.612 min
Delta R.T.: 0.011 min
Response: 428237
Conc: 2.93 ug/ml

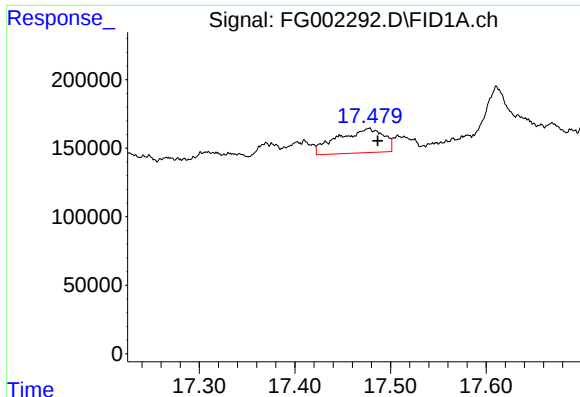

#13 N-TRIACONTANE


R.T.: 17.477 min
Delta R.T.: -0.009 min
Response: 590786
Conc: 3.89 ug/ml

Instrument :
FID_G
ClientSampleId :

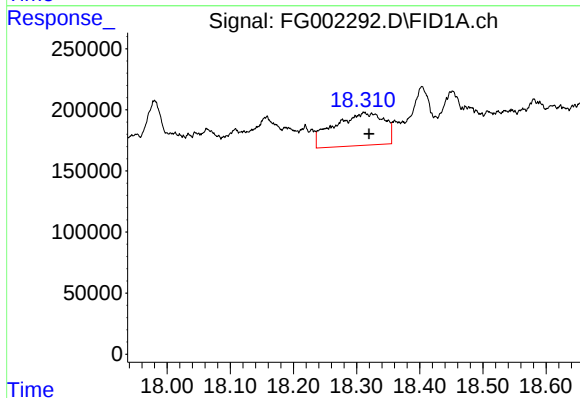


#14 N-DOTRIACONTANE

R.T.: 18.312 min
Delta R.T.: -0.008 min
Response: 1465805
Conc: 9.94 ug/ml

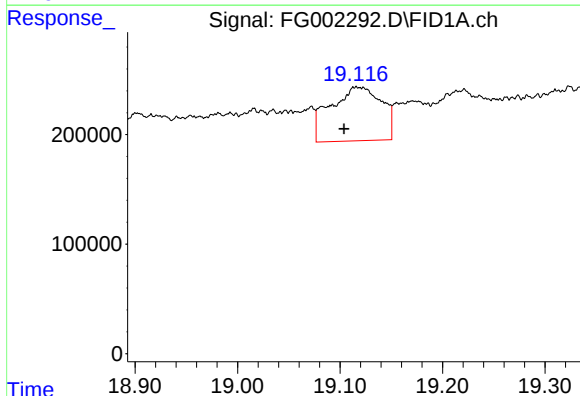


#15 N-TETRATRIACONTANE

R.T.: 19.116 min
Delta R.T.: 0.012 min
Response: 1704373
Conc: 12.35 ug/ml

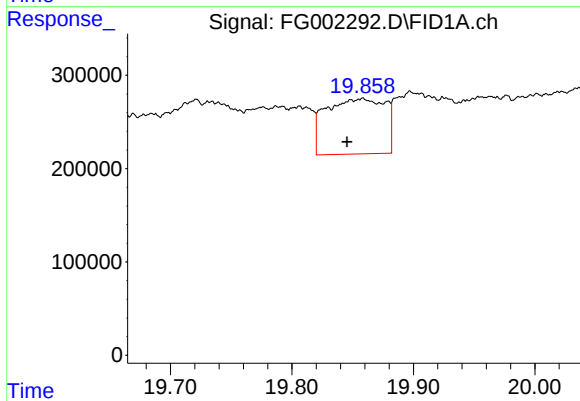

#16 N-HEXATRIACONTANE


R.T.: 19.858 min
Delta R.T.: 0.013 min
Response: 2012331
Conc: 15.69 ug/ml

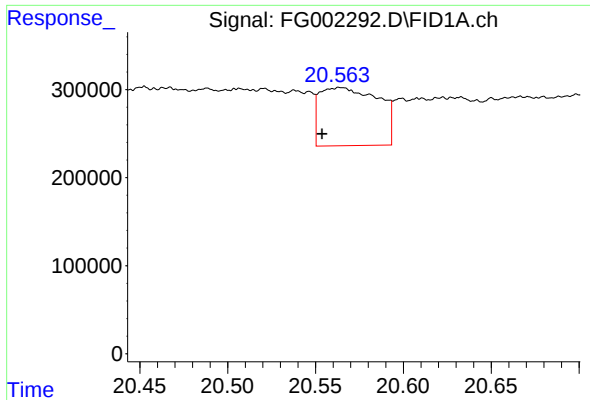

#17 N-OCTATRIACONTANE

R.T.: 20.564 min
Delta R.T.: 0.011 min
Response: 1536833
Conc: 13.67 ug/ml

Instrument :
FID_G
ClientSampleId :

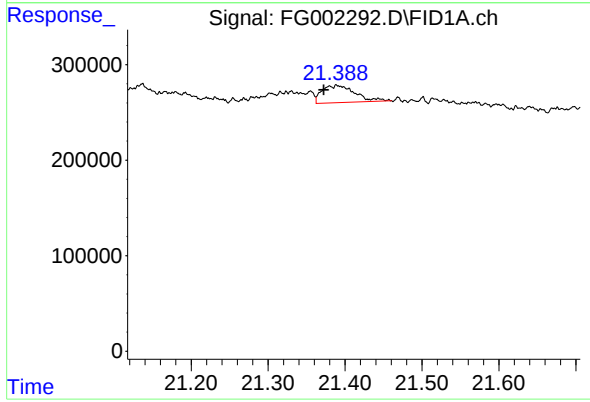

#18 N-TETRACONTANE

R.T.: 21.389 min
Delta R.T.: 0.017 min
Response: 597035
Conc: 5.50 ug/ml