

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG091018\
 Data File : FG002294.D
 Signal(s) : FID1A.ch
 Acq On : 11 Sep 2018 03:08
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Sep 11 04:19:22 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG083018.M
 Quant Title :
 QLast Update : Thu Aug 30 14:49:31 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.429	2150397	17.045 ug/ml
Target Compounds			
13) N-TRIACONTANE	17.486	41569	0.274 ug/ml
14) N-DOTRIACONTANE	18.321	147994	1.003 ug/ml
15) N-TETRATRIACONTANE	19.104	59548	0.432 ug/ml
16) N-HEXATRIACONTANE	19.814	156244	1.218 ug/ml
17) N-OCTATRIACONTANE	20.523	1198727	10.663 ug/ml
18) N-TETRACONTANE	21.369	75400	0.695 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG091018\
Data File : FG002294.D
Signal(s) : FID1A.ch
Acq On : 11 Sep 2018 03:08
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_G
ClientSampled :

Integration File: autoint1.e
Quant Time: Sep 11 04:19:22 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG083018.M
Quant Title :
QLast Update : Thu Aug 30 14:49:31 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

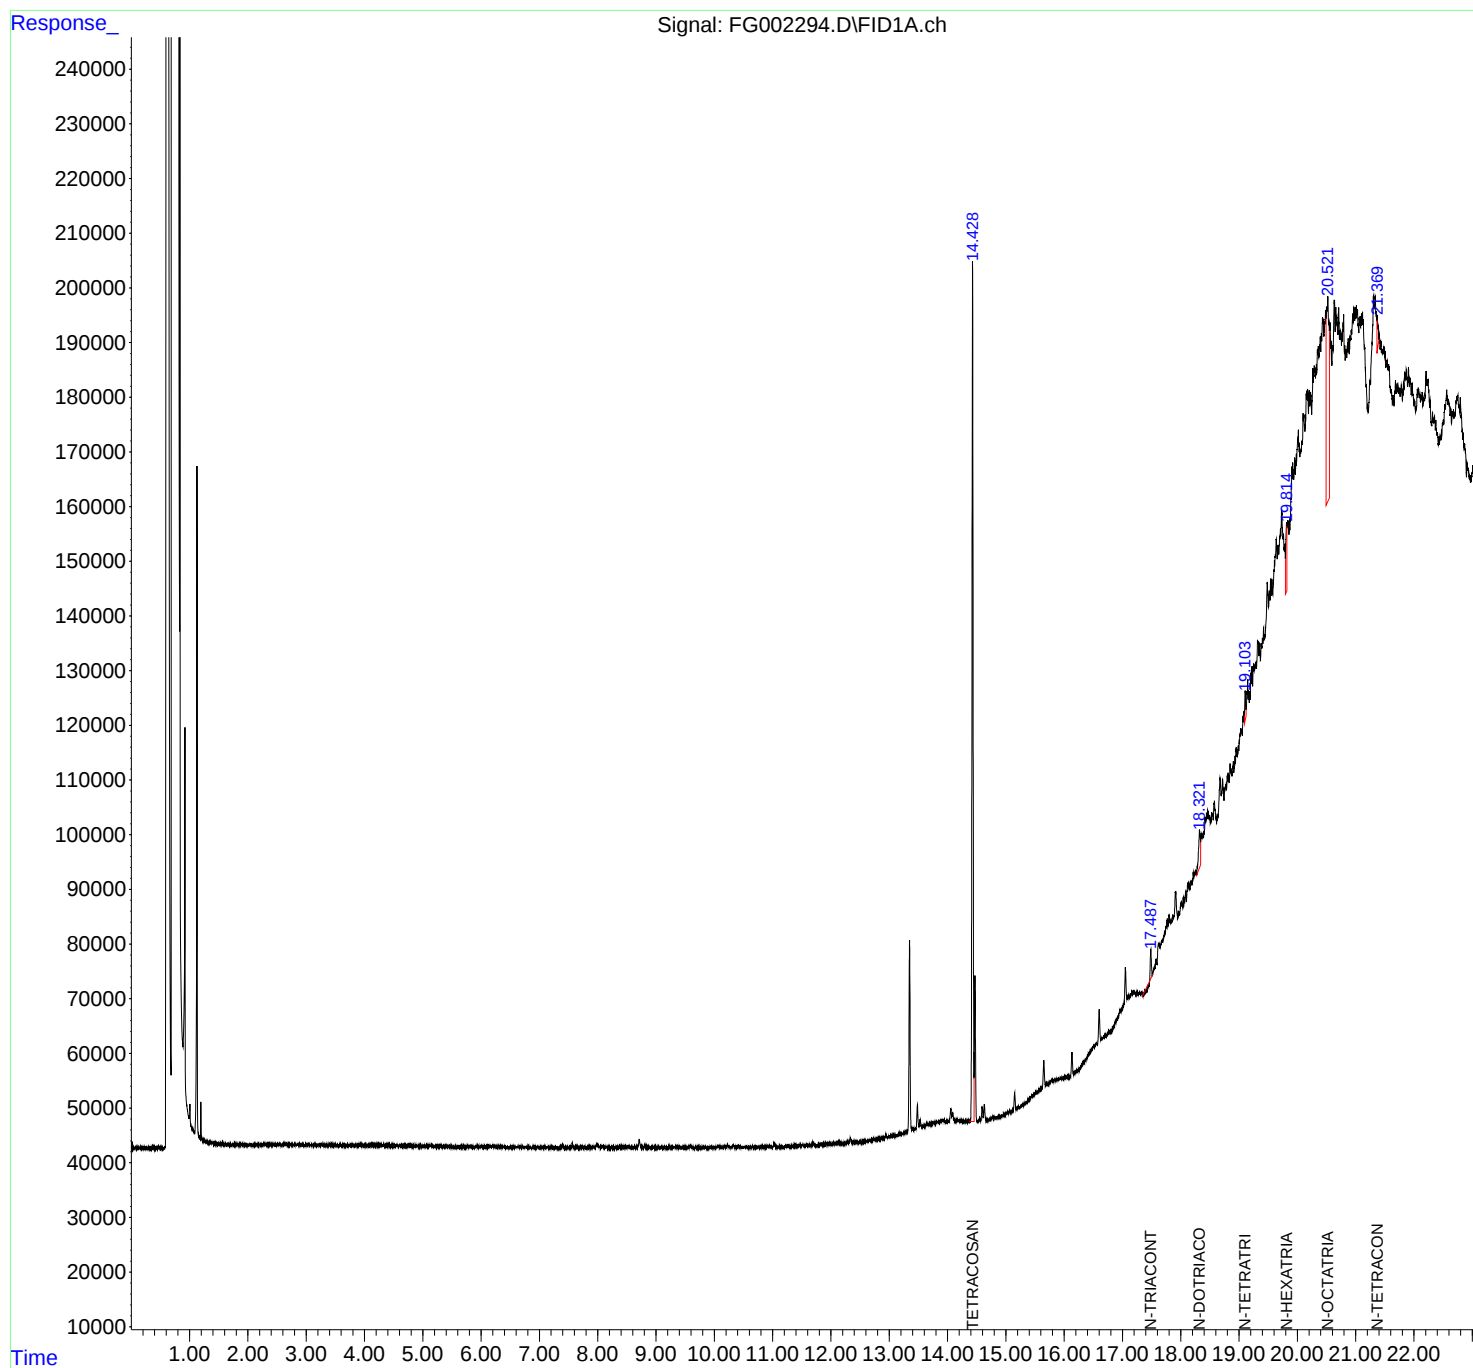


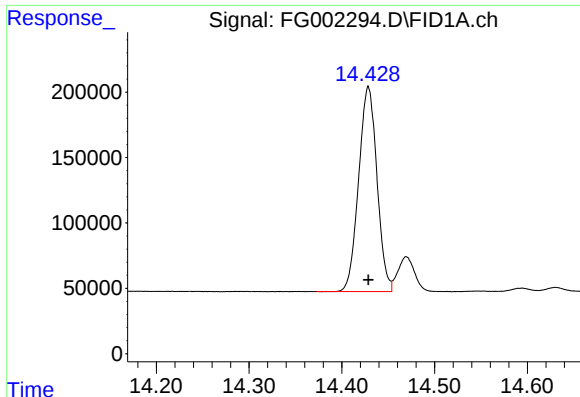

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.429 min
Delta R.T.: 0.000 min
Response: 2150397
Conc: 17.04 ug/ml

Instrument :
FID_G
ClientSampleId :

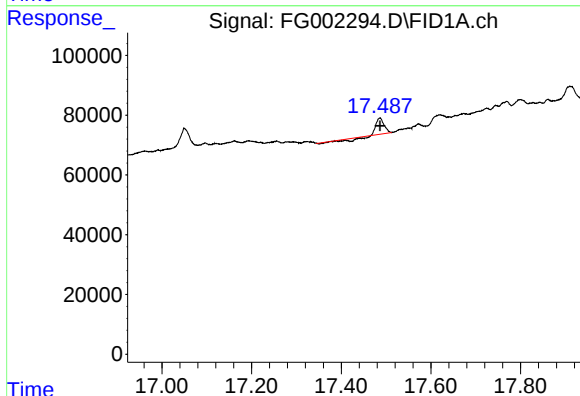


#13 N-TRIACONTANE

R.T.: 17.486 min
Delta R.T.: 0.000 min
Response: 41569
Conc: 0.27 ug/ml

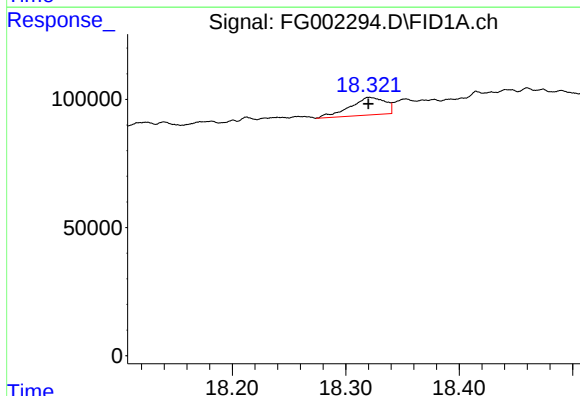


#14 N-DOTRIACONTANE

R.T.: 18.321 min
Delta R.T.: 0.000 min
Response: 147994
Conc: 1.00 ug/ml

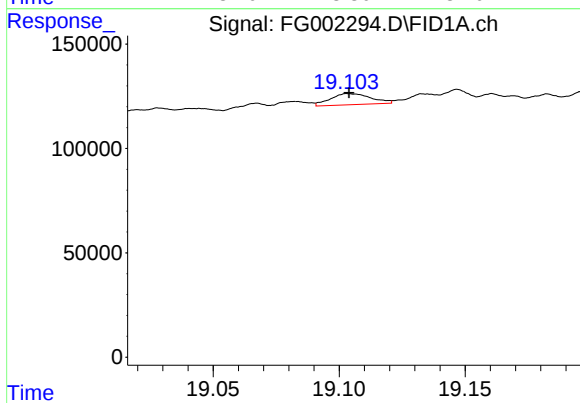

#15 N-TETRATRIACONTANE


R.T.: 19.104 min
Delta R.T.: 0.000 min
Response: 59548
Conc: 0.43 ug/ml

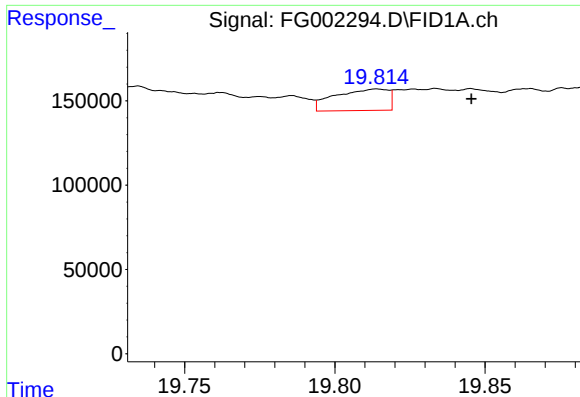

#16 N-HEXATRIACONTANE


R.T.: 19.814 min
Delta R.T.: -0.031 min
Response: 156244
Conc: 1.22 ug/ml

Instrument :
FID_G
ClientSampleId :

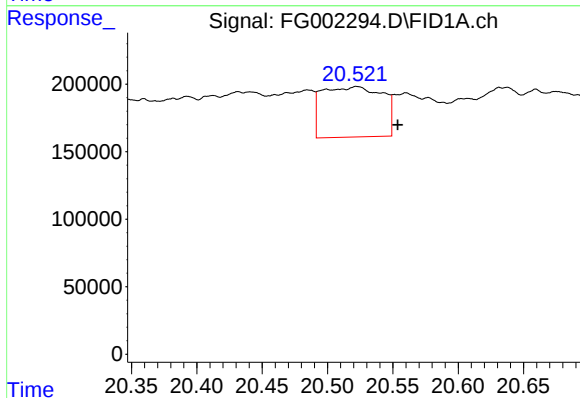

#17 N-OCTATRIACONTANE

R.T.: 20.523 min
Delta R.T.: -0.031 min
Response: 1198727
Conc: 10.66 ug/ml

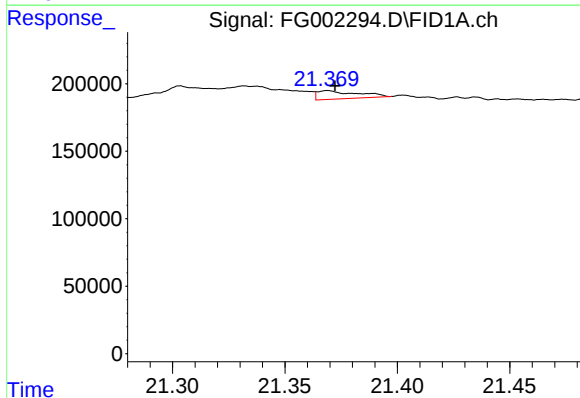

#18 N-TETRACONTANE

R.T.: 21.369 min
Delta R.T.: -0.003 min
Response: 75400
Conc: 0.69 ug/ml