

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG091018\
 Data File : FG002281.D
 Signal(s) : FID1A.ch
 Acq On : 10 Sep 2018 20:38
 Operator : AJ\SJ
 Sample : PB112714BS
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Sep 11 04:17:15 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG083018.M
 Quant Title :
 QLast Update : Thu Aug 30 14:49:31 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.424	1602796	12.704 ug/ml
Target Compounds			
2) N-DECANE	4.185	1918721	15.985 ug/ml
3) N-DODECANE	6.196	2077541	16.508 ug/ml
4) N-TETRADECANE	7.986	2166188	16.501 ug/ml
5) N-HEXADECANE	9.582	2200886	16.170 ug/ml
6) N-OCTADECANE	11.021	2212195	15.749 ug/ml
7) N-EICOSANE	12.329	2184832	15.379 ug/ml
8) N-DOCOSANE	13.525	2158094	15.121 ug/ml
10) N-TETRACOSANE	14.627	2119631	14.827 ug/ml
11) N-HEXACOSANE	15.647	2078999	14.480 ug/ml
12) N-OCTACOSANE	16.597	2059102	14.073 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG091018\
Data File : FG002281.D
Signal(s) : FID1A.ch
Acq On : 10 Sep 2018 20:38
Operator : AJ\SJ
Sample : PB112714BS
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 11 04:17:15 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG083018.M
Quant Title :
QLast Update : Thu Aug 30 14:49:31 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

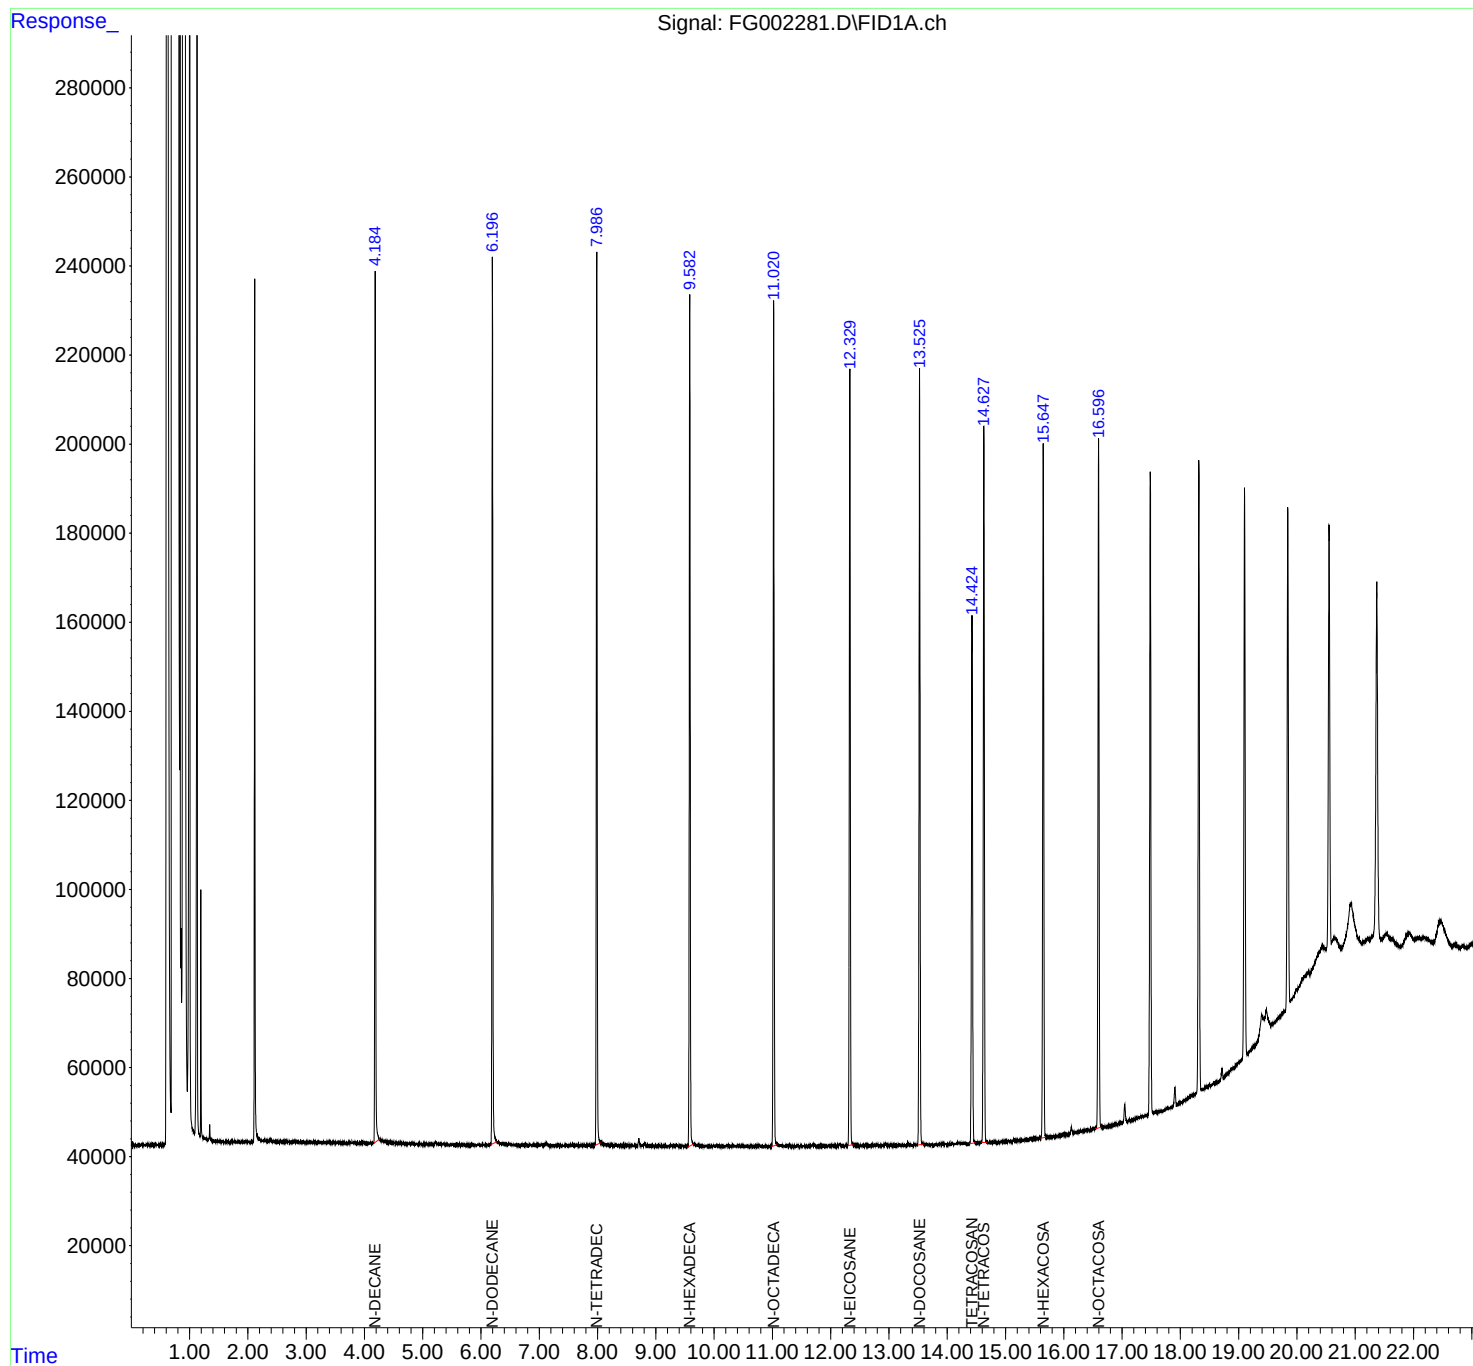


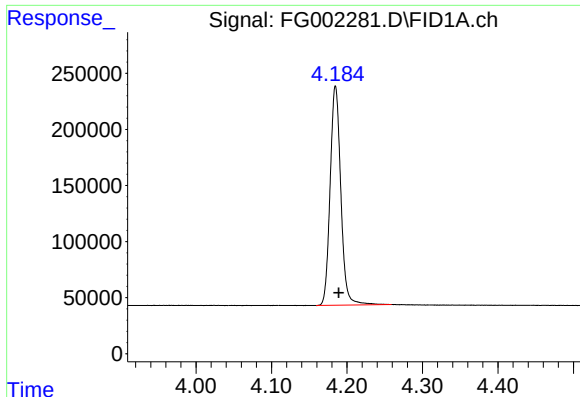

#2 N-DECANE


R.T.: 4.185 min
Delta R.T.: -0.004 min
Response: 1918721
Conc: 15.98 ug/ml

Instrument :
FID_G
ClientSampleId :

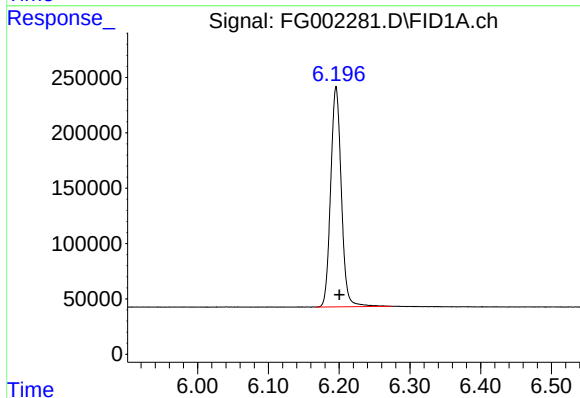


#3 N-DODECANE

R.T.: 6.196 min
Delta R.T.: -0.005 min
Response: 2077541
Conc: 16.51 ug/ml

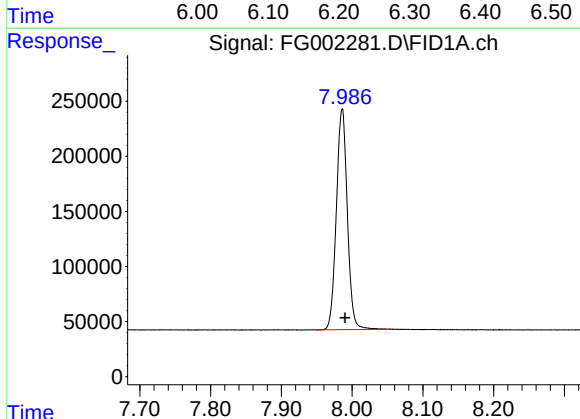


#4 N-TETRADECANE

R.T.: 7.986 min
Delta R.T.: -0.004 min
Response: 2166188
Conc: 16.50 ug/ml

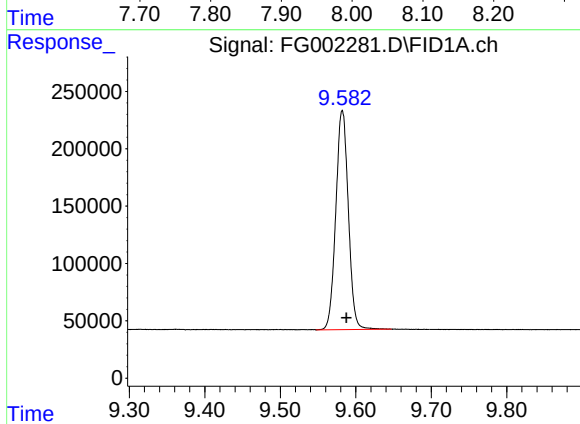

#5 N-HEXADECANE


R.T.: 9.582 min
Delta R.T.: -0.005 min
Response: 2200886
Conc: 16.17 ug/ml

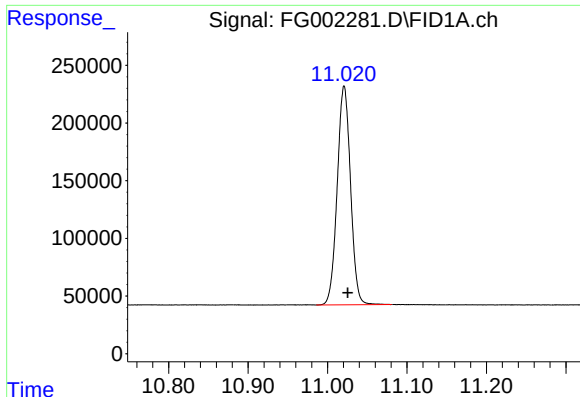

#6 N-OCTADECANE


R.T.: 11.021 min
Delta R.T.: -0.005 min
Response: 2212195
Conc: 15.75 ug/ml

Instrument :
FID_G
ClientSampleId :

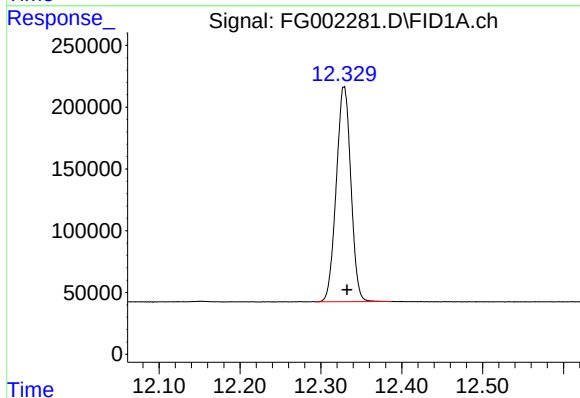


#7 N-EICOSANE

R.T.: 12.329 min
Delta R.T.: -0.004 min
Response: 2184832
Conc: 15.38 ug/ml

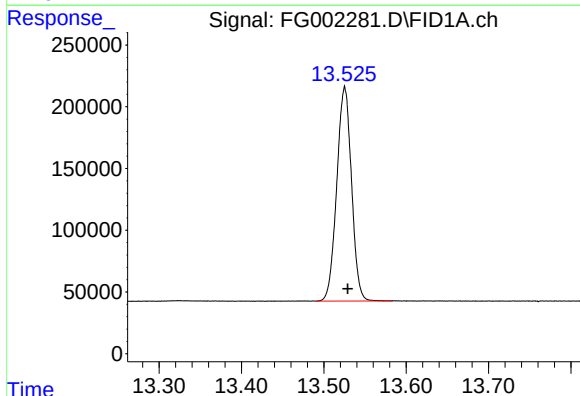


#8 N-DOCOSANE

R.T.: 13.525 min
Delta R.T.: -0.004 min
Response: 2158094
Conc: 15.12 ug/ml

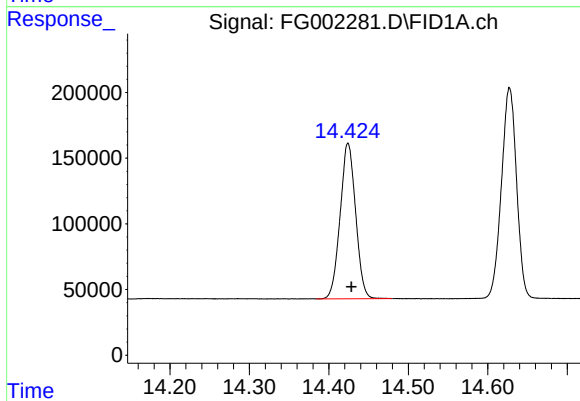

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.424 min
Delta R.T.: -0.004 min
Response: 1602796
Conc: 12.70 ug/ml

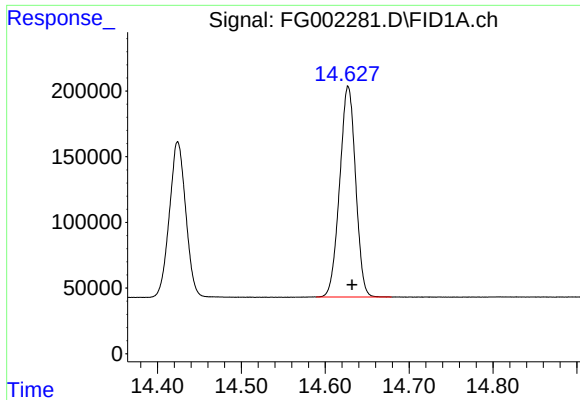

#10 N-TETRACOSANE


R.T.: 14.627 min
Delta R.T.: -0.004 min
Response: 2119631
Conc: 14.83 ug/ml

Instrument :
FID_G
ClientSampleId :

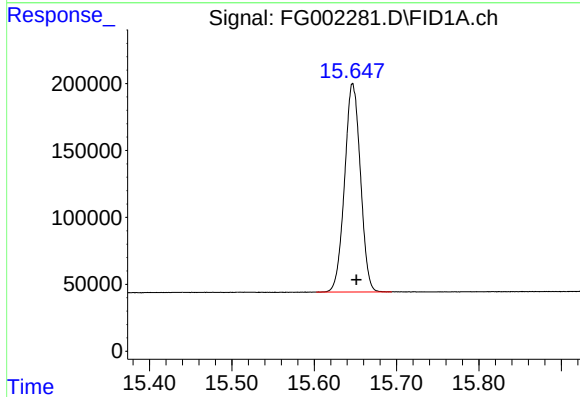

#11 N-HEXACOSANE

R.T.: 15.647 min
Delta R.T.: -0.004 min
Response: 2078999
Conc: 14.48 ug/ml

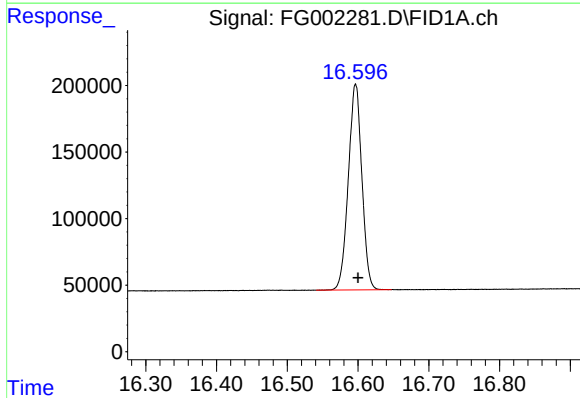

#12 N-OCTACOSANE

R.T.: 16.597 min
Delta R.T.: -0.003 min
Response: 2059102
Conc: 14.07 ug/ml