

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG091223\
Data File : FG012889.D
Signal(s) : FID1A.ch
Acq On : 12 Sep 2023 12:16
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 13 03:07:13 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG090123.M
Quant Title :
QLast Update : Thu Aug 31 16:39:19 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.080	1728872	15.467 ug/ml
Target Compounds			
10) N-TETRACOSANE	15.273	47478	0.383 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG091223\
Data File : FG012889.D
Signal(s) : FID1A.ch
Acq On : 12 Sep 2023 12:16
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 13 03:07:13 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG090123.M
Quant Title :
QLast Update : Thu Aug 31 16:39:19 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

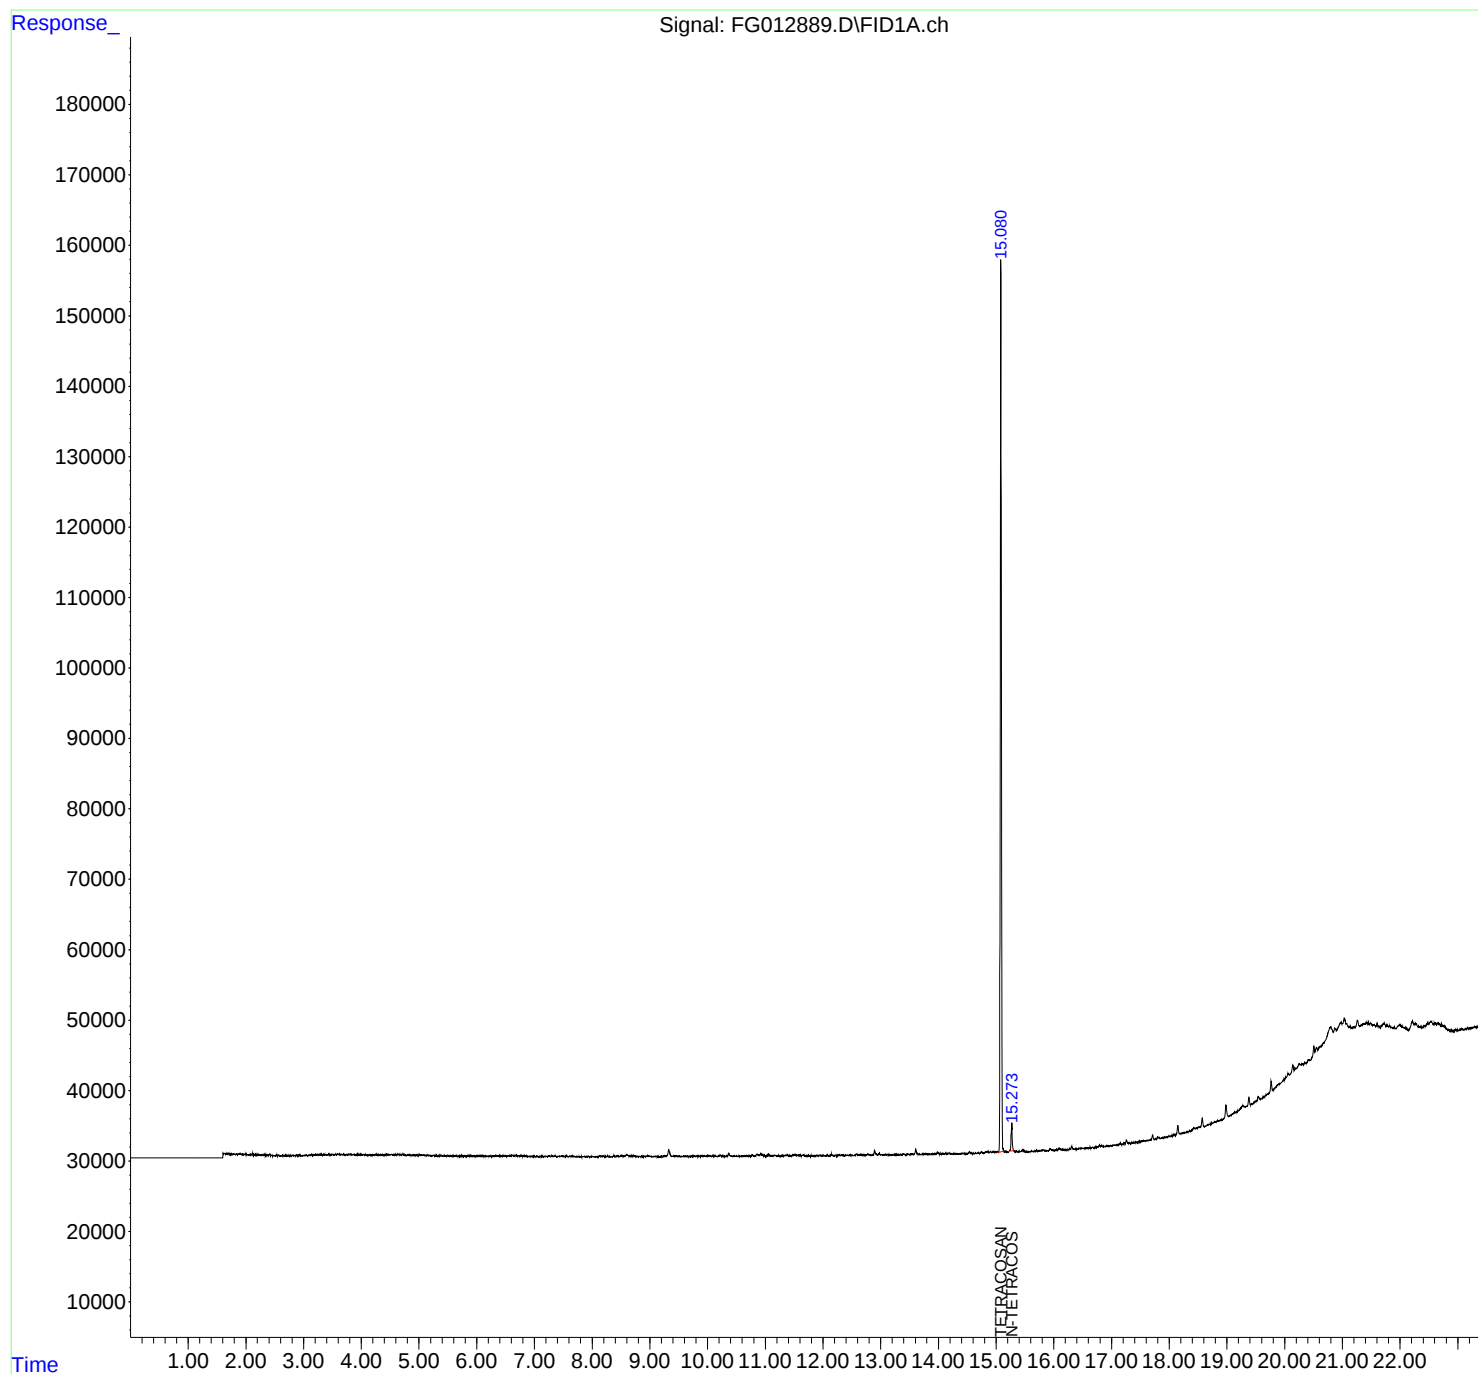


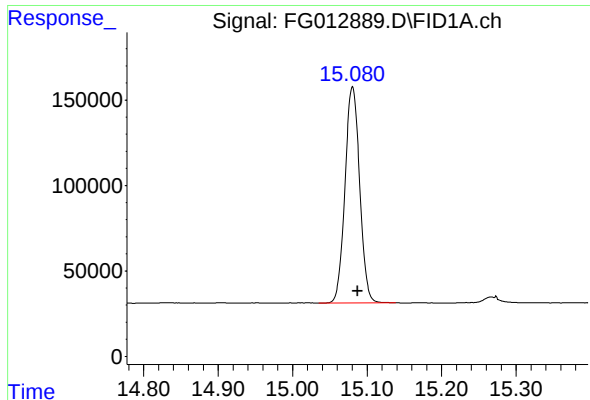

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.080 min
Delta R.T.: -0.007 min
Response: 1728872
Conc: 15.47 ug/ml

Instrument :
FID_G
ClientSampleId :

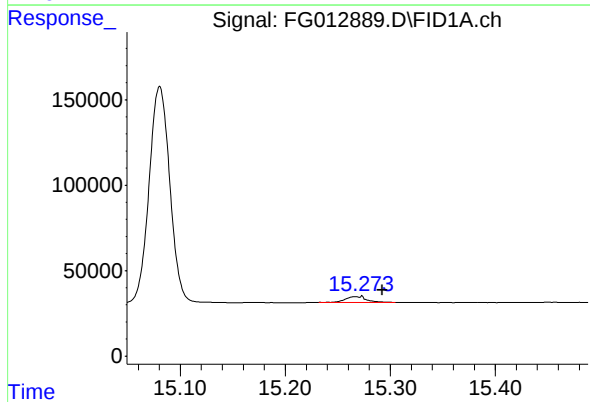

#10 N-TETRACOSANE

R.T.: 15.273 min
Delta R.T.: -0.020 min
Response: 47478
Conc: 0.38 ug/ml