

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG091223\
Data File : FG012901.D
Signal(s) : FID1A.ch
Acq On : 12 Sep 2023 18:45
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 13 03:08:20 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG090123.M
Quant Title :
QLast Update : Thu Aug 31 16:39:19 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.081	1762023	15.764 ug/ml
Target Compounds			
10) N-TETRACOSANE	15.266	57663	0.465 ug/ml
14) N-DOTRIACONTANE	18.979	45367	0.435 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.

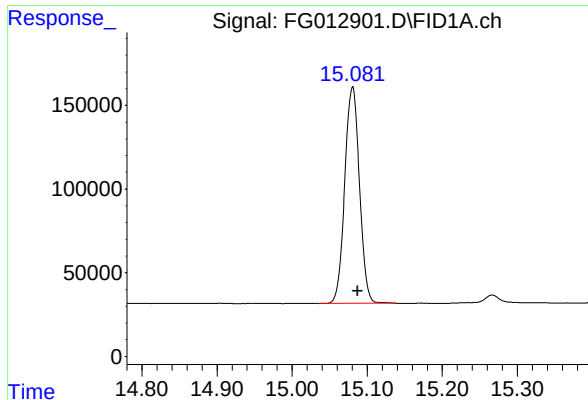

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 15.081 min
Delta R.T.: -0.007 min
Response: 1762023
Conc: 15.76 ug/ml

Instrument :
FID_G
ClientSampleId :

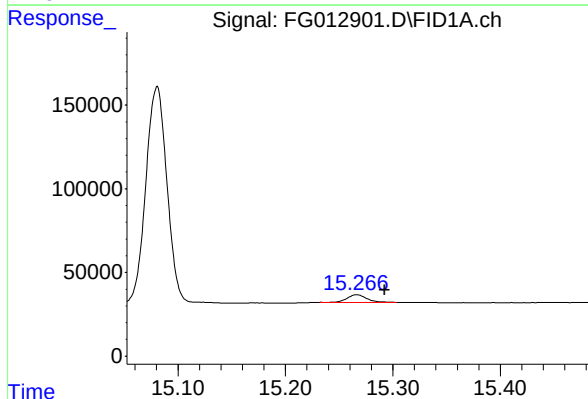

#10 N-TETRACOSANE

R.T.: 15.266 min
Delta R.T.: -0.026 min
Response: 57663
Conc: 0.47 ug/ml

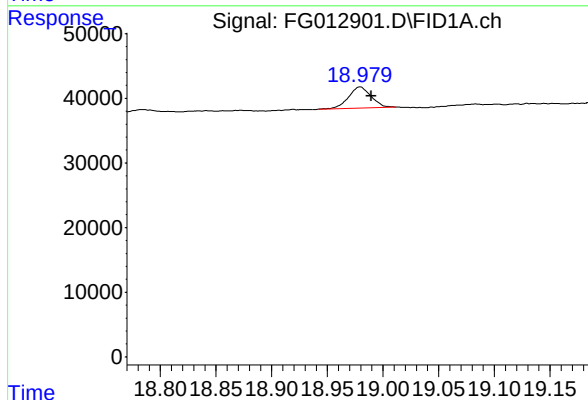

#14 N-DOTRIACONTANE

R.T.: 18.979 min
Delta R.T.: -0.010 min
Response: 45367
Conc: 0.44 ug/ml